

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021565.D
 Acq On : 29 Mar 2016 23:34
 Operator : UM/SJ
 Sample : H1910-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC1

Quant Time: Mar 30 01:37:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 01:34:35 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	11072	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	46095	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	27404	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	70933	20.00	ng/ul	0.00
78) Chrysene-d12	21.66	240	86909	20.00	ng/ul	0.00
86) Perylene-d12	24.87	264	84252	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.37	99	27537	26.31	ng/ul	0.04
7) Bis-(2-Chloroethyl)ether-d	7.37	67	18108	29.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	18534	23.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.84	113	10904	12.16	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	11841	34.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	13046	33.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.56	165	20337	28.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.02	131	598	0.65	ng/ul	0.01
44) Dimethylphthalate-d6	14.07	166	76987	33.74	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	92157	32.77	ng/ul	0.00
52) 4-Nitrophenol-d4	15.11	143	966	2.65	ng/ul	0.02
58) Fluorene-d10	15.66	176	69679	33.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	12808	27.33	ng/ul	0.00
71) Anthracene-d10	17.51	188	117067	33.68	ng/ul	0.00
79) Pyrene-d10	19.79	212	142952	35.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	150690	38.75	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
17) Hexachloroethane	9.23	117	443	1.29	ng/ul#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021565.D
Acq On : 29 Mar 2016 23:34
Operator : UM/SJ
Sample : H1910-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC1

Quant Time: Mar 30 01:37:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 01:34:35 2016
Response via : Initial Calibration

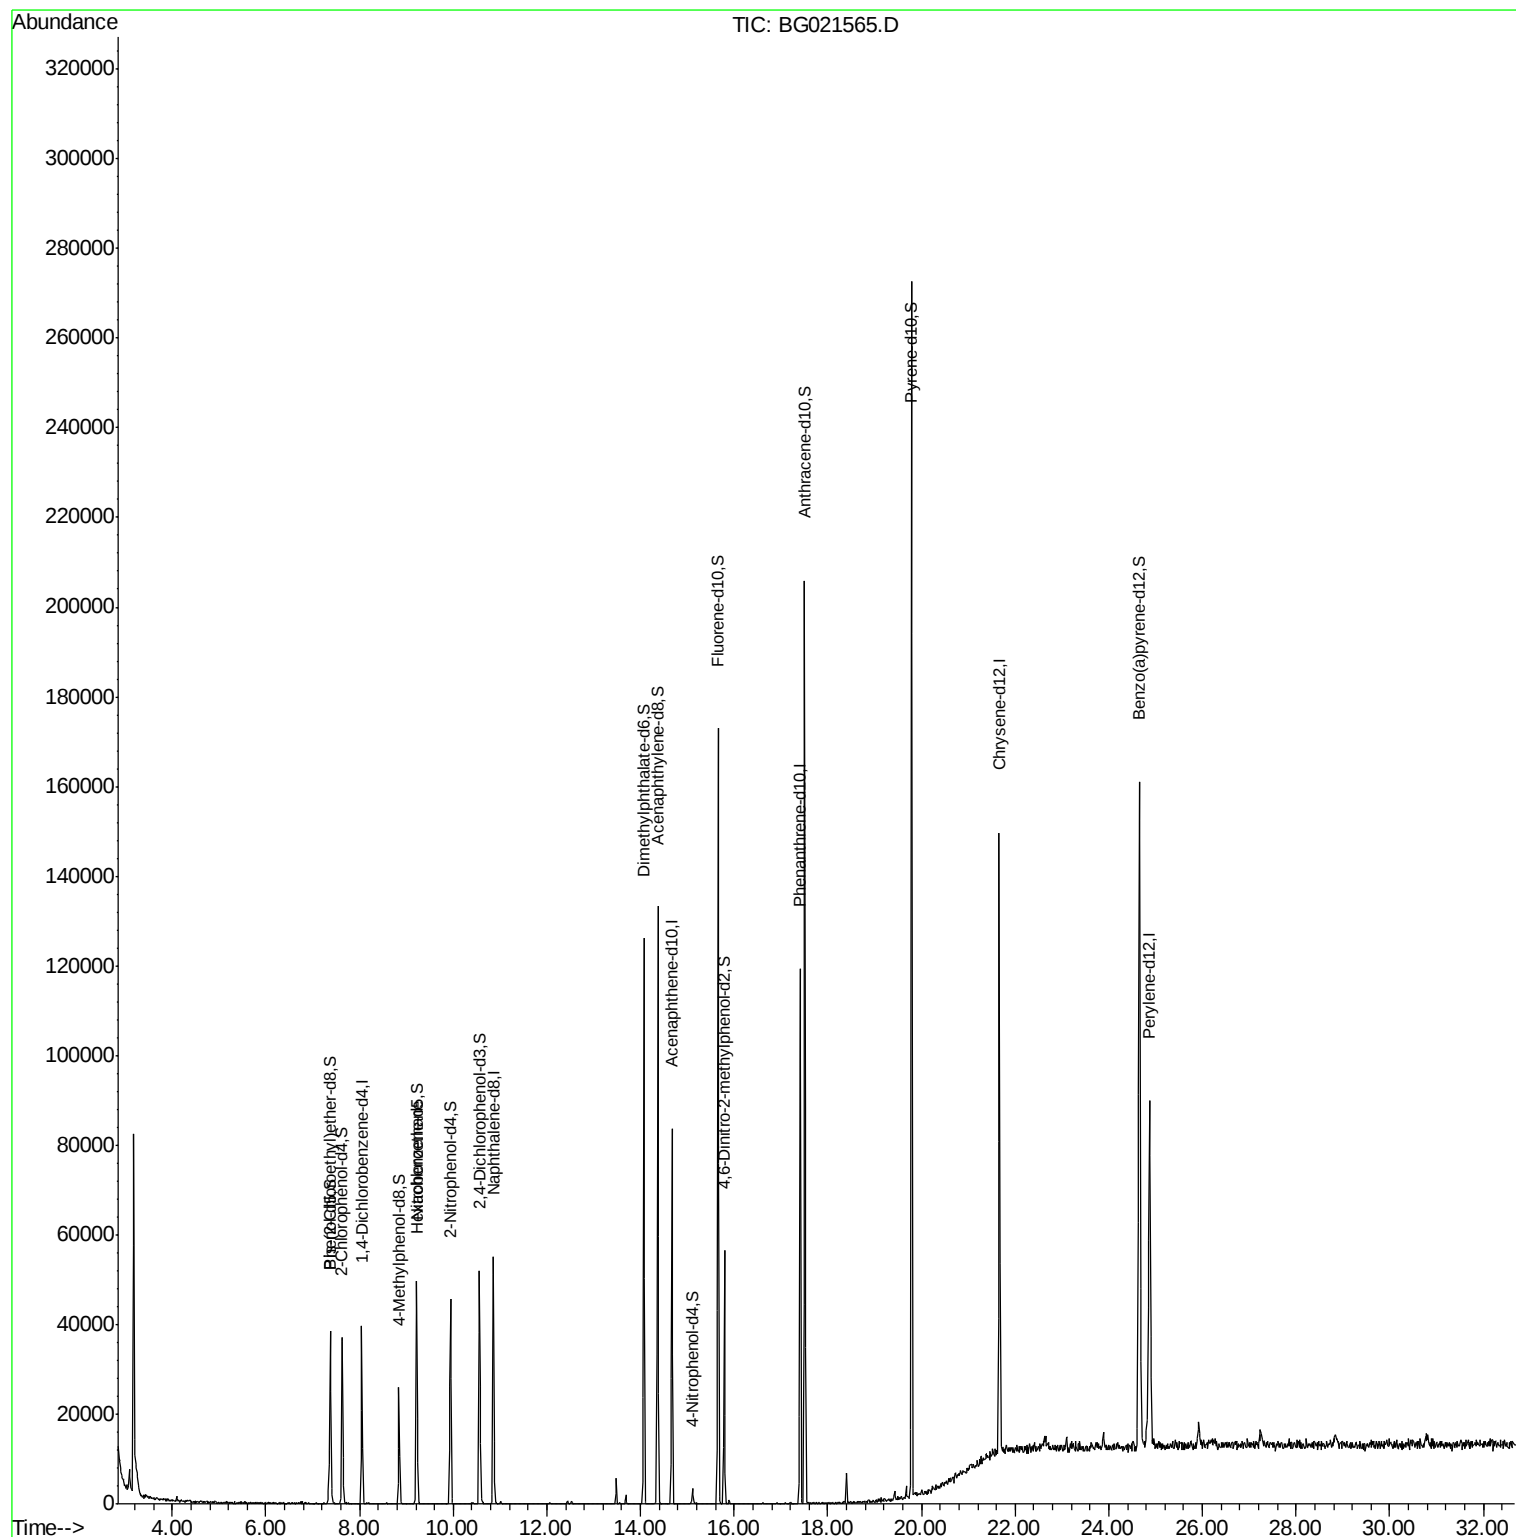

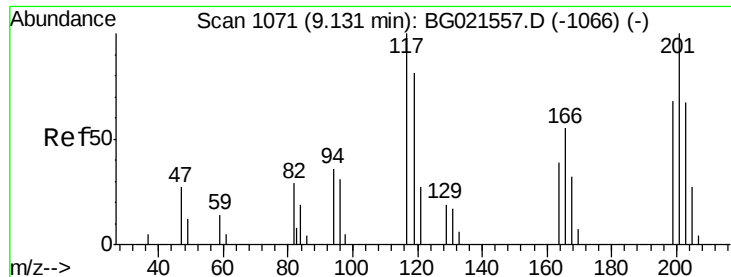

#17
 Hexachloroethane
 Concen: 1.29 ng/ul
 RT: 9.23 min Scan# 1088
 Delta R.T. 0.10 min
 Lab File: BG021565.D
 Acq: 29 Mar 2016 23:34

Instrument :
 BNA_G
 ClientSampleId :
 C0AC1

Tgt Ion:117 Resp: 443
 Ion Ratio Lower Upper
 117 100
 201 0.0 83.5 125.3#
 199 0.0 49.3 73.9#

