

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021554.D
 Acq On : 29 Mar 2016 15:12
 Operator : UM/SJ
 Sample : H1935-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Manual Integrations
 APPROVED

Sohil
 3/30/2016 7:11:06 PM

Quant Time: Mar 30 01:24:02 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 30 01:11:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	10798	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	48679	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	33523	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	90494	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	103644	20.00	ng/ul	0.00
86) Perylene-d12	24.88	264	101800	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.36	99	1435m	1.41	ng/ul	0.03
7) Bis-(2-Chloroethyl)ether-d	7.38	67	4874	8.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.63	132	5282	6.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.85	113	3404	3.89	ng/ul	0.01
19) Nitrobenzene-d5	9.23	128	3373	9.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.95	143	3667	8.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	6093	8.16	ng/ul	0.01
29) 4-Chloroaniline-d4	11.02	131	870	0.89	ng/ul	0.01
44) Dimethylphthalate-d6	14.07	166	26733	9.58	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	32212	9.36	ng/ul	0.00
52) 4-Nitrophenol-d4	15.12	143	404m	0.91	ng/ul	0.04
58) Fluorene-d10	15.66	176	25006	9.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.79	200	4632	7.75	ng/ul	0.00
71) Anthracene-d10	17.51	188	42926	9.68	ng/ul	0.00
79) Pyrene-d10	19.79	212	53780	11.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.65	264	48224	10.26	ng/ul	0.00

Target Compounds

					Qvalue
37) 1,2,4,5-Tetrachlorobenzene	12.87	216	3886	3.31 ng/ul#	94
45) Dimethylphthalate	14.12	163	4204	1.45 ng/ul	98
73) 1,2,3,4-Tetrachlorobenzene	13.48	216	4401	3.47 ng/uL	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021554.D
Acq On : 29 Mar 2016 15:12
Operator : UM/SJ
Sample : H1935-04
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
C0AA0

Manual Integrations
APPROVED

Sohil
3/30/2016 7:11:06 PM

Quant Time: Mar 30 01:24:02 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 30 01:11:49 2016
Response via : Initial Calibration

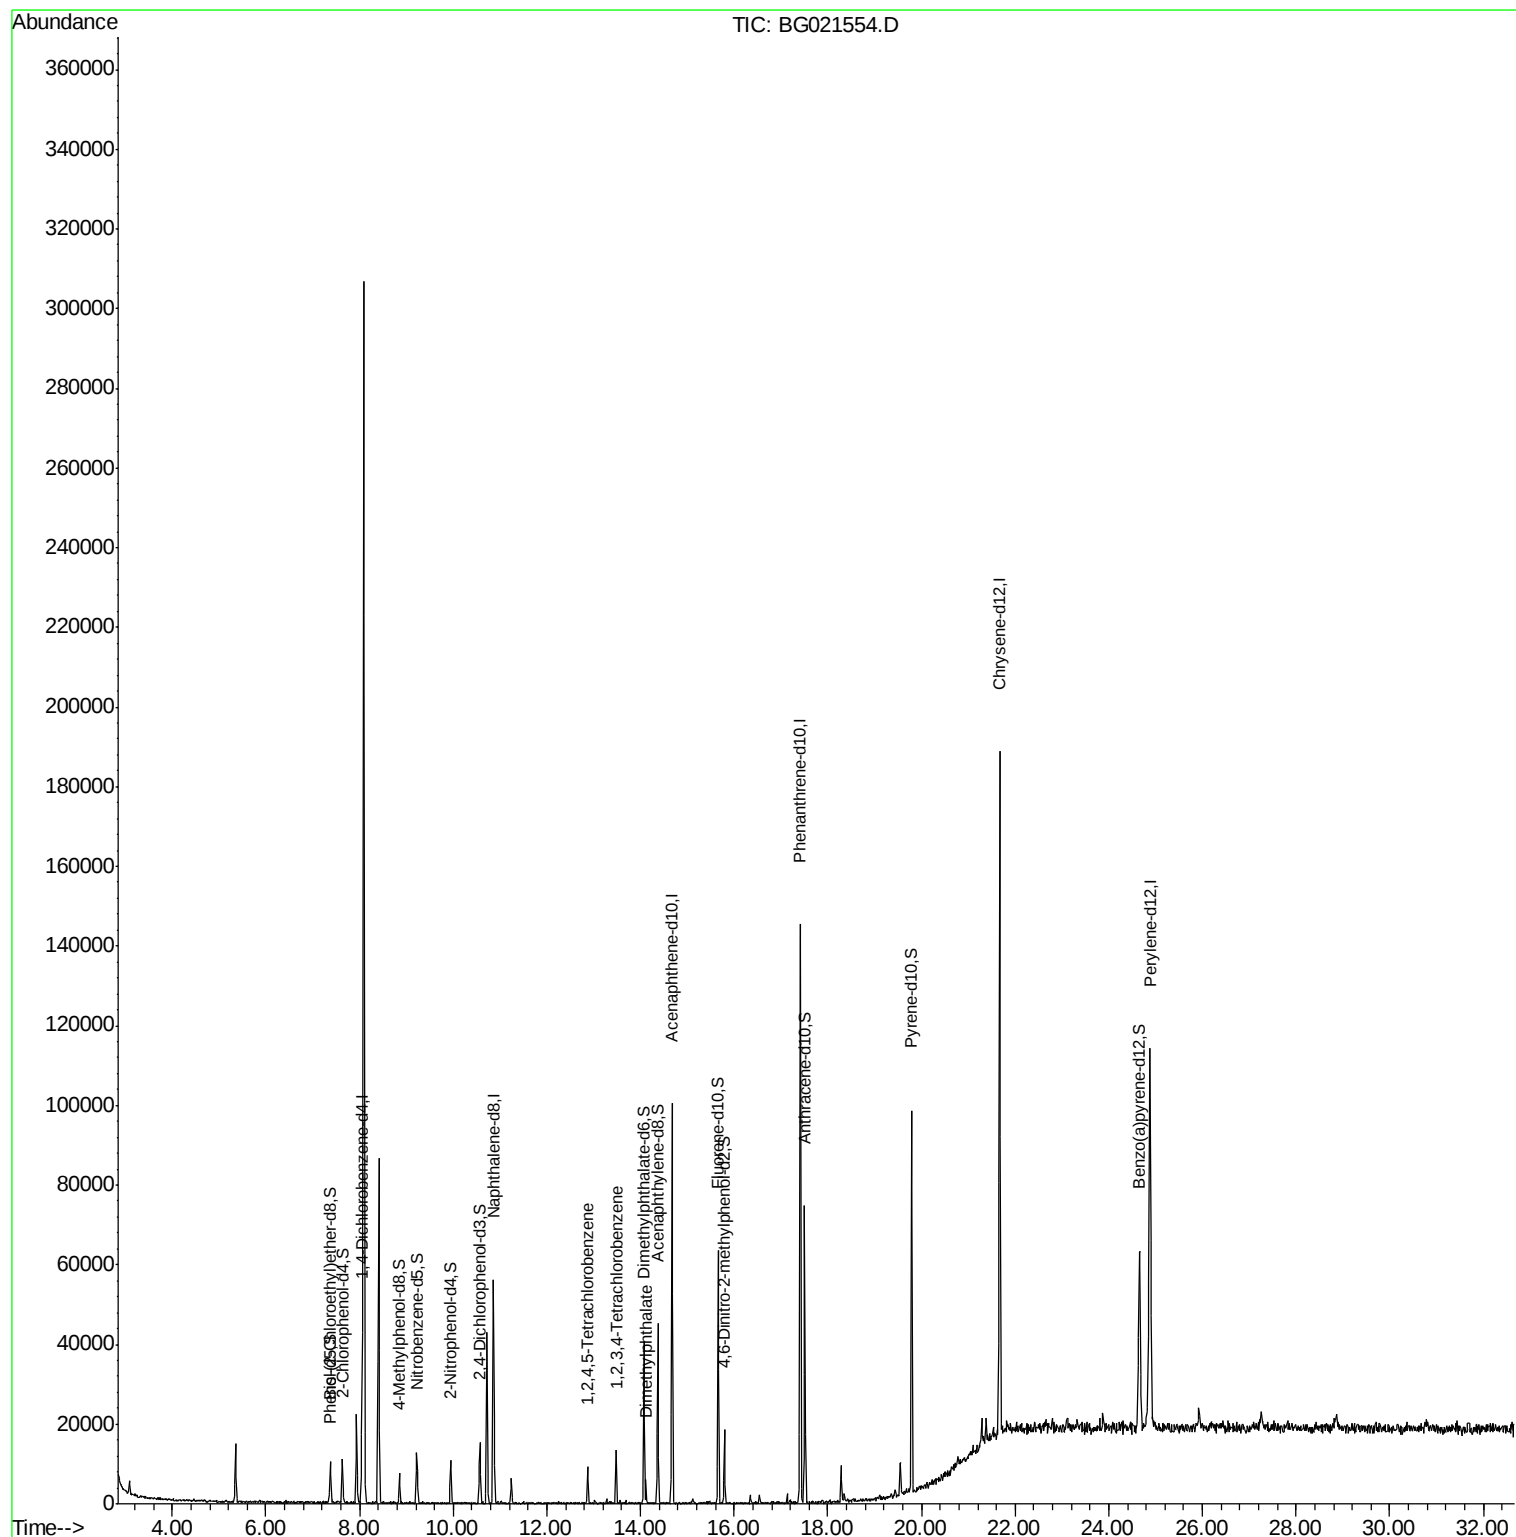

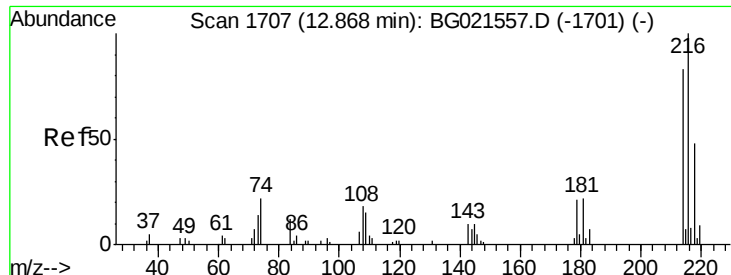





#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 3.31 ng/ul
 RT: 12.87 min Scan# 1708
 Delta R.T. 0.00 min
 Lab File: BG021554.D
 Acq: 29 Mar 2016 15:12

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Tgt Ion	Ratio	Lower	Upper
216	100		
214	71.6	57.8	86.8
179	15.5	19.5	29.3
108	16.5	15.8	23.8




Manual Integrations
 APPROVED


Sohil
 3/30/2016 7:11:06 PM

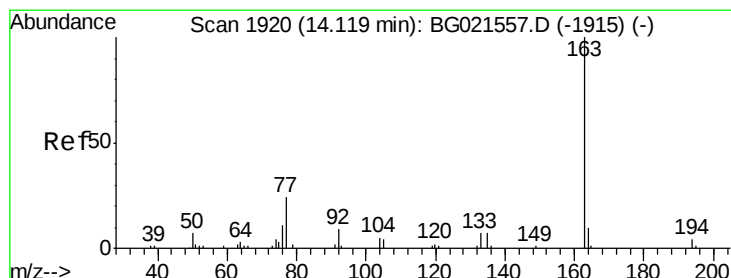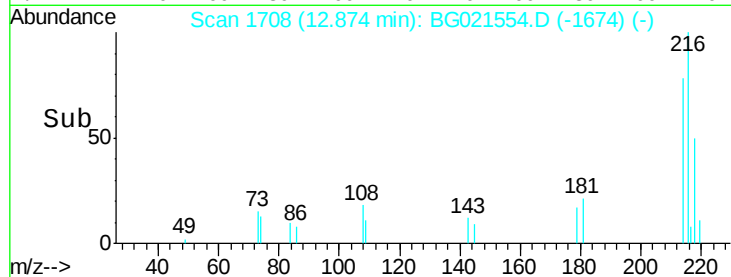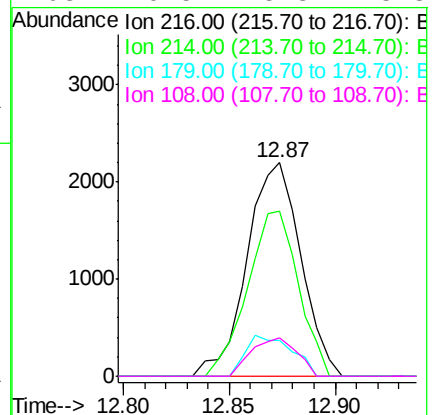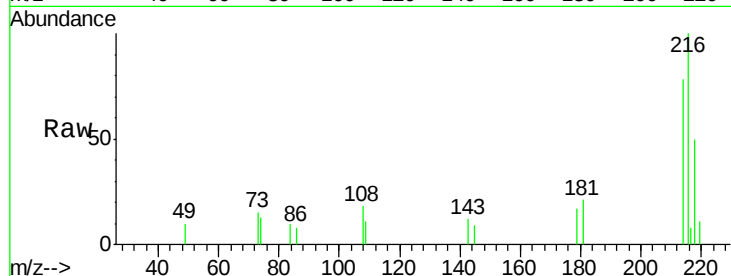

#45
 Dimethylphthalate
 Concen: 1.45 ng/ul
 RT: 14.12 min Scan# 1920
 Delta R.T. 0.00 min
 Lab File: BG021554.D
 Acq: 29 Mar 2016 15:12

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.3	3.9	5.9
164	9.9	8.7	13.1

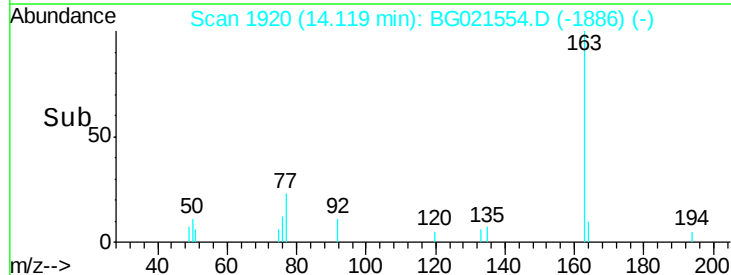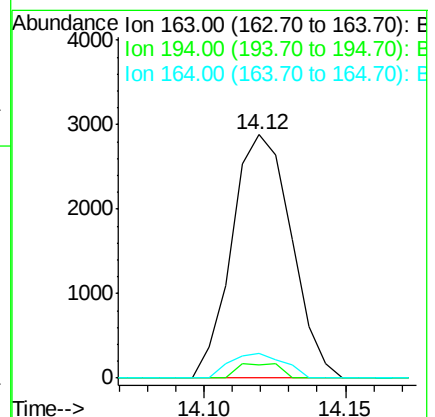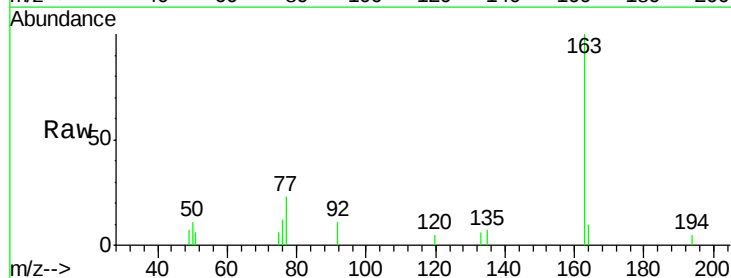

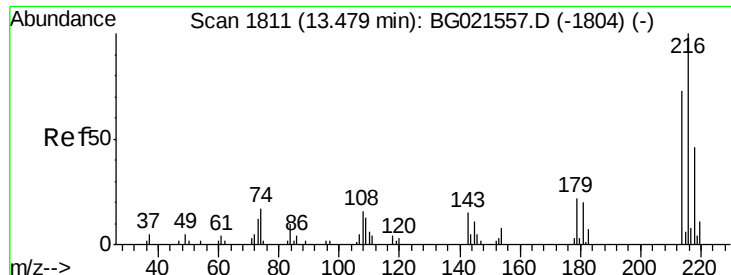


#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 3.47 ng/uL
 RT: 13.48 min Scan# 1811
 Delta R.T. 0.00 min
 Lab File: BG021554.D
 Acq: 29 Mar 2016 15:12

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Tgt Ion	Ratio	Lower	Upper
216	100		
214	74.9	69.2	103.8
218	49.9	41.4	62.0

Manual Integrations
 APPROVED

Sohil
 3/30/2016 7:11:06 PM

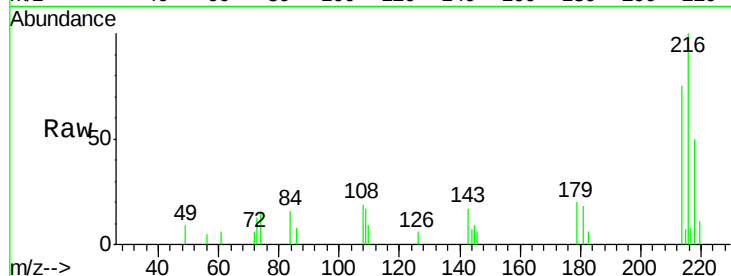

Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 218.00 (217.70 to 218.70): E

