

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021554.D
 Acq On : 29 Mar 2016 15:12
 Operator : UM/SJ
 Sample : H1935-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.085	38	42	48	rVB3	3369	5125	0.96%	0.189%
2	3.209	61	63	68	rVB2	737	806	0.15%	0.030%
3	3.749	151	155	156	rVB2	553	586	0.11%	0.022%
4	4.131	218	220	222	rBV	580	599	0.11%	0.022%
5	5.353	423	428	435	rVB	14687	23786	4.48%	0.877%
6	5.576	461	466	470	rBV2	480	851	0.16%	0.031%
7	5.712	484	489	492	rBV3	502	1001	0.19%	0.037%
8	6.387	602	604	607	rBV	526	680	0.13%	0.025%
9	6.434	607	612	613	rVB	696	627	0.12%	0.023%
10	6.810	674	676	679	rBV	488	643	0.12%	0.024%
11	7.028	712	713	717	rBV2	631	760	0.14%	0.028%
12	7.380	764	773	779	rVB2	10204	19395	3.65%	0.715%
13	7.633	811	816	823	rVB	10900	16896	3.18%	0.623%
14	7.938	863	868	875	rBV	22370	34918	6.57%	1.288%
15	8.091	888	894	902	rVB	306426	531200	100.00%	19.588%
16	8.408	941	948	956	rBV	86295	147111	27.69%	5.425%
17	8.849	1019	1023	1029	rVV3	7804	12675	2.39%	0.467%
18	9.225	1080	1087	1095	rBV2	13006	23648	4.45%	0.872%
19	9.349	1103	1108	1110	rVB2	584	653	0.12%	0.024%
20	9.554	1140	1143	1146	rBV	441	624	0.12%	0.023%
21	9.772	1175	1180	1181	rBV	411	589	0.11%	0.022%
22	9.942	1204	1209	1218	rVB	10966	18679	3.52%	0.689%
23	10.571	1310	1316	1323	rVV	15581	26184	4.93%	0.966%
24	10.717	1335	1341	1348	rBV	42951	74152	13.96%	2.734%
25	10.859	1357	1365	1372	rBV	55954	99495	18.73%	3.669%
26	10.953	1377	1381	1384	rVV	733	903	0.17%	0.033%
27	11.011	1388	1391	1392	rBV	515	656	0.12%	0.024%
28	11.023	1392	1393	1398	rVB	765	784	0.15%	0.029%
29	11.246	1422	1431	1437	rBV2	6440	11007	2.07%	0.406%
30	12.868	1700	1707	1713	rBB2	9176	14871	2.80%	0.548%
31	13.273	1772	1776	1778	rVB3	1072	780	0.15%	0.029%
32	13.479	1805	1811	1816	rBB	13481	19890	3.74%	0.733%
33	13.690	1844	1847	1850	rBV2	1015	1247	0.23%	0.046%
34	14.072	1906	1912	1917	rBV	40936	57767	10.87%	2.130%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021554.D
 Acq On : 29 Mar 2016 15:12
 Operator : UM/SJ
 Sample : H1935-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	14.119	1917	1920	1925	rVB2	5925	7762	1.46%	0.286%
36	14.366	1955	1962	1968	rBV	45184	65805	12.39%	2.427%
37	14.672	2008	2014	2023	rBB2	100464	156999	29.56%	5.789%
38	14.989	2065	2068	2073	rBB	394	626	0.12%	0.023%
39	15.118	2087	2090	2095	rBV2	1185	1473	0.28%	0.054%
40	15.477	2147	2151	2152	rVV	558	635	0.12%	0.023%
41	15.659	2176	2182	2189	rBB	63548	90278	17.00%	3.329%
42	15.706	2189	2190	2196	rBV	325	602	0.11%	0.022%
43	15.788	2200	2204	2210	rVV2	18594	26057	4.91%	0.961%
44	16.129	2259	2262	2266	rBB2	408	651	0.12%	0.024%
45	16.346	2294	2299	2307	rBB	2376	3370	0.63%	0.124%
46	16.534	2328	2331	2339	rVB	2001	2202	0.41%	0.081%
47	16.675	2350	2355	2356	rVB	432	583	0.11%	0.021%
48	16.804	2373	2377	2378	rBV	687	711	0.13%	0.026%
49	16.916	2393	2396	2401	rBB	552	763	0.14%	0.028%
50	17.010	2411	2412	2418	rVB	494	676	0.13%	0.025%
51	17.134	2430	2433	2436	rVB2	2652	2667	0.50%	0.098%
52	17.192	2440	2443	2444	rVV	677	691	0.13%	0.025%
53	17.204	2444	2445	2448	rVB2	915	741	0.14%	0.027%
54	17.410	2474	2480	2488	rBV	145145	219708	41.36%	8.102%
55	17.510	2491	2497	2504	rVB2	74381	107738	20.28%	3.973%
56	17.668	2523	2524	2527	rBV	755	733	0.14%	0.027%
57	17.874	2556	2559	2562	rVB	847	881	0.17%	0.032%
58	18.044	2584	2588	2590	rVV2	663	763	0.14%	0.028%
59	18.215	2615	2617	2621	rVV	563	658	0.12%	0.024%
60	18.285	2625	2629	2634	rBV	9280	12357	2.33%	0.456%
61	18.356	2637	2641	2646	rVV2	2230	3490	0.66%	0.129%
62	18.414	2648	2651	2653	rVV2	738	915	0.17%	0.034%
63	18.456	2656	2658	2661	rBV3	565	679	0.13%	0.025%
64	18.749	2705	2708	2711	rVB2	652	652	0.12%	0.024%
65	18.879	2727	2730	2731	rVB	782	630	0.12%	0.023%
66	18.920	2735	2737	2739	rBV2	803	743	0.14%	0.027%
67	19.014	2749	2753	2754	rVB2	696	706	0.13%	0.026%
68	19.043	2754	2758	2764	rBV4	858	1835	0.35%	0.068%
69	19.108	2767	2769	2772	rVB2	1137	718	0.14%	0.026%
70	19.208	2785	2786	2790	rVB2	668	736	0.14%	0.027%
71	19.249	2790	2793	2794	rBV3	668	701	0.13%	0.026%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021554.D
Acq On : 29 Mar 2016 15:12
Operator : UM/SJ
Sample : H1935-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Title : SVOA CALIBRATION

72	19.354	2808	2811	2812	rBV3	1143	922	0.17%	0.034%
73	19.407	2817	2820	2822	rBV	943	1088	0.20%	0.040%
74	19.425	2822	2823	2827	rVV4	1778	1217	0.23%	0.045%
75	19.501	2831	2836	2837	rBV4	688	983	0.19%	0.036%
76	19.548	2839	2844	2852	rBV5	8257	13037	2.45%	0.481%
77	19.636	2857	2859	2860	rBV2	759	641	0.12%	0.024%
78	19.683	2863	2867	2869	rVV4	1123	1194	0.22%	0.044%
79	19.725	2872	2874	2877	rBV2	1001	821	0.15%	0.030%
80	19.789	2879	2885	2892	rBV2	95781	137573	25.90%	5.073%
81	19.842	2892	2894	2899	rVB3	1310	1432	0.27%	0.053%
82	19.895	2902	2903	2906	rVB3	1103	750	0.14%	0.028%
83	19.924	2906	2908	2910	rBV3	926	1020	0.19%	0.038%
84	19.960	2910	2914	2917	rBV4	839	1070	0.20%	0.039%
85	19.983	2917	2918	2920	rBV2	975	638	0.12%	0.024%
86	20.054	2928	2930	2931	rBV2	752	686	0.13%	0.025%
87	20.165	2948	2949	2951	rBV2	1201	1054	0.20%	0.039%
88	20.230	2958	2960	2961	rVB2	1406	865	0.16%	0.032%
89	20.248	2961	2963	2966	rBV3	980	1166	0.22%	0.043%
90	20.318	2973	2975	2976	rBV2	1387	973	0.18%	0.036%
91	20.424	2992	2993	2995	rBV2	1314	828	0.16%	0.031%
92	20.465	2998	3000	3003	rBV4	2104	2387	0.45%	0.088%
93	20.782	3050	3054	3058	rBV5	2428	3742	0.70%	0.138%
94	21.205	3124	3126	3128	rBV3	1927	1449	0.27%	0.053%
95	21.287	3136	3140	3144	rBV5	6720	9460	1.78%	0.349%
96	21.381	3153	3156	3161	rVB2	5825	7667	1.44%	0.283%
97	21.669	3199	3205	3212	rBV	170949	278322	52.39%	10.263%
98	23.814	3568	3570	3571	rBV2	3295	1539	0.29%	0.057%
99	24.654	3706	3713	3725	rVB	45064	122083	22.98%	4.502%
100	24.883	3743	3752	3760	rVB2	93205	249693	47.01%	9.208%


Sum of corrected areas: 2711823

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021554.D
Acq On : 29 Mar 2016 15:12
Operator : UM/SJ
Sample : H1935-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

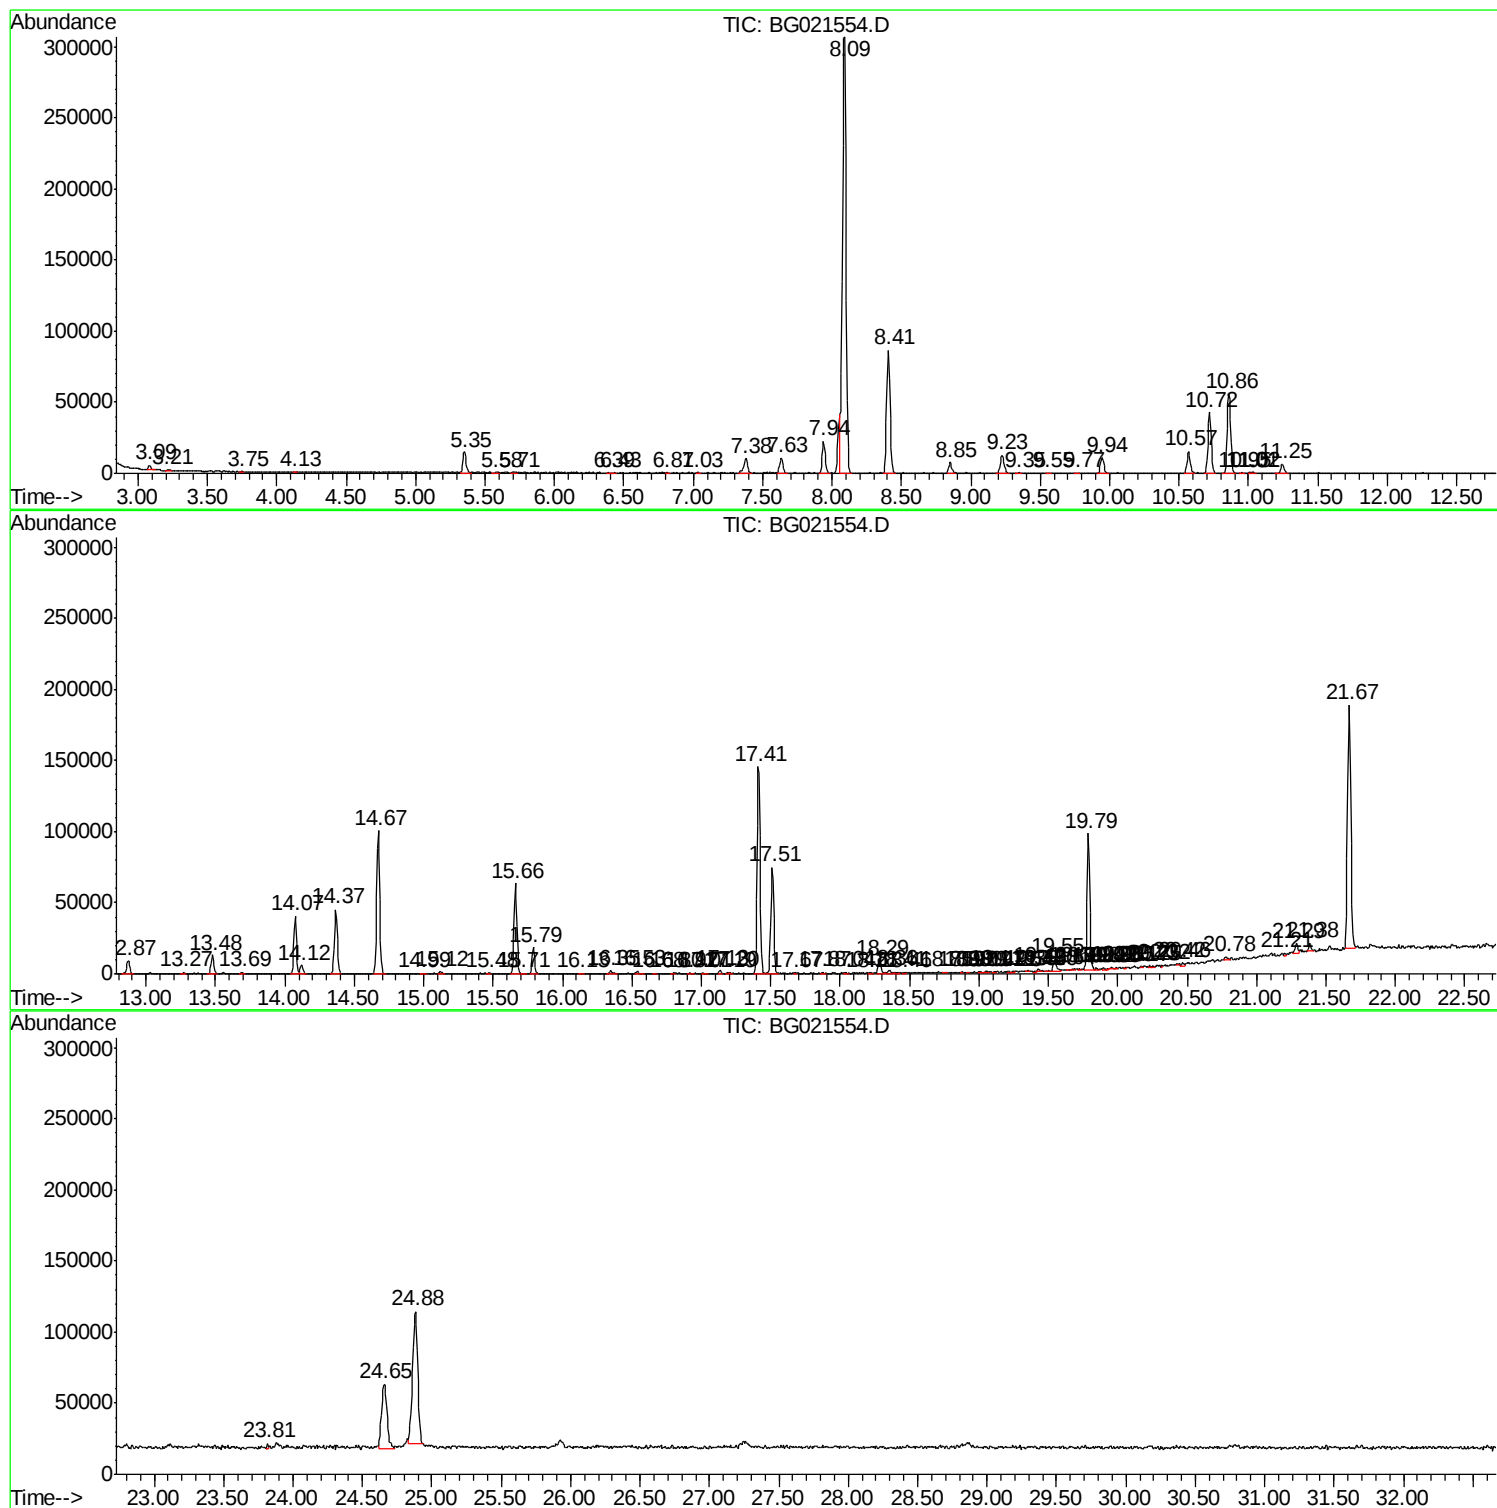

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021554.D
Acq On : 29 Mar 2016 15:12
Operator : UM/SJ
Sample : H1935-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021554.D
Acq On : 29 Mar 2016 15:12
Operator : UM/SJ
Sample : H1935-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc