

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021560.D
 Acq On : 29 Mar 2016 20:16
 Operator : UM/SJ
 Sample : H1935-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	82	83	86	rVB	553	333	0.10%	0.011%
2	3.451	102	104	105	rVB2	663	434	0.13%	0.015%
3	3.651	135	138	139	rVB3	355	333	0.10%	0.011%
4	3.792	161	162	166	rBV	391	417	0.13%	0.014%
5	4.203	229	232	234	rBV	464	507	0.16%	0.017%
6	4.397	262	265	268	rBV2	300	515	0.16%	0.018%
7	4.473	277	278	281	rVB2	497	374	0.11%	0.013%
8	4.497	281	282	285	rBV2	550	328	0.10%	0.011%
9	4.697	314	316	321	rVB2	381	568	0.17%	0.020%
10	4.797	331	333	335	rVB2	449	429	0.13%	0.015%
11	4.826	335	338	340	rVB	322	356	0.11%	0.012%
12	4.850	340	342	345	rBV2	344	377	0.12%	0.013%
13	4.885	345	348	350	rBV	367	429	0.13%	0.015%
14	4.926	352	355	356	rVB	576	361	0.11%	0.012%
15	4.955	356	360	361	rBV	428	466	0.14%	0.016%
16	4.991	365	366	369	rVV	473	350	0.11%	0.012%
17	5.026	369	372	374	rVV	237	351	0.11%	0.012%
18	5.137	390	391	394	rBV	383	351	0.11%	0.012%
19	5.290	416	417	420	rVB2	594	415	0.13%	0.014%
20	5.314	420	421	424	rBV	367	366	0.11%	0.013%
21	5.355	426	428	430	rBV	496	572	0.18%	0.020%
22	5.519	455	456	459	rBV	393	459	0.14%	0.016%
23	5.590	467	468	471	rBV	511	424	0.13%	0.015%
24	5.748	492	495	497	rBV	411	480	0.15%	0.017%
25	5.842	507	511	513	rBB	557	671	0.21%	0.023%
26	5.884	516	518	520	rBB	343	352	0.11%	0.012%
27	5.966	529	532	535	rBV	397	496	0.15%	0.017%
28	6.266	581	583	585	rVB	380	362	0.11%	0.012%
29	7.376	761	772	782	rBB	27632	56363	17.29%	1.944%
30	7.635	810	816	825	rBV2	27381	48597	14.91%	1.676%
31	8.052	881	887	896	rBB	39267	67897	20.82%	2.342%
32	8.845	1017	1022	1033	rBB	19719	33573	10.30%	1.158%
33	9.221	1080	1086	1096	rBB	36985	66633	20.44%	2.299%
34	9.944	1202	1209	1216	rBB	31882	57407	17.61%	1.980%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021560.D
 Acq On : 29 Mar 2016 20:16
 Operator : UM/SJ
 Sample : H1935-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	10.566	1309	1315	1328	rBB	39700	70794	21.71%	2.442%
36	10.860	1358	1365	1373	rBB	56369	100853	30.93%	3.479%
37	11.019	1390	1392	1394	rBV	308	349	0.11%	0.012%
38	12.441	1632	1634	1636	rBB	385	329	0.10%	0.011%
39	13.486	1807	1812	1816	rBB2	7220	8918	2.74%	0.308%
40	13.551	1821	1823	1826	rBB2	371	352	0.11%	0.012%
41	13.692	1842	1847	1851	rBB	3440	5450	1.67%	0.188%
42	14.074	1906	1912	1919	rBB	101990	146904	45.06%	5.068%
43	14.368	1955	1962	1969	rBV	106984	163274	50.08%	5.632%
44	14.667	2007	2013	2020	rBB2	92477	147656	45.29%	5.094%
45	15.108	2085	2088	2095	rBB2	2886	4741	1.45%	0.164%
46	15.660	2176	2182	2189	rBB	147503	224949	68.99%	7.760%
47	15.784	2199	2203	2213	rBB	50561	69792	21.41%	2.408%
48	15.895	2219	2222	2225	rBB	799	855	0.26%	0.029%
49	16.530	2328	2330	2333	rBB	689	605	0.19%	0.021%
50	17.194	2441	2443	2447	rBB	351	499	0.15%	0.017%
51	17.411	2473	2480	2486	rBV2	134206	198336	60.83%	6.842%
52	17.505	2490	2496	2504	rVV	174848	267865	82.16%	9.240%
53	17.905	2562	2564	2567	rBB	402	334	0.10%	0.012%
54	18.351	2637	2640	2645	rBV2	857	1163	0.36%	0.040%
55	18.398	2645	2648	2653	rVB2	1198	1796	0.55%	0.062%
56	18.716	2699	2702	2703	rBV	316	377	0.12%	0.013%
57	18.792	2709	2715	2716	rBV2	314	448	0.14%	0.015%
58	19.168	2777	2779	2782	rBV	535	457	0.14%	0.016%
59	19.197	2782	2784	2787	rVB	529	371	0.11%	0.013%
60	19.221	2787	2788	2792	rVB2	484	520	0.16%	0.018%
61	19.256	2792	2794	2795	rBV	551	384	0.12%	0.013%
62	19.291	2798	2800	2802	rVB2	611	400	0.12%	0.014%
63	19.350	2808	2810	2811	rVV2	433	334	0.10%	0.012%
64	19.432	2819	2824	2827	rBV	1669	2558	0.78%	0.088%
65	19.509	2836	2837	2840	rBV2	578	643	0.20%	0.022%
66	19.679	2863	2866	2870	rVB3	1687	2276	0.70%	0.079%
67	19.720	2870	2873	2874	rBV2	699	675	0.21%	0.023%
68	19.785	2878	2884	2891	rVV	230217	326037	100.00%	11.247%
69	19.838	2891	2893	2894	rVV2	1412	1114	0.34%	0.038%
70	19.879	2898	2900	2901	rVB	811	533	0.16%	0.018%
71	19.897	2901	2903	2904	rBV2	1051	528	0.16%	0.018%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021560.D
 Acq On : 29 Mar 2016 20:16
 Operator : UM/SJ
 Sample : H1935-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	19.955	2909	2913	2915	rBV2	1129	1438	0.44%	0.050%
73	19.973	2915	2916	2920	rBV2	770	757	0.23%	0.026%
74	20.020	2922	2924	2925	rBV	739	632	0.19%	0.022%
75	20.061	2929	2931	2932	rVB	1051	735	0.23%	0.025%
76	20.079	2932	2934	2936	rBV3	1070	888	0.27%	0.031%
77	20.096	2936	2937	2940	rVB2	881	447	0.14%	0.015%
78	20.132	2940	2943	2944	rBV2	879	935	0.29%	0.032%
79	20.161	2947	2948	2949	rBV	804	381	0.12%	0.013%
80	20.173	2949	2950	2952	rBV2	594	461	0.14%	0.016%
81	20.261	2961	2965	2966	rBV	1278	1529	0.47%	0.053%
82	20.402	2988	2989	2990	rBV	997	488	0.15%	0.017%
83	20.467	2997	3000	3001	rBV2	855	1025	0.31%	0.035%
84	20.525	3009	3010	3011	rBV	1046	615	0.19%	0.021%
85	20.672	3033	3035	3037	rBV2	1293	910	0.28%	0.031%
86	20.754	3047	3049	3052	rBV4	1094	1619	0.50%	0.056%
87	21.254	3132	3134	3135	rBV2	1662	1044	0.32%	0.036%
88	21.530	3177	3181	3186	rVB2	7899	11439	3.51%	0.395%
89	21.665	3198	3204	3210	rBV	154455	241742	74.15%	8.339%
90	22.411	3329	3331	3335	rBV5	2658	2431	0.75%	0.084%
91	24.650	3703	3712	3722	rBV	113645	300239	92.09%	10.357%
92	24.873	3742	3750	3763	rVB2	81510	227148	69.67%	7.836%
93	28.017	4283	4285	4288	rBV4	2088	1750	0.54%	0.060%
94	29.685	4567	4569	4573	rBV4	2050	2225	0.68%	0.077%
95	30.449	4697	4699	4701	rBV3	2255	2152	0.66%	0.074%


Sum of corrected areas: 2898845

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021560.D
Acq On : 29 Mar 2016 20:16
Operator : UM/SJ
Sample : H1935-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

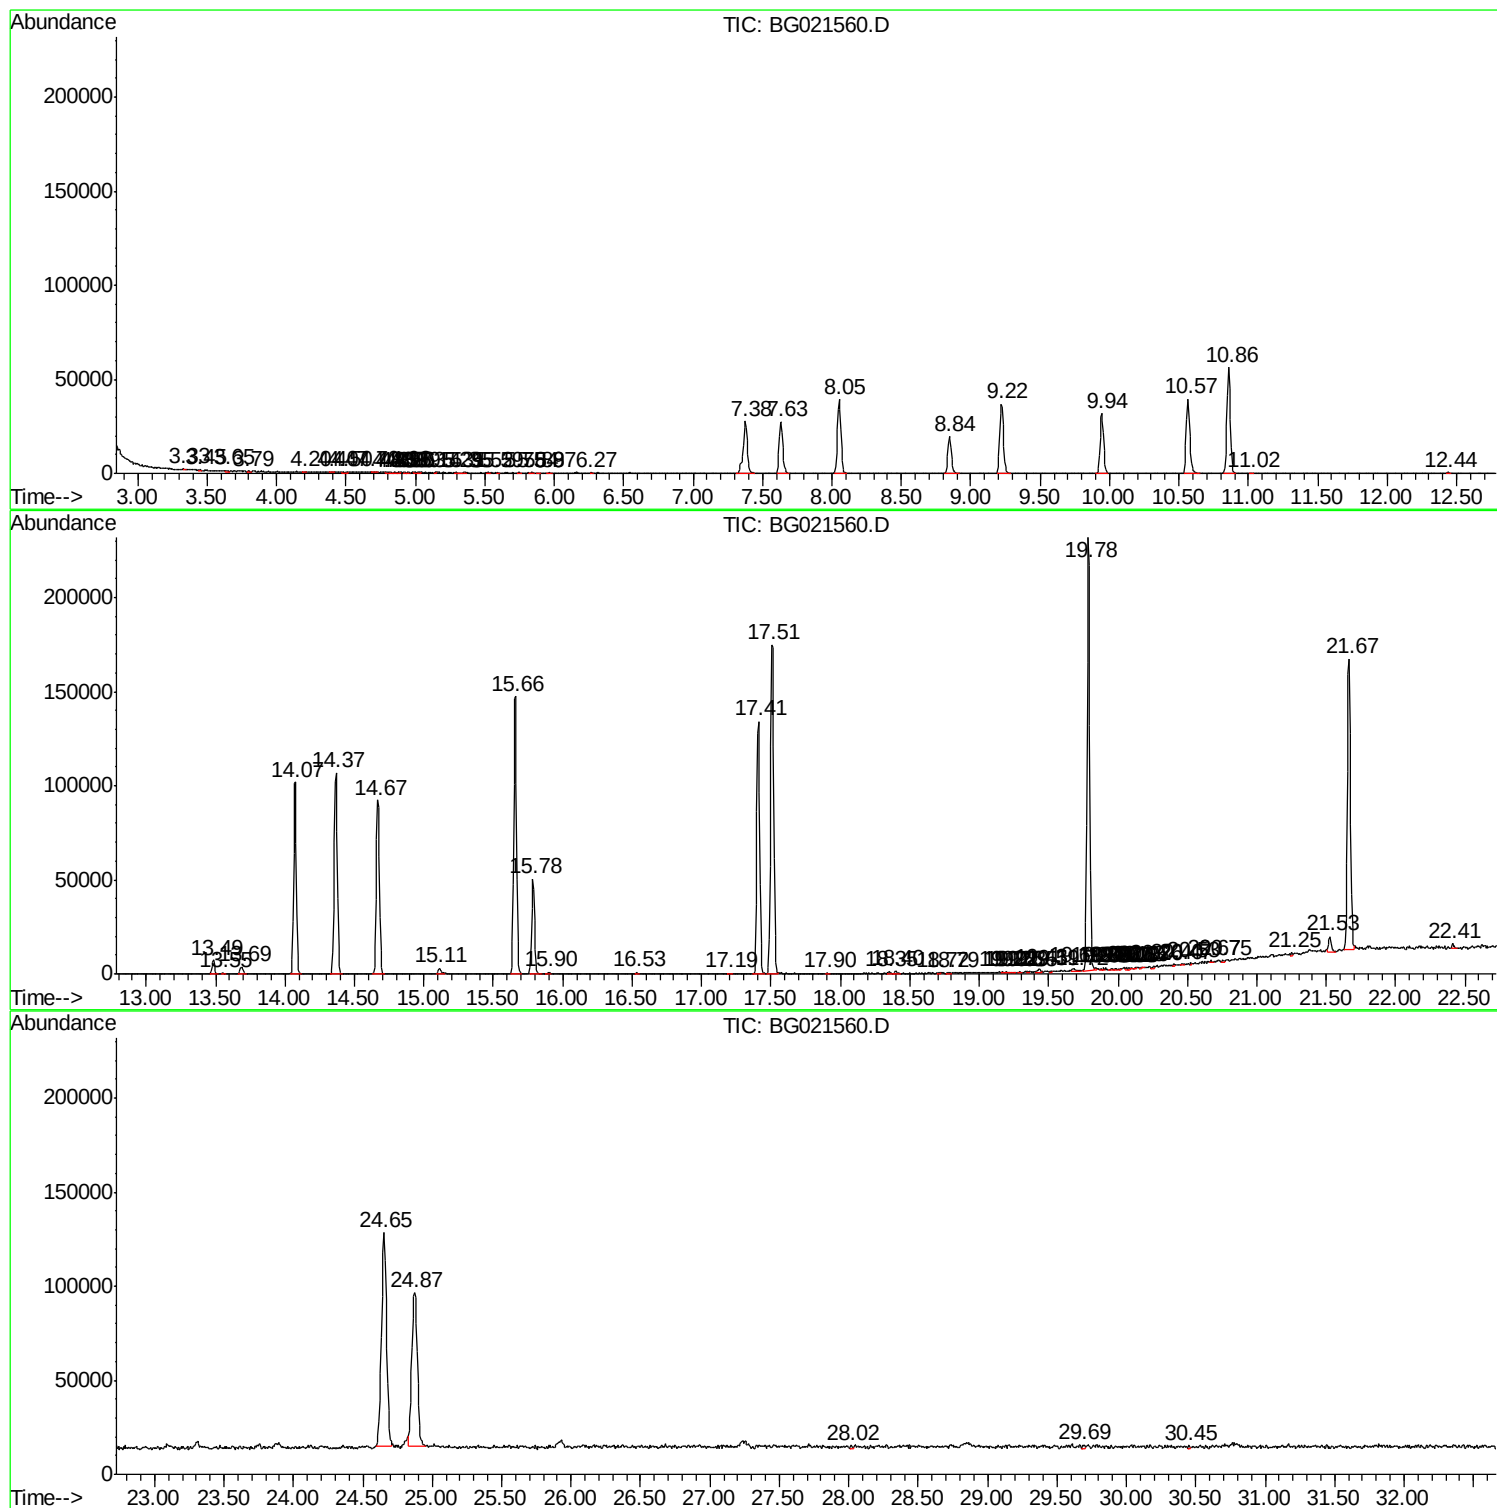

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021560.D
Acq On : 29 Mar 2016 20:16
Operator : UM/SJ
Sample : H1935-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021560.D
Acq On : 29 Mar 2016 20:16
Operator : UM/SJ
Sample : H1935-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AF9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc