

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021561.D
 Acq On : 29 Mar 2016 20:56
 Operator : UM/SJ
 Sample : H1935-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.238	66	68	69	rVB2	641	367	0.11%	0.012%
2	3.255	69	71	72	rBV2	460	354	0.10%	0.012%
3	3.332	82	84	88	rVB2	502	516	0.15%	0.018%
4	3.385	91	93	94	rVB	645	379	0.11%	0.013%
5	3.414	96	98	100	rBV2	412	350	0.10%	0.012%
6	3.473	105	108	109	rVB2	532	395	0.12%	0.013%
7	3.537	116	119	122	rVB2	333	347	0.10%	0.012%
8	3.561	122	123	127	rBV2	463	429	0.13%	0.015%
9	3.749	152	155	159	rVB2	588	649	0.19%	0.022%
10	3.778	159	160	163	rBV2	303	344	0.10%	0.012%
11	3.908	178	182	185	rBV2	298	509	0.15%	0.017%
12	4.002	195	198	200	rVB	403	431	0.13%	0.015%
13	4.031	200	203	204	rBV2	390	349	0.10%	0.012%
14	4.337	251	255	257	rVB3	329	396	0.12%	0.013%
15	4.366	257	260	264	rVB2	311	403	0.12%	0.014%
16	4.401	264	266	268	rVB	444	362	0.11%	0.012%
17	4.689	310	315	317	rBV	362	612	0.18%	0.021%
18	4.777	327	330	332	rBV	322	425	0.12%	0.014%
19	4.895	348	350	352	rBV	483	418	0.12%	0.014%
20	5.053	376	377	379	rBV	546	518	0.15%	0.018%
21	5.265	410	413	414	rVB	387	388	0.11%	0.013%
22	5.418	436	439	442	rVB	432	614	0.18%	0.021%
23	5.476	447	449	450	rBV	448	383	0.11%	0.013%
24	5.594	468	469	473	rBB	425	413	0.12%	0.014%
25	5.670	478	482	485	rBV2	361	665	0.19%	0.023%
26	6.152	562	564	567	rVB2	358	372	0.11%	0.013%
27	7.374	763	772	785	rBB	30772	61460	17.94%	2.087%
28	7.633	810	816	824	rBB	31900	53917	15.74%	1.831%
29	8.050	882	887	895	rBB	36893	61833	18.05%	2.100%
30	8.843	1017	1022	1031	rBB2	21129	36032	10.52%	1.223%
31	9.219	1080	1086	1094	rBV	39907	72582	21.19%	2.464%
32	9.942	1204	1209	1216	rBB	36137	64117	18.72%	2.177%
33	10.565	1309	1315	1324	rBV	43664	77605	22.65%	2.635%
34	10.858	1358	1365	1374	rBB	55541	94307	27.53%	3.202%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021561.D
 Acq On : 29 Mar 2016 20:56
 Operator : UM/SJ
 Sample : H1935-10
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	12.439	1632	1634	1637	rBB	426	424	0.12%	0.014%
36	14.072	1906	1912	1920	rBB	112577	155034	45.26%	5.264%
37	14.366	1956	1962	1971	rBV	116673	175770	51.31%	5.968%
38	14.671	2007	2014	2020	rBB2	87429	138924	40.55%	4.717%
39	15.112	2085	2089	2097	rBB2	3082	4922	1.44%	0.167%
40	15.659	2176	2182	2190	rBB	163079	234080	68.33%	7.948%
41	15.788	2199	2204	2213	rBB	49666	75424	22.02%	2.561%
42	15.899	2220	2223	2226	rBB	897	903	0.26%	0.031%
43	17.198	2441	2444	2447	rBB	292	356	0.10%	0.012%
44	17.409	2474	2480	2486	rBV2	125749	184822	53.95%	6.276%
45	17.509	2491	2497	2510	rVB	183828	273511	79.84%	9.287%
46	18.126	2601	2602	2606	rBV	317	355	0.10%	0.012%
47	18.355	2637	2641	2645	rBV	819	1108	0.32%	0.038%
48	18.673	2693	2695	2699	rBV	342	412	0.12%	0.014%
49	18.784	2710	2714	2716	rVB	402	539	0.16%	0.018%
50	18.878	2725	2730	2732	rVV2	452	524	0.15%	0.018%
51	18.931	2736	2739	2742	rVB	302	391	0.11%	0.013%
52	18.961	2742	2744	2747	rBV	558	386	0.11%	0.013%
53	19.037	2756	2757	2759	rBV	532	403	0.12%	0.014%
54	19.090	2764	2766	2768	rBV2	519	401	0.12%	0.014%
55	19.149	2773	2776	2777	rBV	779	578	0.17%	0.020%
56	19.207	2784	2786	2788	rBV	424	408	0.12%	0.014%
57	19.337	2805	2808	2809	rBV2	508	524	0.15%	0.018%
58	19.360	2809	2812	2814	rVB2	652	693	0.20%	0.024%
59	19.431	2820	2824	2826	rVV2	1695	2282	0.67%	0.077%
60	19.536	2839	2842	2843	rVB3	418	365	0.11%	0.012%
61	19.566	2846	2847	2850	rBV3	631	461	0.13%	0.016%
62	19.601	2852	2853	2855	rBV2	439	412	0.12%	0.014%
63	19.677	2863	2866	2869	rBV3	1322	1686	0.49%	0.057%
64	19.707	2869	2871	2872	rVB	673	455	0.13%	0.015%
65	19.789	2878	2885	2895	rVV	239260	342558	100.00%	11.631%
66	19.901	2903	2904	2906	rBV	681	449	0.13%	0.015%
67	19.930	2908	2909	2910	rBV	820	369	0.11%	0.013%
68	19.948	2910	2912	2913	rBV	582	461	0.13%	0.016%
69	19.971	2913	2916	2917	rVB2	708	680	0.20%	0.023%
70	20.006	2917	2922	2924	rBV3	887	1230	0.36%	0.042%
71	20.065	2930	2932	2933	rBV	668	630	0.18%	0.021%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021561.D
Acq On : 29 Mar 2016 20:56
Operator : UM/SJ
Sample : H1935-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Title : SVOA CALIBRATION

72	20.106	2938	2939	2941	rBV2	1320	1107	0.32%	0.038%
73	20.136	2943	2944	2948	rVV3	735	911	0.27%	0.031%
74	20.165	2948	2949	2952	rVB2	789	661	0.19%	0.022%
75	20.236	2957	2961	2964	rVV3	783	1152	0.34%	0.039%
76	20.259	2964	2965	2967	rBV2	803	583	0.17%	0.020%
77	20.371	2982	2984	2986	rBV2	943	846	0.25%	0.029%
78	20.576	3017	3019	3020	rVB2	999	411	0.12%	0.014%
79	20.612	3023	3025	3028	rBV3	961	975	0.28%	0.033%
80	20.729	3044	3045	3049	rBV4	1769	2531	0.74%	0.086%
81	20.905	3074	3075	3076	rBV	1209	774	0.23%	0.026%
82	20.982	3087	3088	3092	rBV3	1347	1714	0.50%	0.058%
83	21.099	3106	3108	3112	rBV4	1701	1708	0.50%	0.058%
84	21.369	3152	3154	3155	rBV2	1753	1125	0.33%	0.038%
85	21.663	3198	3204	3211	rBV	150475	244436	71.36%	8.300%
86	24.654	3703	3713	3725	rVB	122066	324068	94.60%	11.004%
87	24.871	3741	3750	3760	rVB	79323	222471	64.94%	7.554%
88	30.300	4672	4674	4677	rBV4	2184	2178	0.64%	0.074%
89	31.328	4847	4849	4852	rBV3	2112	1301	0.38%	0.044%


Sum of corrected areas: 2945123

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021561.D
Acq On : 29 Mar 2016 20:56
Operator : UM/SJ
Sample : H1935-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG8

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

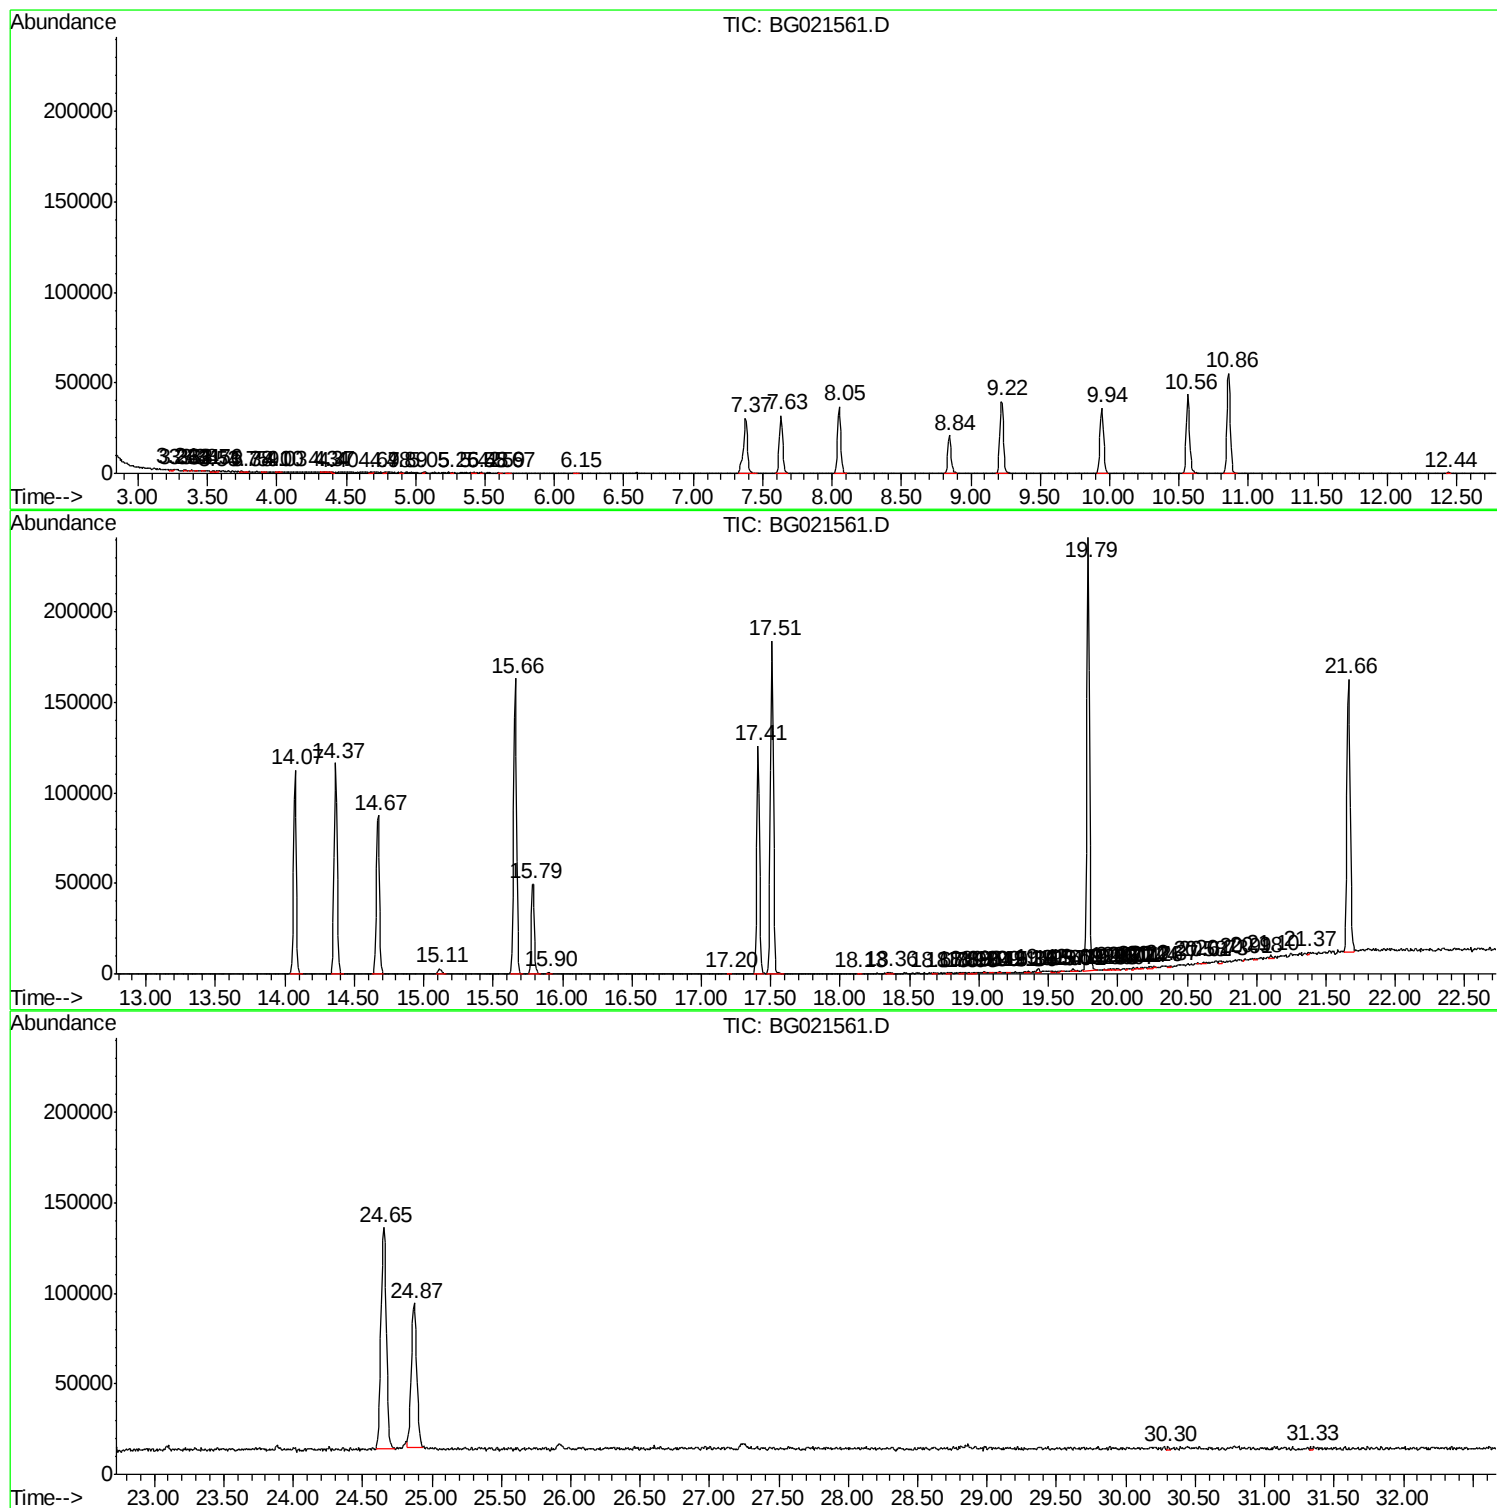

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021561.D
Acq On : 29 Mar 2016 20:56
Operator : UM/SJ
Sample : H1935-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG8

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021561.D
Acq On : 29 Mar 2016 20:56
Operator : UM/SJ
Sample : H1935-10
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG8

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc