

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021567.D
 Acq On : 30 Mar 2016 00:53
 Operator : UM/SJ
 Sample : H1910-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.397	94	95	97	rBV	553	425	0.12%	0.014%
2	3.444	102	103	106	rVV	923	696	0.19%	0.023%
3	3.491	109	111	113	rBV3	578	628	0.18%	0.021%
4	3.561	122	123	128	rVB	780	694	0.19%	0.023%
5	3.638	134	136	138	rBV	412	460	0.13%	0.015%
6	3.691	143	145	147	rVV2	650	461	0.13%	0.015%
7	3.714	147	149	153	rVB3	344	464	0.13%	0.015%
8	3.785	159	161	162	rBV2	574	519	0.15%	0.017%
9	3.896	179	180	185	rVB3	389	415	0.12%	0.014%
10	4.025	200	202	204	rBV2	574	585	0.16%	0.019%
11	4.137	219	221	224	rVB2	441	385	0.11%	0.013%
12	4.437	268	272	274	rBV2	362	502	0.14%	0.016%
13	4.513	283	285	287	rBV	309	363	0.10%	0.012%
14	4.537	287	289	292	rVV2	421	504	0.14%	0.017%
15	4.654	306	309	310	rVB	418	404	0.11%	0.013%
16	4.754	322	326	332	rVB2	374	736	0.21%	0.024%
17	4.795	332	333	335	rBV	492	375	0.10%	0.012%
18	4.848	339	342	345	rBV2	342	486	0.14%	0.016%
19	5.065	376	379	382	rVB	599	724	0.20%	0.024%
20	5.218	402	405	408	rBV	400	390	0.11%	0.013%
21	5.277	412	415	416	rVB	488	440	0.12%	0.014%
22	5.295	416	418	421	rBV	492	508	0.14%	0.017%
23	5.424	437	440	444	rBV	341	503	0.14%	0.017%
24	5.594	466	469	471	rBV	474	491	0.14%	0.016%
25	7.345	762	767	768	rBV2	16716	23557	6.59%	0.774%
26	7.374	768	772	782	rVB2	38140	70519	19.72%	2.316%
27	7.627	810	815	826	rBB	44779	77524	21.68%	2.546%
28	8.050	881	887	896	rBB	34560	58983	16.49%	1.937%
29	8.843	1016	1022	1032	rBB2	40430	69827	19.52%	2.293%
30	9.219	1080	1086	1096	rBB	49366	85637	23.94%	2.812%
31	9.942	1203	1209	1218	rBB2	43090	75003	20.97%	2.463%
32	10.559	1309	1314	1326	rBB	50167	95025	26.57%	3.120%
33	10.853	1358	1364	1373	rBB	48489	86074	24.07%	2.826%
34	11.017	1389	1392	1396	rBB	353	508	0.14%	0.017%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
 Data File : BG021567.D
 Acq On : 30 Mar 2016 00:53
 Operator : UM/SJ
 Sample : H1910-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	12.445	1631	1635	1637	rBB	697	592	0.17%	0.019%
36	14.072	1906	1912	1918	rBV	120959	165970	46.41%	5.450%
37	14.366	1955	1962	1970	rBB	129680	195434	54.64%	6.418%
38	14.672	2008	2014	2020	rBB2	74996	116760	32.65%	3.834%
39	15.101	2083	2087	2096	rBV2	9447	17608	4.92%	0.578%
40	15.659	2175	2182	2190	rBB	174729	252201	70.52%	8.282%
41	15.788	2199	2204	2211	rBV	51612	73665	20.60%	2.419%
42	15.900	2219	2223	2225	rBB	694	903	0.25%	0.030%
43	17.410	2474	2480	2489	rBB	104524	155539	43.49%	5.107%
44	17.510	2491	2497	2504	rBV	198131	283487	79.26%	9.309%
45	18.655	2686	2692	2694	rBV	506	828	0.23%	0.027%
46	19.067	2758	2762	2763	rBV	486	591	0.17%	0.019%
47	19.172	2775	2780	2784	rBV	347	600	0.17%	0.020%
48	19.296	2797	2801	2803	rBV	395	518	0.14%	0.017%
49	19.360	2809	2812	2815	rVB2	542	586	0.16%	0.019%
50	19.384	2815	2816	2818	rBV	572	413	0.12%	0.014%
51	19.425	2818	2823	2827	rVV2	1981	2531	0.71%	0.083%
52	19.484	2832	2833	2834	rBV	736	442	0.12%	0.015%
53	19.519	2838	2839	2841	rVB	552	372	0.10%	0.012%
54	19.584	2847	2850	2851	rBV	474	403	0.11%	0.013%
55	19.642	2857	2860	2861	rBV	616	504	0.14%	0.017%
56	19.654	2861	2862	2863	rBV	676	369	0.10%	0.012%
57	19.672	2863	2865	2872	rVB4	1325	2229	0.62%	0.073%
58	19.736	2872	2876	2877	rBV2	698	640	0.18%	0.021%
59	19.789	2877	2885	2891	rBV	247097	357645	100.00%	11.744%
60	19.889	2901	2902	2905	rBV3	652	779	0.22%	0.026%
61	19.971	2914	2916	2917	rBV	636	462	0.13%	0.015%
62	19.989	2917	2919	2921	rVB2	916	795	0.22%	0.026%
63	20.007	2921	2922	2923	rBV	744	399	0.11%	0.013%
64	20.024	2923	2925	2927	rVB3	822	645	0.18%	0.021%
65	20.054	2927	2930	2931	rBV2	566	612	0.17%	0.020%
66	20.083	2933	2935	2938	rVB4	692	514	0.14%	0.017%
67	20.165	2946	2949	2950	rBV2	538	440	0.12%	0.014%
68	20.183	2950	2952	2954	rBV	469	560	0.16%	0.018%
69	20.312	2968	2974	2975	rBV4	864	1629	0.46%	0.053%
70	20.365	2981	2983	2985	rBV2	784	702	0.20%	0.023%
71	20.383	2985	2986	2987	rBV	796	377	0.11%	0.012%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021567.D
Acq On : 30 Mar 2016 00:53
Operator : UM/SJ
Sample : H1910-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AEO

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Title : SVOA CALIBRATION

72	20.494	3003	3005	3007	rBV2	827	807	0.23%	0.026%
73	20.553	3013	3015	3017	rBV2	931	887	0.25%	0.029%
74	20.653	3030	3032	3034	rBV3	1277	1411	0.39%	0.046%
75	20.706	3039	3041	3044	rVV	1305	1230	0.34%	0.040%
76	21.041	3096	3098	3099	rBV2	1199	978	0.27%	0.032%
77	21.135	3112	3114	3115	rBV2	1424	734	0.21%	0.024%
78	21.664	3198	3204	3213	rBV	119829	202218	56.54%	6.640%
79	21.840	3233	3234	3235	rVB	1927	680	0.19%	0.022%
80	24.067	3611	3613	3615	rBV3	1941	1382	0.39%	0.045%
81	24.654	3703	3713	3724	rBV	132387	349739	97.79%	11.484%
82	24.872	3742	3750	3762	rVB	66519	188896	52.82%	6.203%
83	25.876	3919	3921	3922	rBV2	2307	1884	0.53%	0.062%
84	30.489	4704	4706	4707	rBV2	1766	920	0.26%	0.030%


Sum of corrected areas: 3045325

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021567.D
Acq On : 30 Mar 2016 00:53
Operator : UM/SJ
Sample : H1910-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

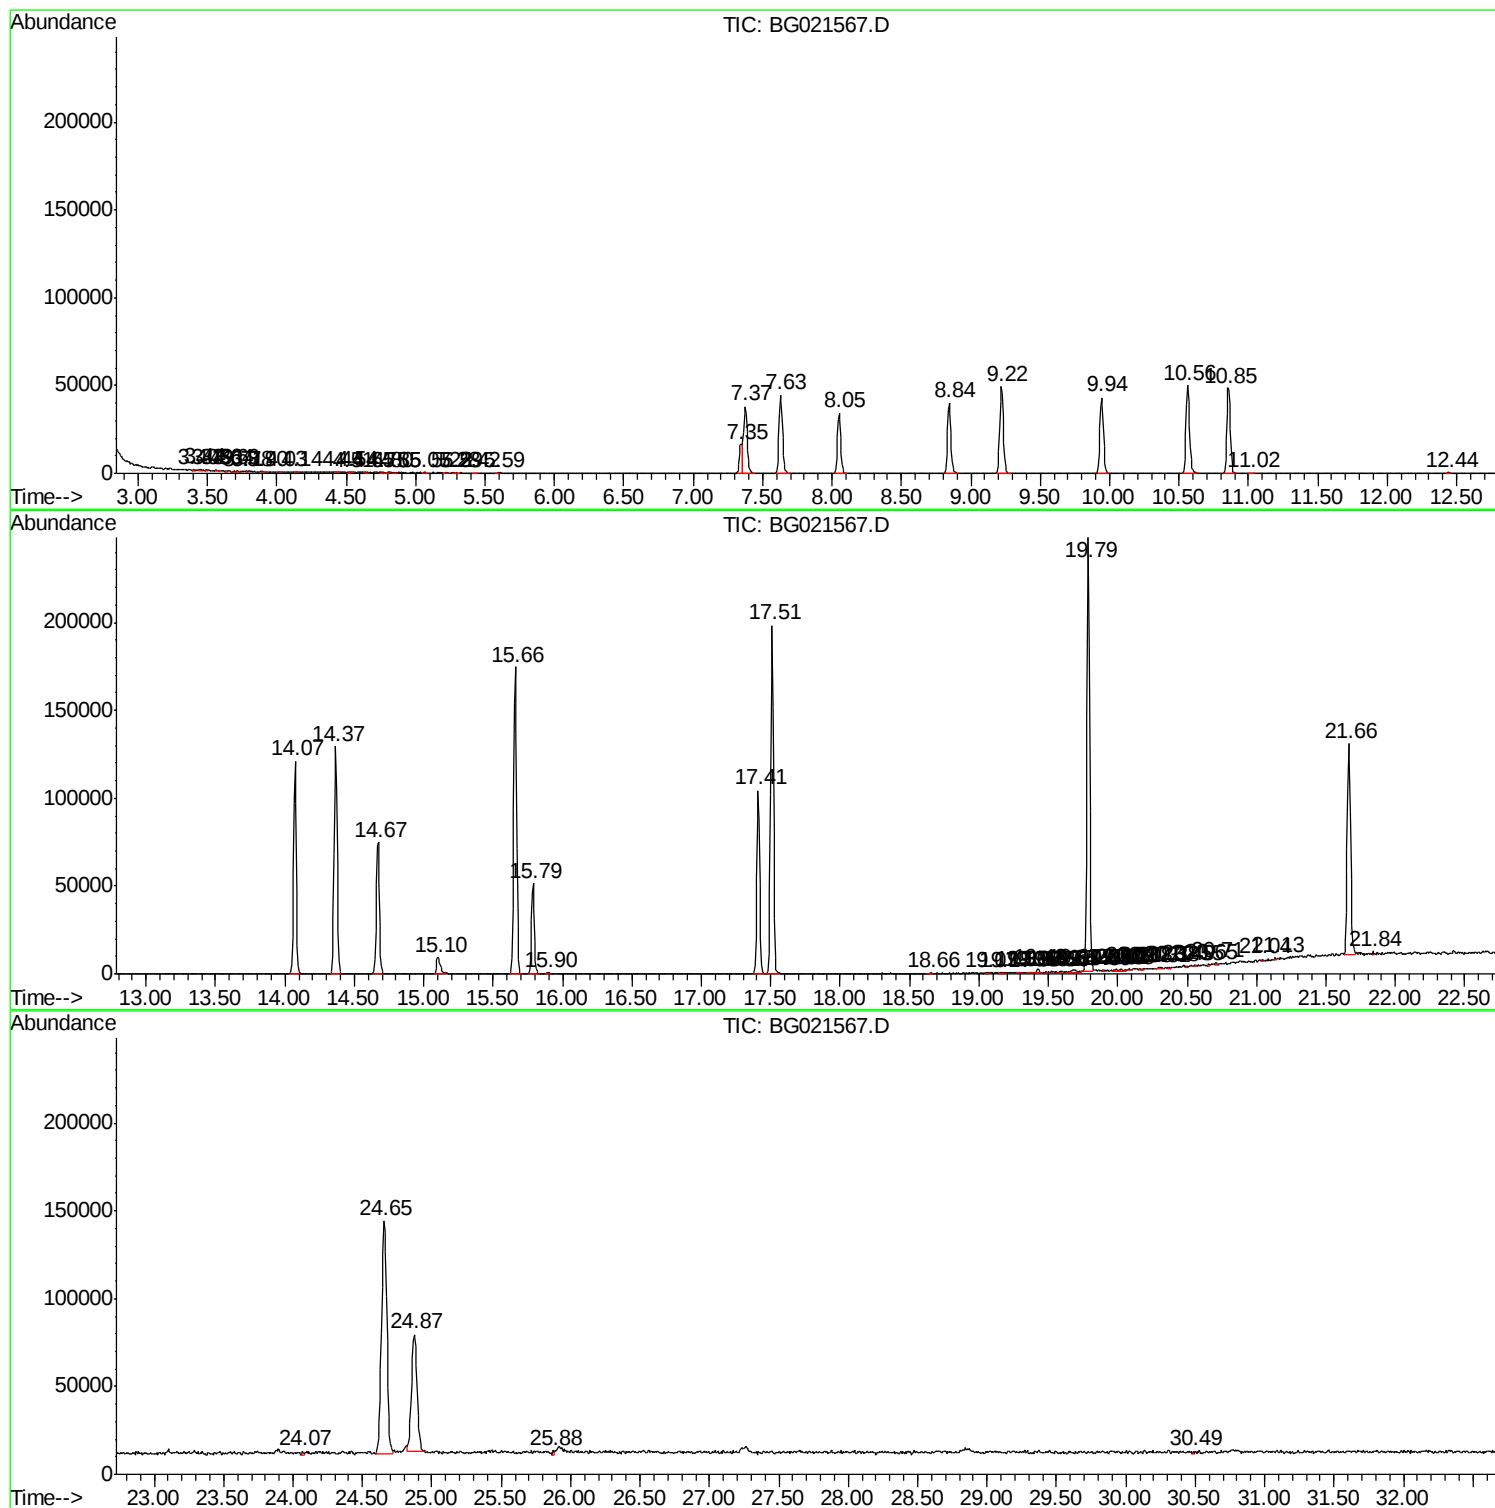

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021567.D
Acq On : 30 Mar 2016 00:53
Operator : UM/SJ
Sample : H1910-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG032916\
Data File : BG021567.D
Acq On : 30 Mar 2016 00:53
Operator : UM/SJ
Sample : H1910-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AE0

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc