

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032917\
 Data File : BG026494.D
 Acq On : 30 Mar 2017 2:38
 Operator : SJ/MA
 Sample : I2391-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BL6

Quant Time: Mar 30 03:23:28 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 03:23:34 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	188136	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	769999	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.64	164	457176	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.38	188	1089618	20.00	ng/ul	0.00
77) Chrysene-d12	21.62	240	1293175	20.00	ng/ul	0.00
85) Perylene-d12	24.80	264	1285624	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	20724	5.27	ng/uL	0.00
5) Phenol-d5	7.21	99	88712	6.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	245313	31.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	305448	24.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	145348	13.02	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	189231	34.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	228663	35.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	349000	29.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	27123	2.30	ng/ul	0.02
43) Dimethylphthalate-d6	14.04	166	1232845	34.82	ng/ul	0.00
46) Acenaphthylene-d8	14.34	160	1495809	33.91	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	41209	5.98	ng/ul	0.01
57) Fluorene-d10	15.63	176	1166807	36.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.75	200	244178	34.85	ng/ul	0.00
70) Anthracene-d10	17.48	188	1756383	35.50	ng/ul	0.00
78) Pyrene-d10	19.76	212	2043642	35.43	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.59	264	2089565	37.83	ng/ul	0.00


Target Compounds					Ovalue
20) Nitrobenzene	9.24	77	24591	2.25 ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032917\
Data File : BG026494.D
Acq On : 30 Mar 2017 2:38
Operator : SJ/MA
Sample : I2391-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BL6

Quant Time: Mar 30 03:23:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 03:23:34 2017
Response via : Initial Calibration

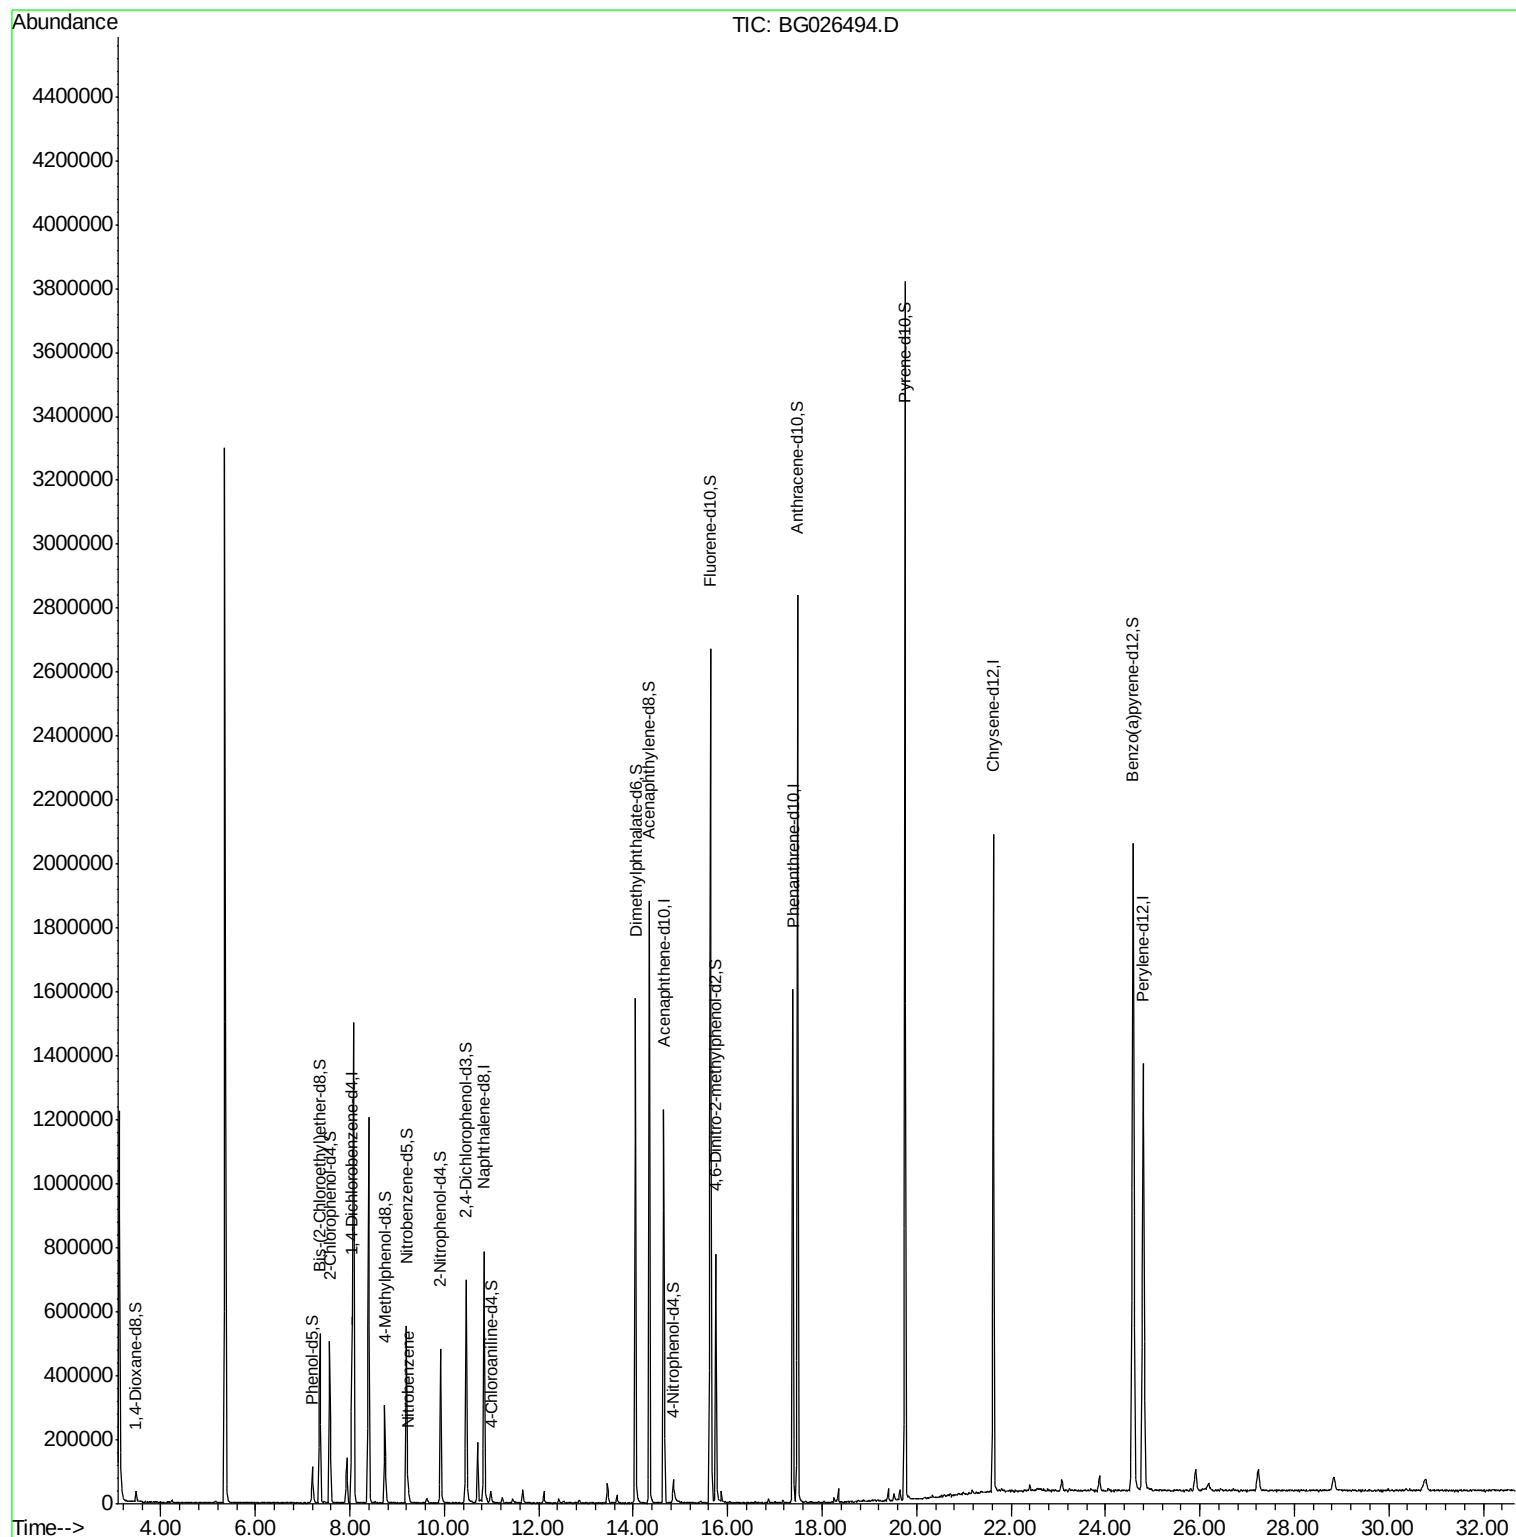


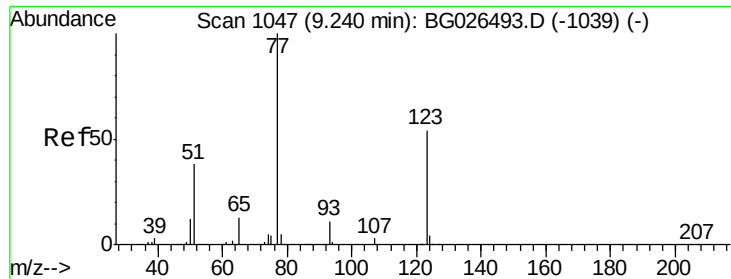

#20
 Nitrobenzene
 Concen: 2.25 ng/ul
 RT: 9.24 min Scan# 1048
 Delta R.T. 0.00 min
 Lab File: BG026494.D
 Acq: 30 Mar 2017 2:38

Instrument :
 BNA_G
 ClientSampleID :
 C0BL6

Tot Ion	Ratio	Lower	Upper
77	100		
123	52.4	39.0	58.4
65	9.6	10.4	15.6

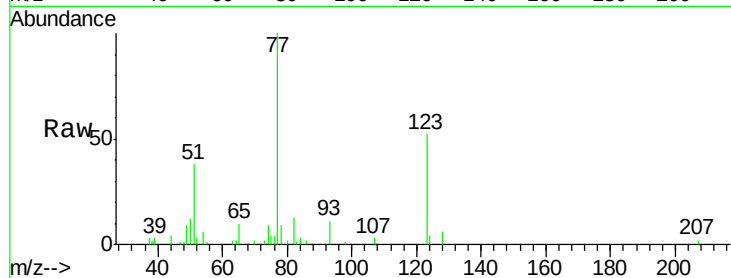

Abundance Ion 77.00 (76.70 to 77.70): BGC
 Ion 123.00 (122.70 to 123.70): BGC
 Ion 65.00 (64.70 to 65.70): BGC

