
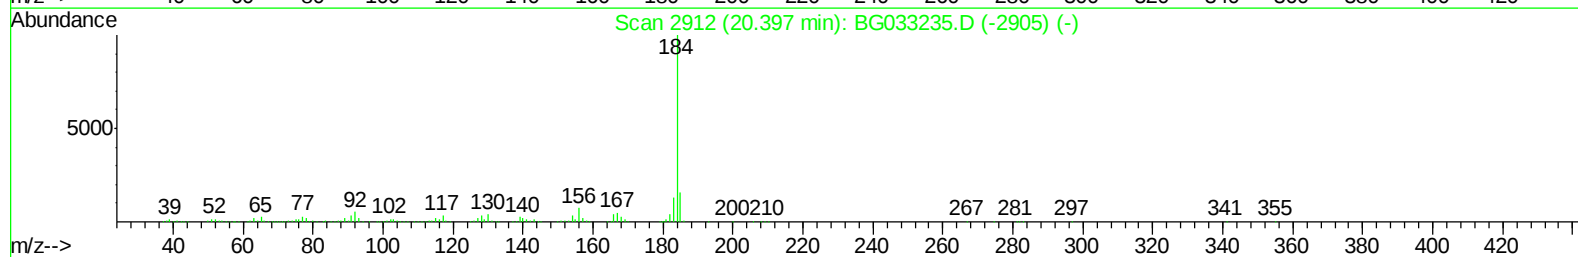
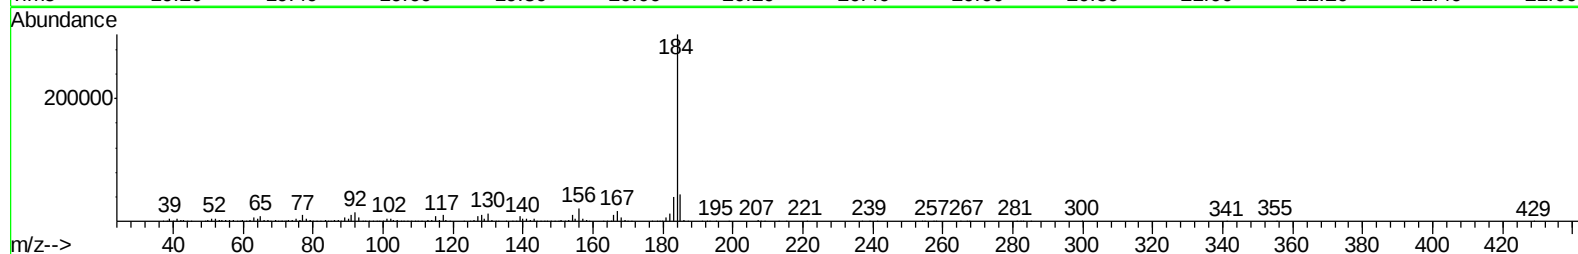


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
 Data File : BG033423.D
 Acq On : 29 Mar 2018 17:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:55:59 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 18:34:58 2018
 Response via : Initial Calibration

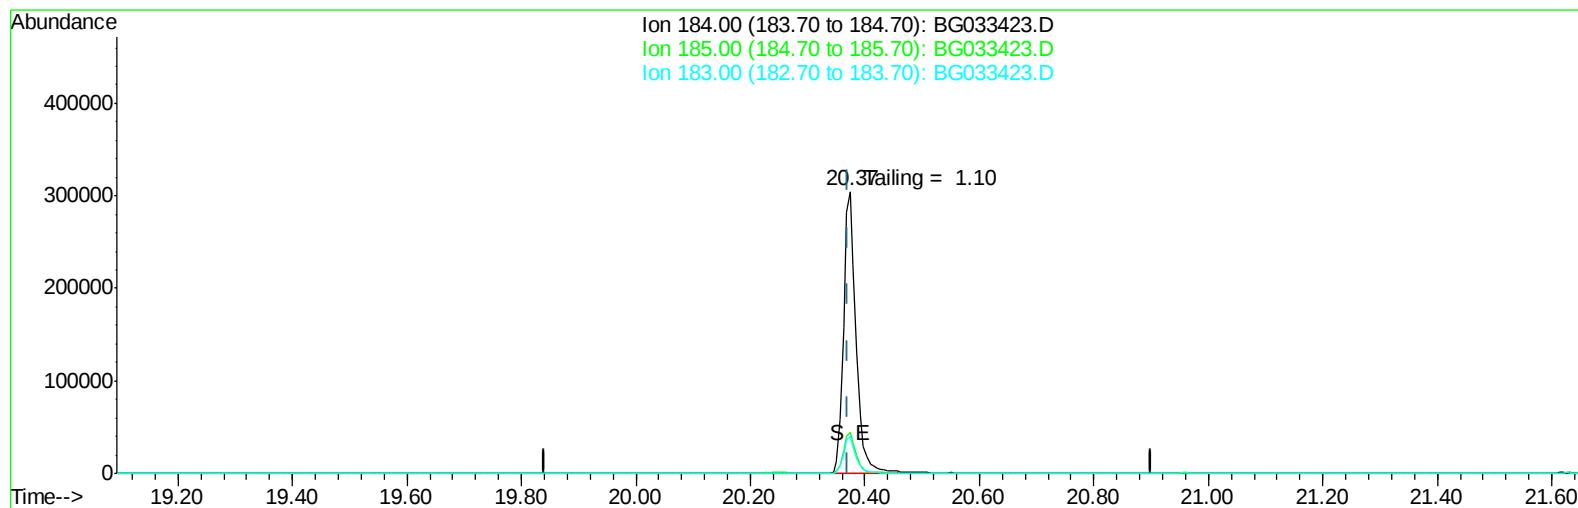

TIC: BG033423.D

(76) Benzidine




20.374min (+0.003) 302019.23ng

response 466848

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.78
183.00	13.30	13.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
Data File : BG033423.D
Acq On : 29 Mar 2018 17:04
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:55:59 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

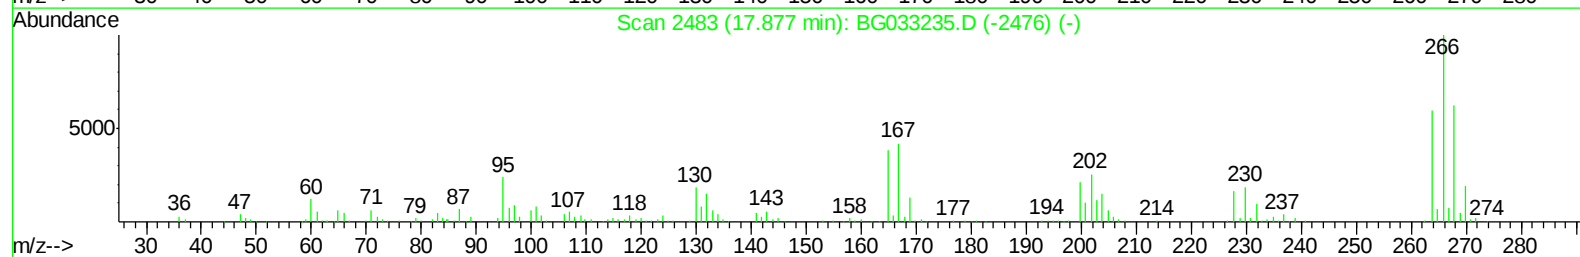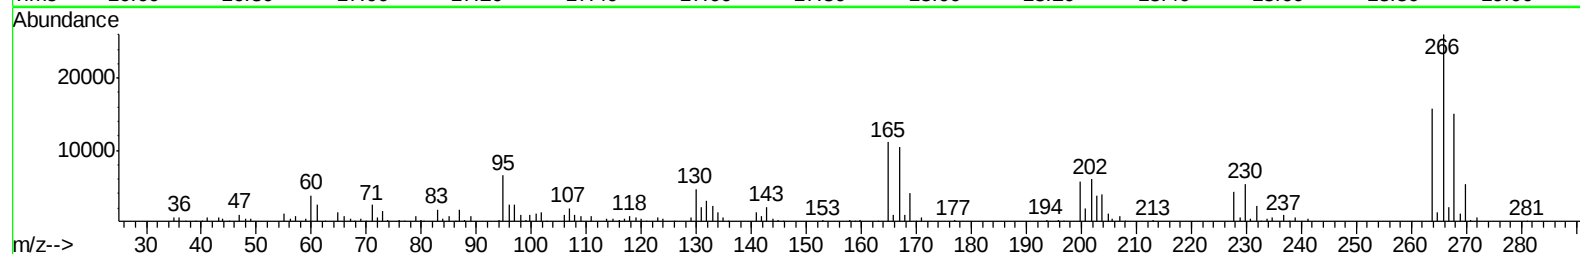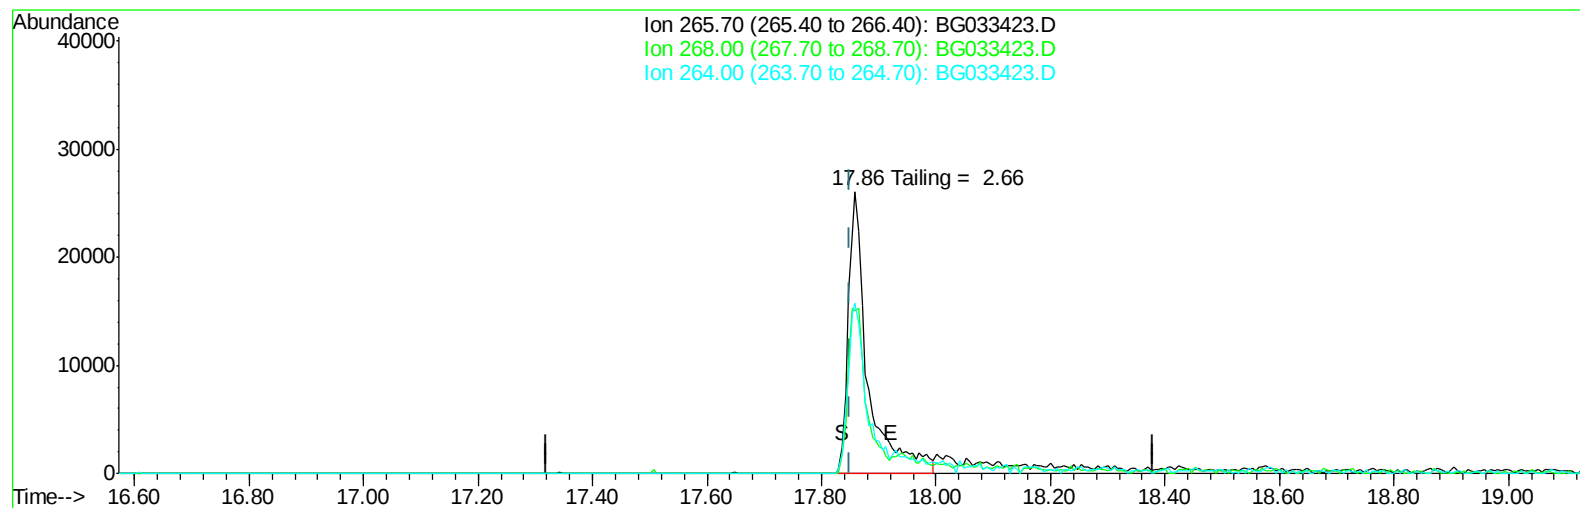

TIC: BG033423.D

(69) Pentachlorophenol (C)

17.859min (+0.009) 11609.91ng m

response 62320

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.88
264.00	62.00	60.43
0.00	0.00	0.00