
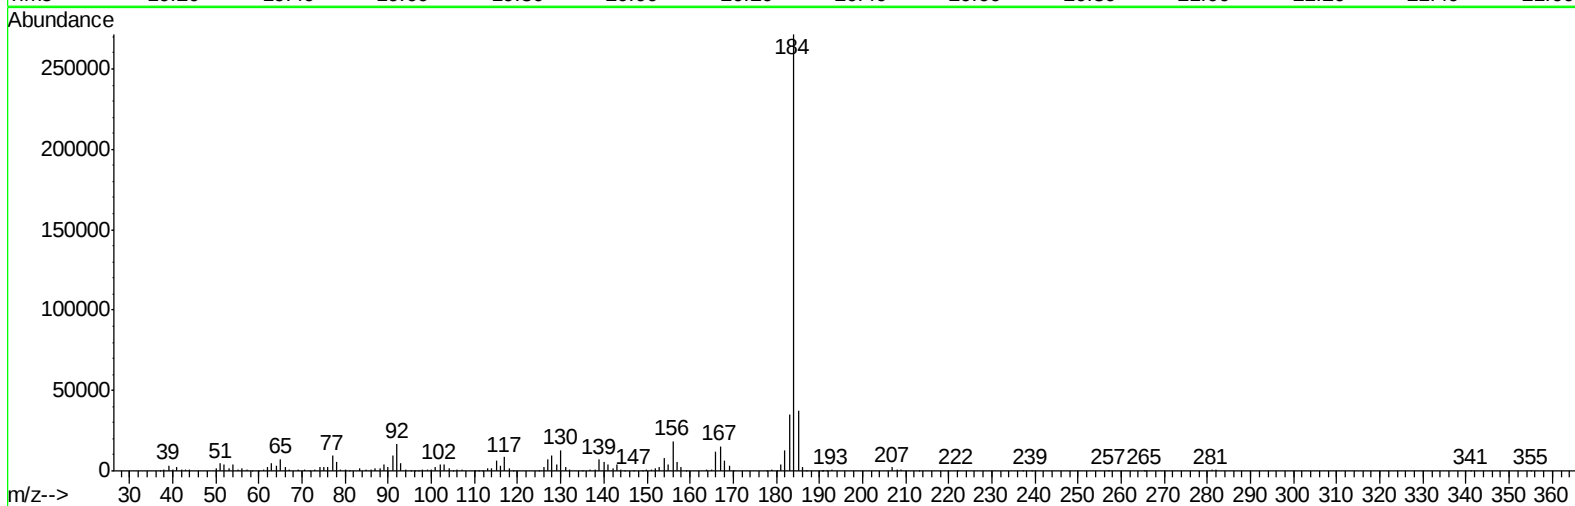


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
Data File : BG033442.D
Acq On : 30 Mar 2018 6:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:57:21 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

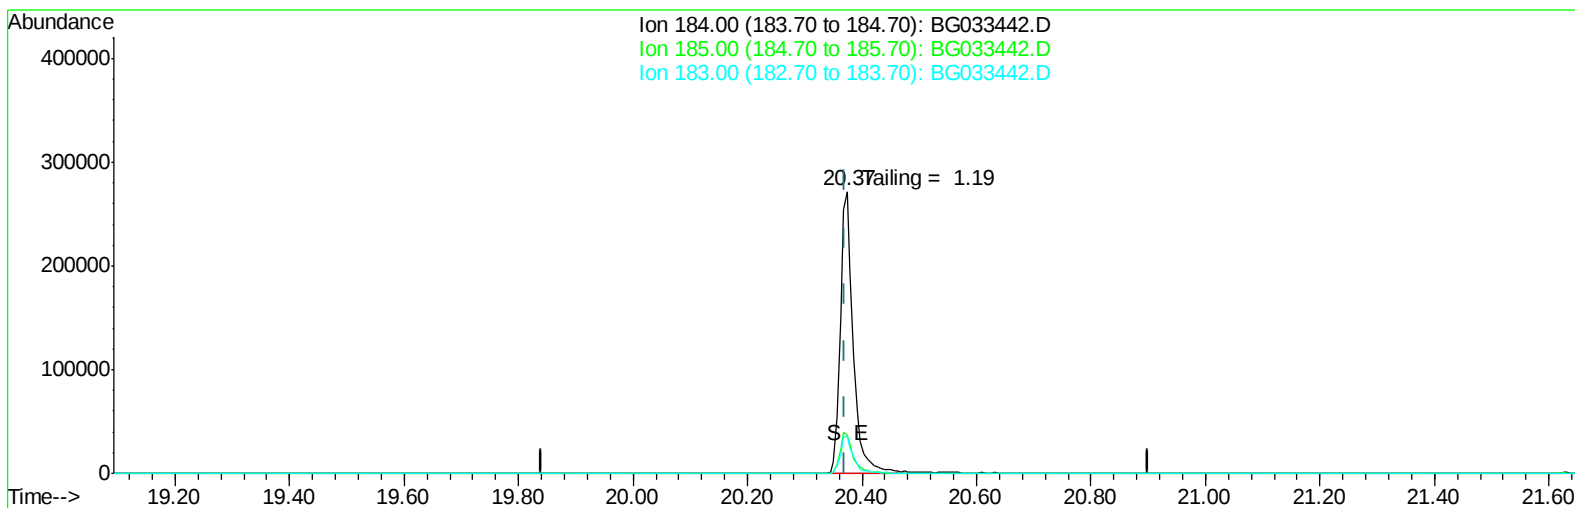

TIC: BG033442.D

(76) Benzidine



20.374min (+0.003) 0.00ng

response 432504

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.82
183.00	13.30	13.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
Data File : BG033442.D
Acq On : 30 Mar 2018 6:51
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:57:21 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

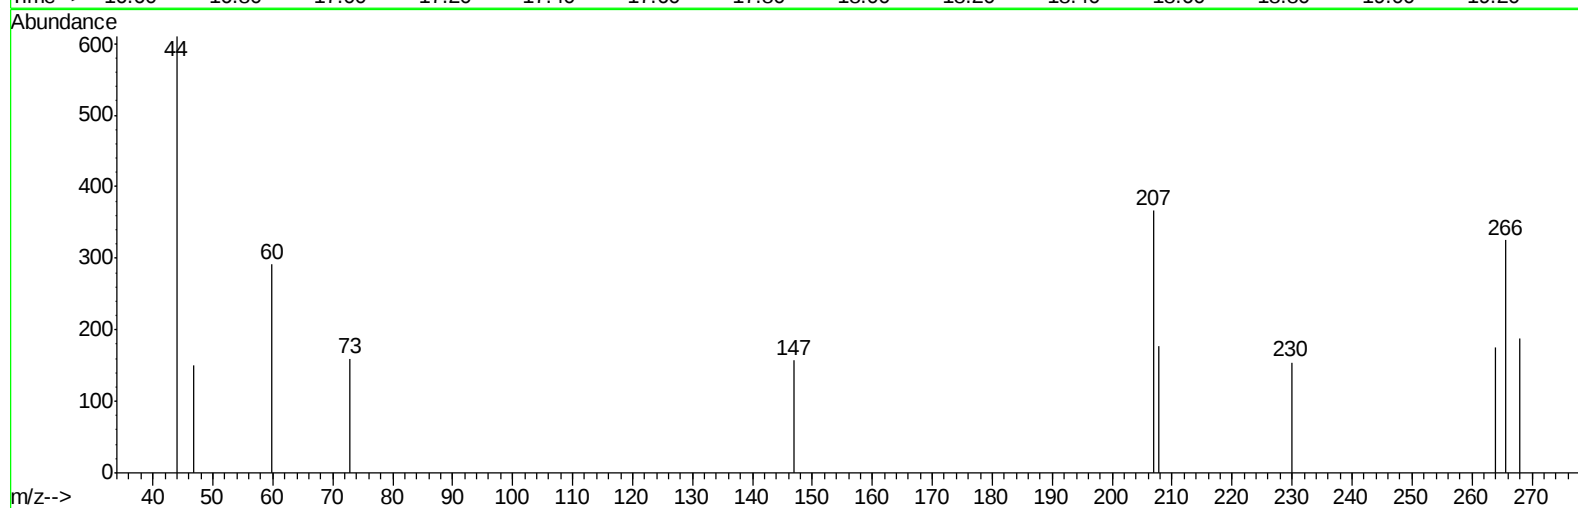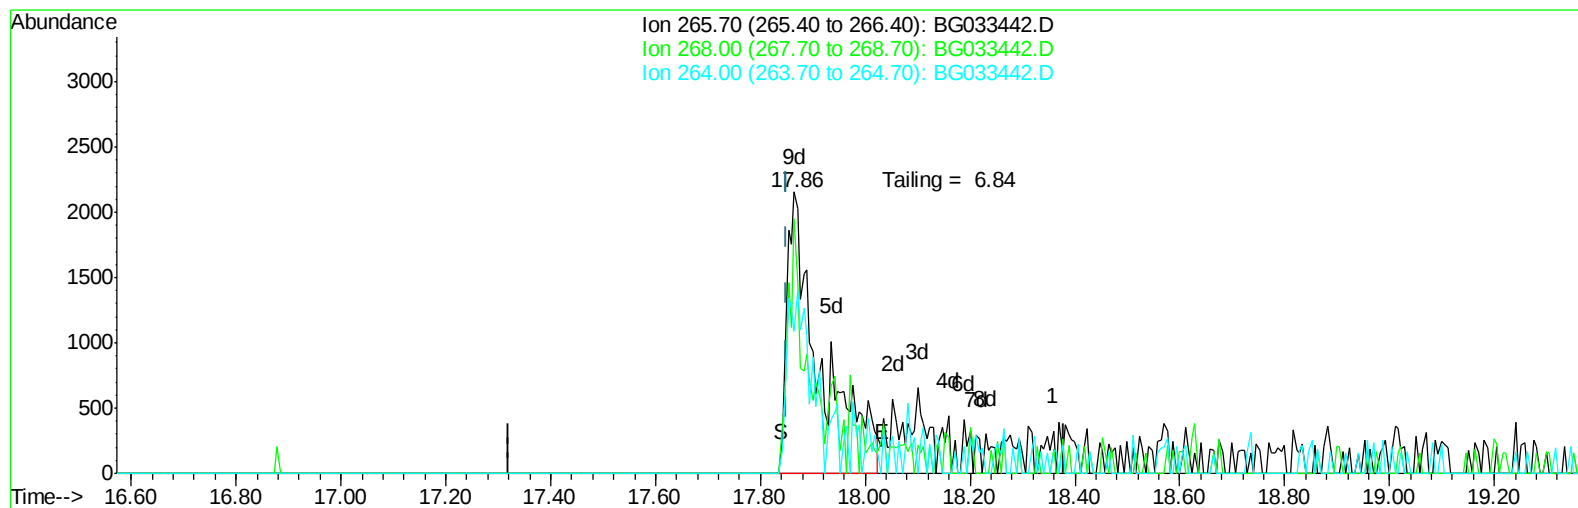

TIC: BG033442.D

(69) Pentachlorophenol (C)

18.359min (+0.508) 822.87ng

response 420

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.54
264.00	62.00	53.85
0.00	0.00	0.00