

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
 Data File : BG033440.D
 Acq On : 30 Mar 2018 3:44
 Operator : SJ/JU
 Sample : PB107742BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB107742BL

Quant Time: Mar 30 08:19:44 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 18:34:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	27824	20.00	ng	-0.01
21) Naphthalene-d8	11.75	136	111667	20.00	ng	0.00
38) Acenaphthene-d10	15.48	164	92792	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	288354	20.00	ng	0.00
75) Chrysene-d12	22.56	240	331522	20.00	ng	0.00
86) Perylene-d12	26.33	264	352567	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	238260	160.57	ng	0.00
7) Phenol-d6	7.99	99	340660	133.62	ng	0.00
23) Nitrobenzene-d5	10.07	82	210827	86.74	ng	-0.01
41) 2,4,6-Tribromophenol	16.96	330	106886	77.02	ng	0.00
44) 2-Fluorobiphenyl	14.11	172	553115	86.05	ng	0.00
78) Terphenyl-d14	20.73	244	1327933	85.66	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
Data File : BG033440.D
Acq On : 30 Mar 2018 3:44
Operator : SJ/JU
Sample : PB107742BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB107742BL

Quant Time: Mar 30 08:19:44 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

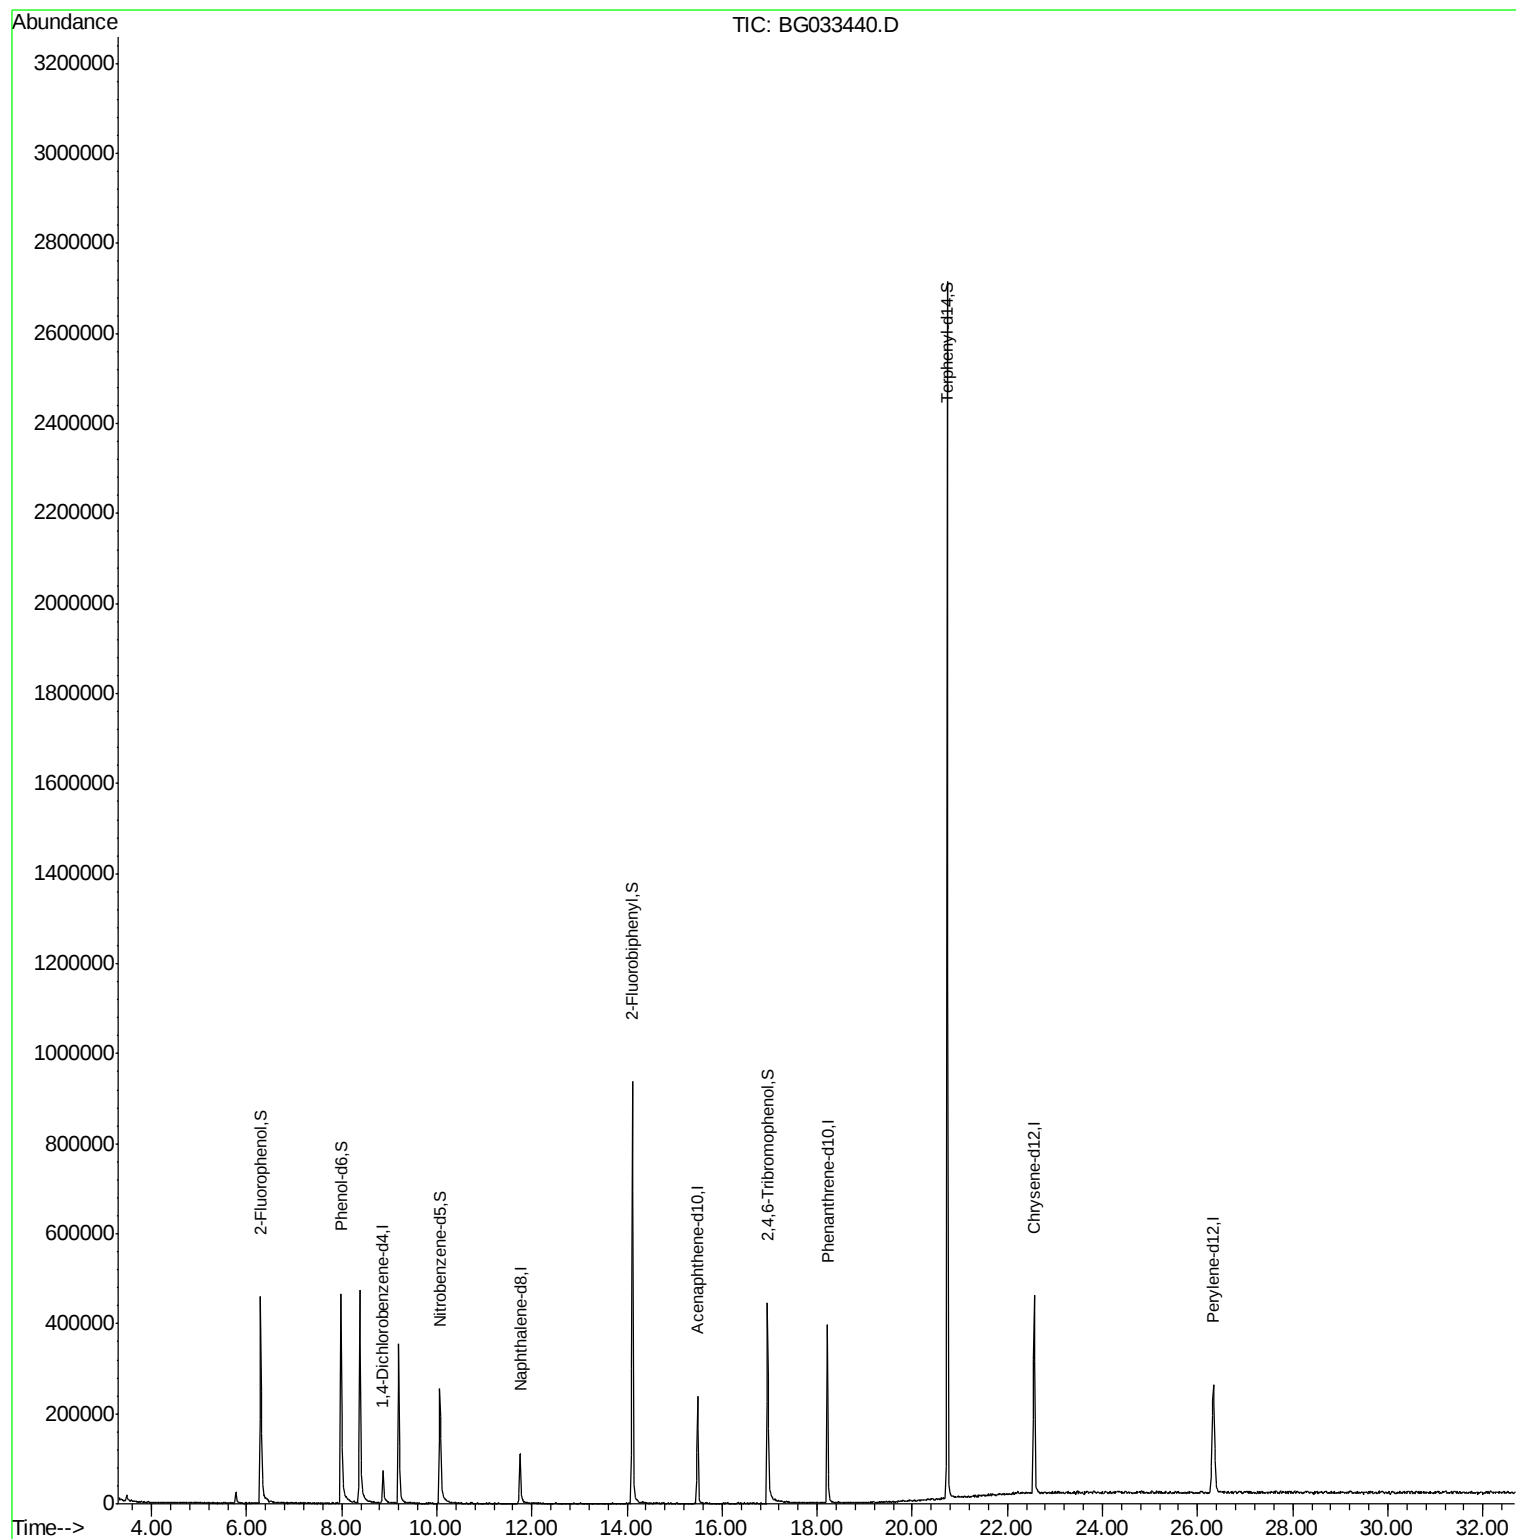




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.87 min Scan# 949
 Delta R.T. -0.01 min
 Lab File: BG033440.D
 Acq: 30 Mar 2018 3:44

Instrument :
 BNA_G
 ClientSampleId :
 PB107742BL

Tot Ion:152 Resp: 27824
 Ion Ratio Lower Upper
 152 100
 150 151.4 126.6 189.8
 115 61.3 53.0 79.4

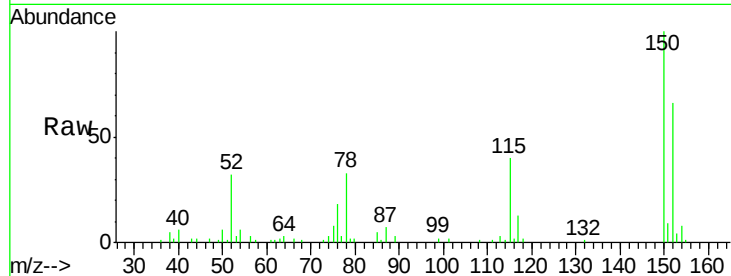


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

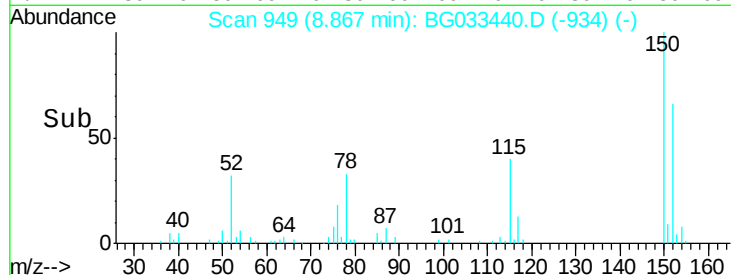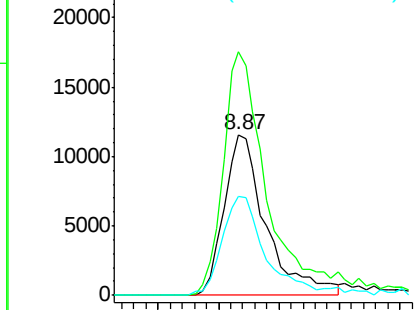



#5


2-Fluorophenol
 Concen: 160.569 ng
 RT: 6.29 min Scan# 511
 Delta R.T. -0.00 min
 Lab File: BG033440.D
 Acq: 30 Mar 2018 3:44

Tgt Ion:112 Resp: 238260
 Ion Ratio Lower Upper
 112 100
 64 72.2 56.3 84.5
 63 40.8 30.1 45.1

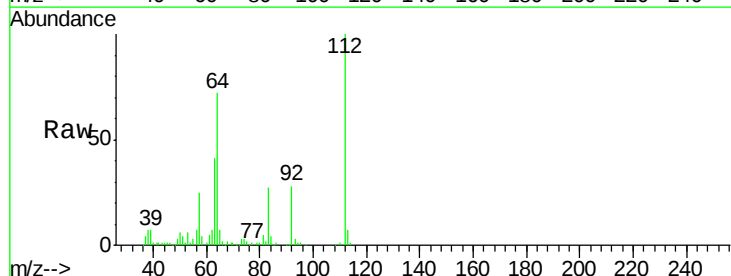

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

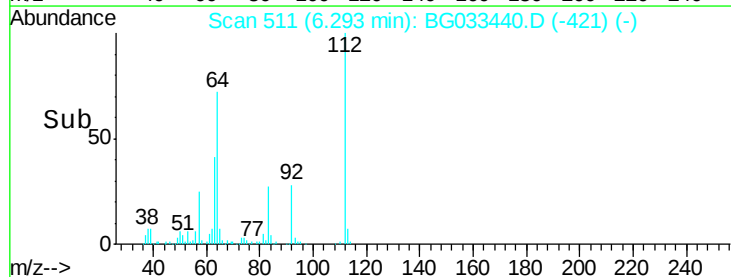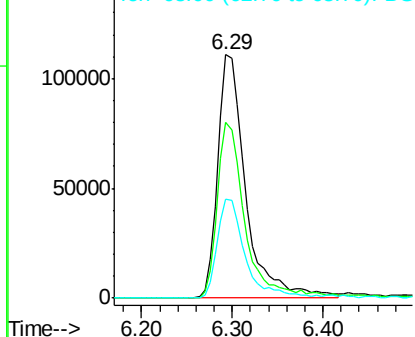

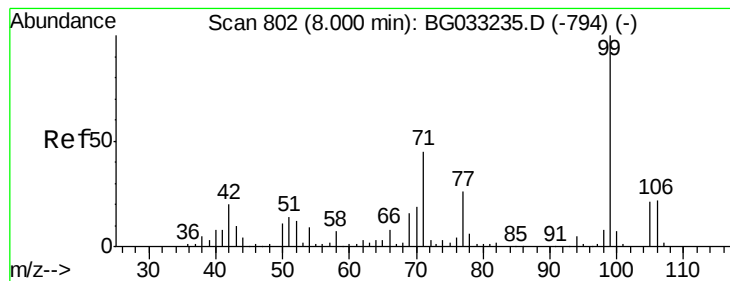

#7

Phenol-d6

Concen: 133.615 ng

RT: 7.99 min Scan# 799

Delta R.T. 0.01 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44

Instrument :

BNA_G

ClientSampleId :

PB107742BL


Tot Ion: 99 Resp: 340660

Ion Ratio Lower Upper




99 100

42 18.6 14.1 21.1

71 40.3 26.1 39.1#

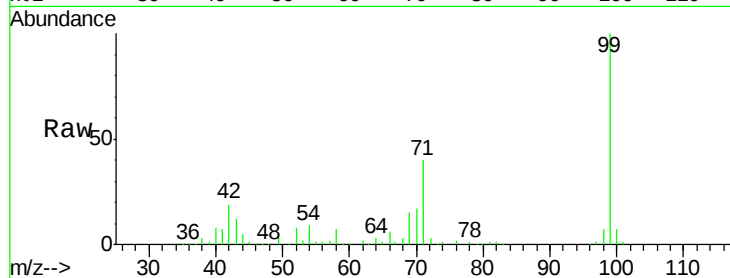

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

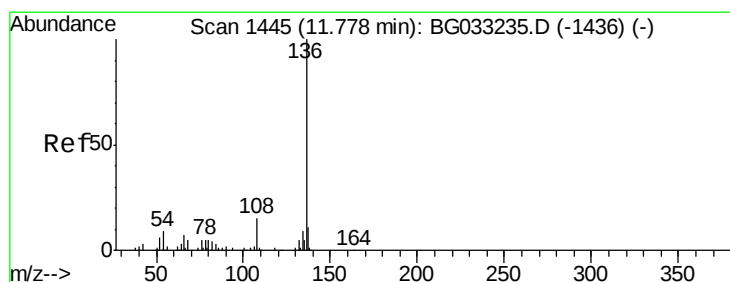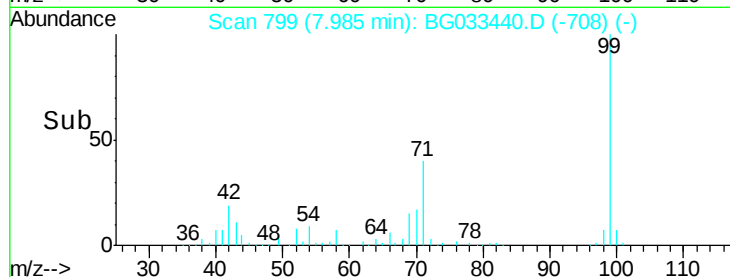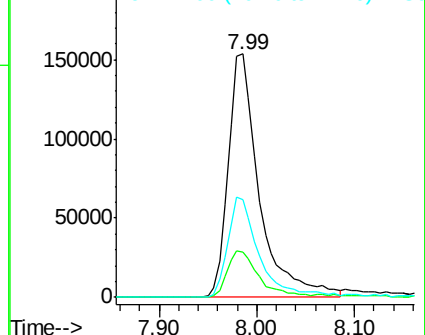

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.75 min Scan# 1440

Delta R.T. -0.01 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44

Tgt Ion: 136 Resp: 111667


Ion Ratio Lower Upper

136 100



137 9.4 9.2 13.8


54 10.9 10.3 15.5

68 5.0 4.5 6.7

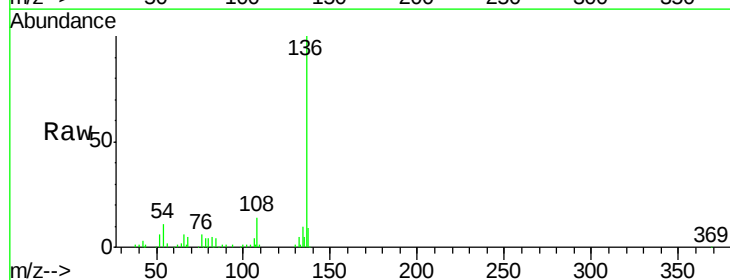

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

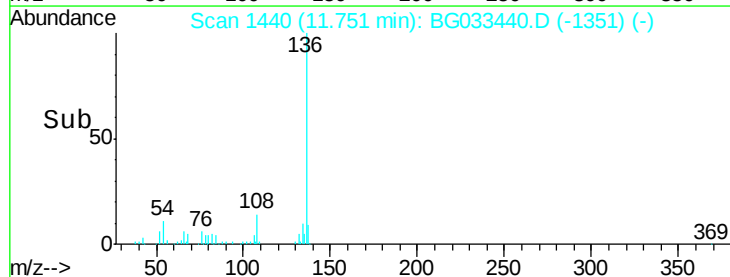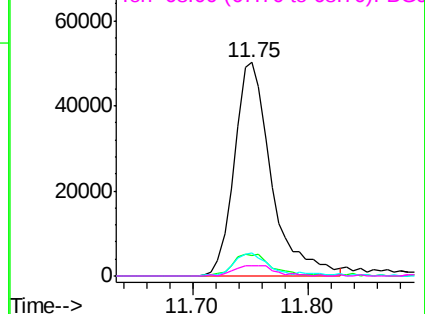

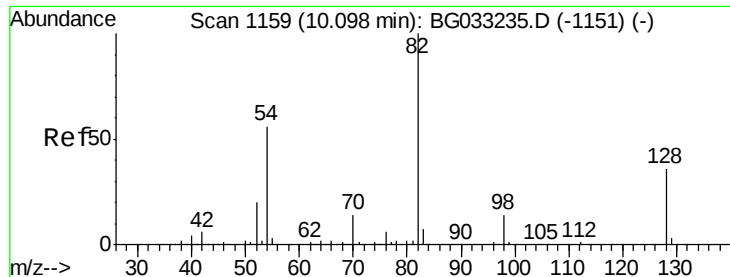

#23

Nitrobenzene-d5

Concen: 86.742 ng

RT: 10.07 min Scan# 1153

Delta R.T. -0.01 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44

Instrument :

BNA_G

ClientSampleId :

PB107742BL


Tot Ion: 82 Resp: 210827

Ion Ratio Lower Upper




82 100

128 36.3 29.7 44.5

54 54.5 43.1 64.7

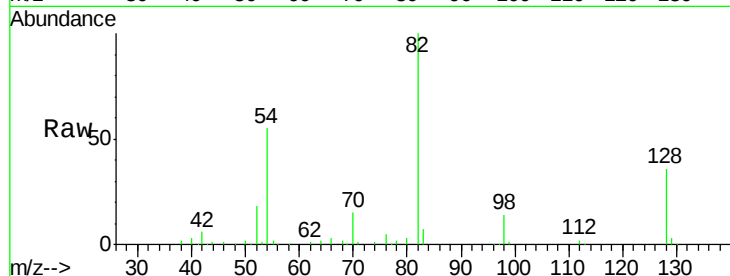

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

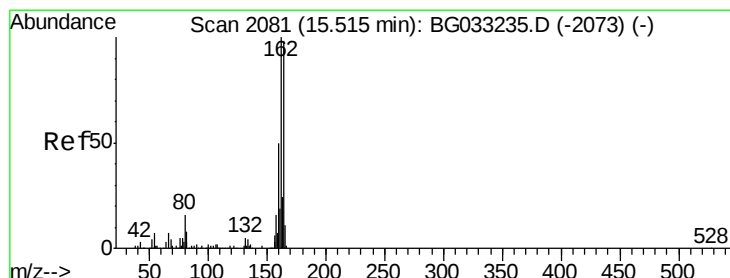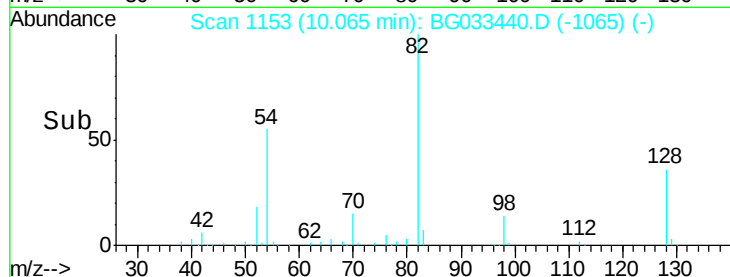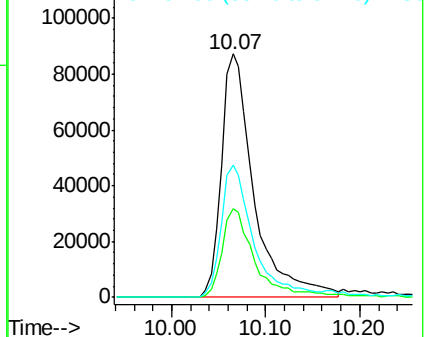

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.48 min Scan# 2075

Delta R.T. -0.01 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44


Tgt Ion: 164 Resp: 92792

Ion Ratio Lower Upper



164 100

162 96.6 78.8 118.2

160 46.8 35.4 53.0

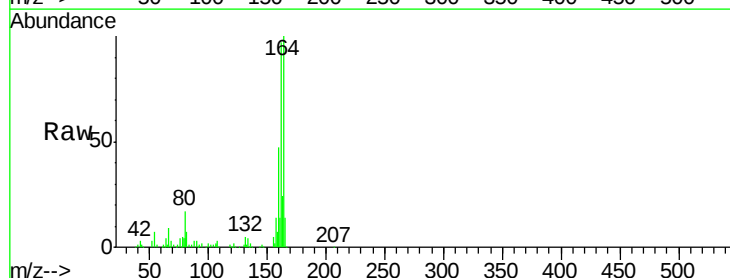

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC



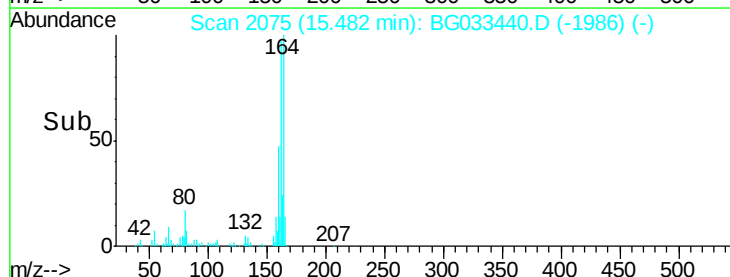
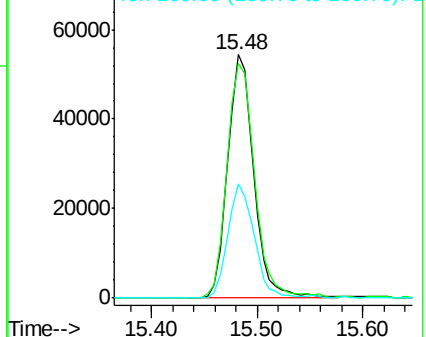




#41
 2,4,6-Tribromophenol
 Concen: 77.018 ng
 RT: 16.96 min Scan# 2326
 Delta R.T. -0.00 min
 Lab File: BG033440.D
 Acq: 30 Mar 2018 3:44




Instrument :
 BNA_G
 ClientSampleId :
 PB107742BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	98.8	77.0	115.6
141	35.0	25.2	37.8

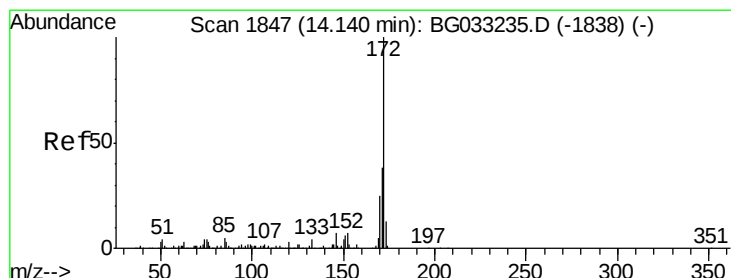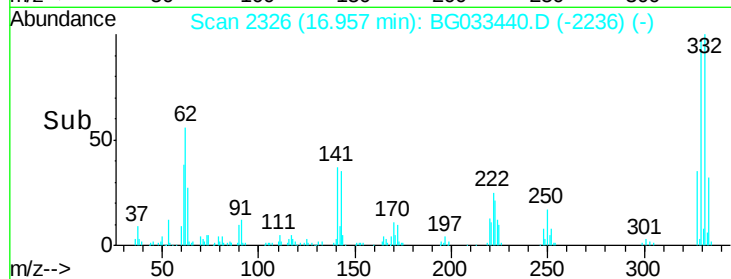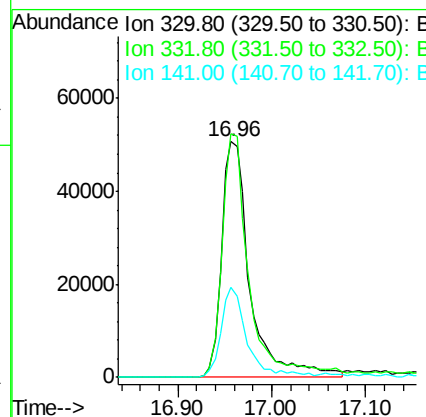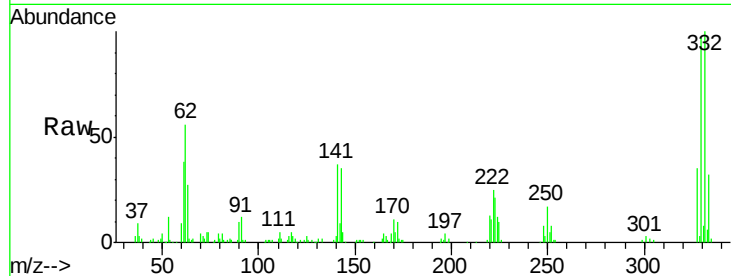

#44
 2-Fluorobiphenyl
 Concen: 86.052 ng
 RT: 14.11 min Scan# 1842
 Delta R.T. -0.00 min
 Lab File: BG033440.D
 Acq: 30 Mar 2018 3:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	30.0	45.0
170	25.0	19.5	29.3


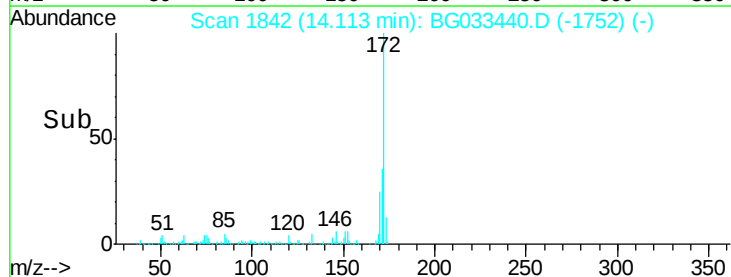
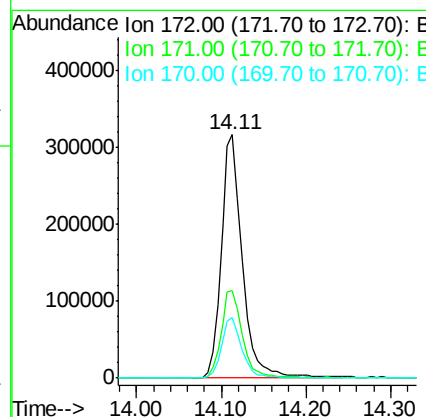
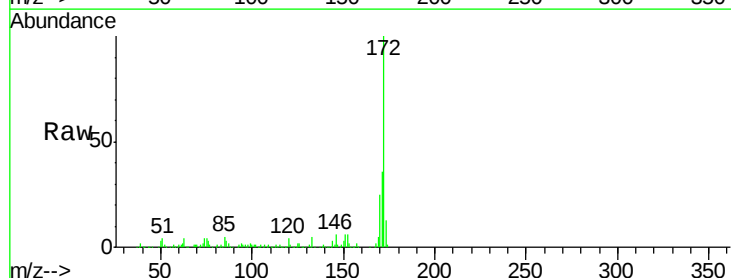


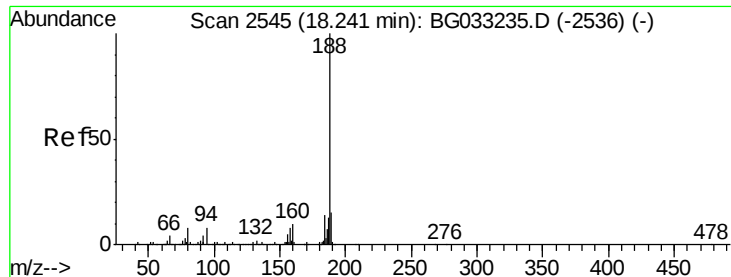

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.21 min Scan# 2540
Delta R.T. -0.00 min
Lab File: BG033440.D
Acq: 30 Mar 2018 3:44




Instrument :
BNA_G
ClientSampleId :
PB107742BL


Tot Ion:188 Resp: 288354
Ion Ratio Lower Upper
188 100
94 7.1 6.9 10.3
80 9.0 7.7 11.5

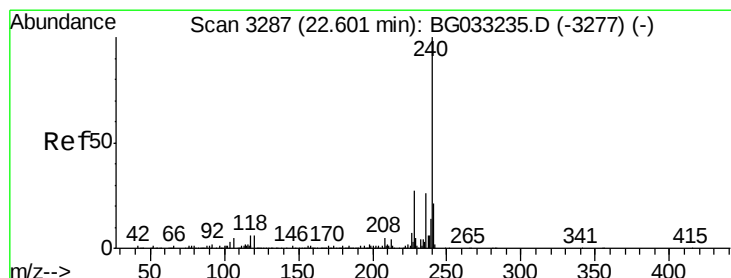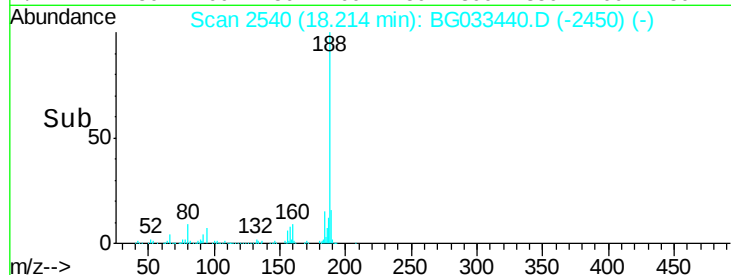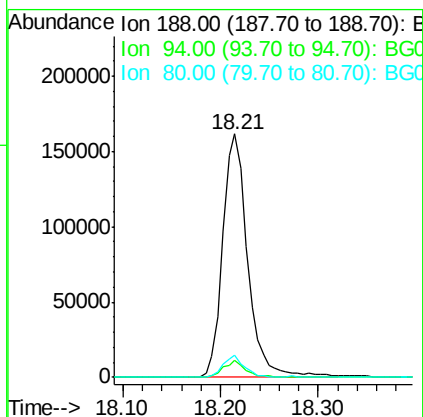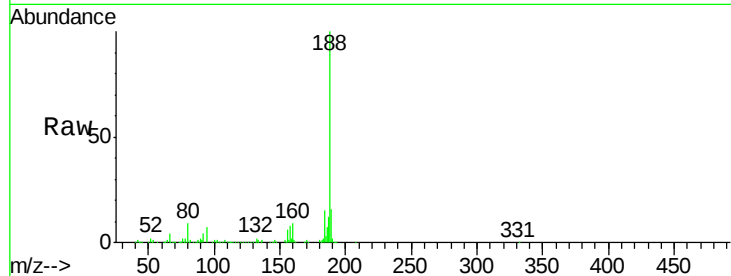

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.56 min Scan# 3280
Delta R.T. -0.00 min
Lab File: BG033440.D
Acq: 30 Mar 2018 3:44

Tgt Ion:240 Resp: 331522
Ion Ratio Lower Upper
240 100
120 7.1 6.8 10.2
236 27.9 20.9 31.3

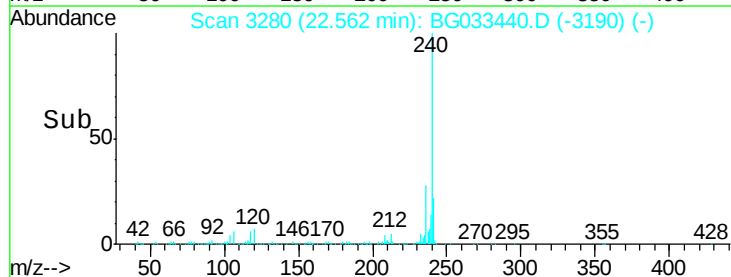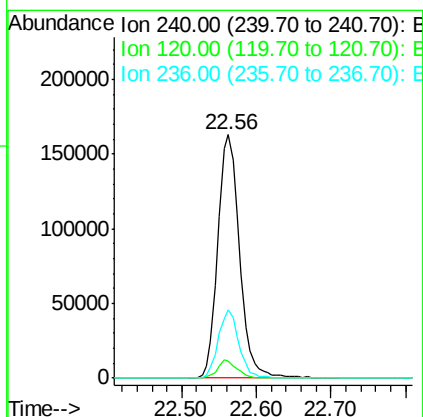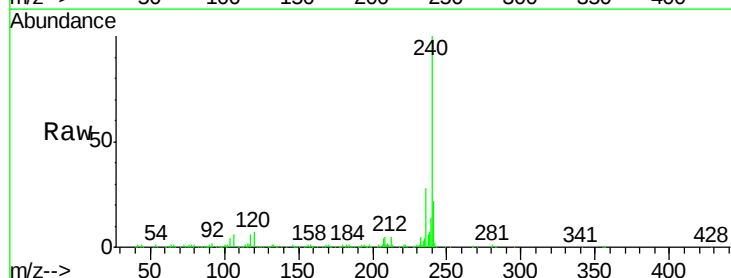

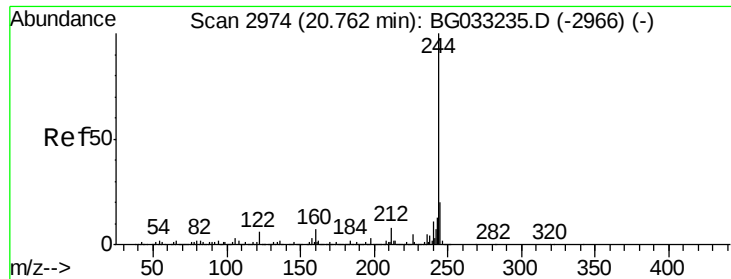

#78

Terphenyl-d14

Concen: 85.663 ng

RT: 20.73 min Scan# 2969

Delta R.T. -0.00 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44

Instrument :

BNA_G

ClientSampleId :

PB107742BL


Tot Ion:244 Resp: 1327933

Ion Ratio Lower Upper

244 100

212 8.6 5.8 8.8



122 6.9 7.0 10.4#

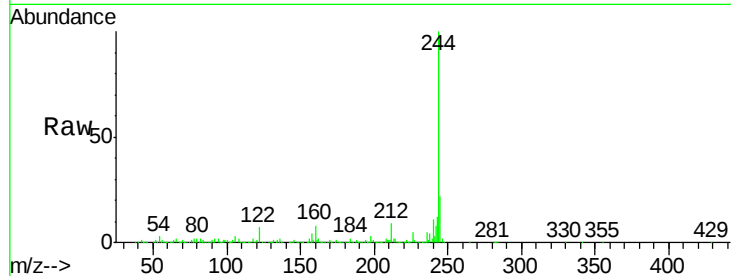

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

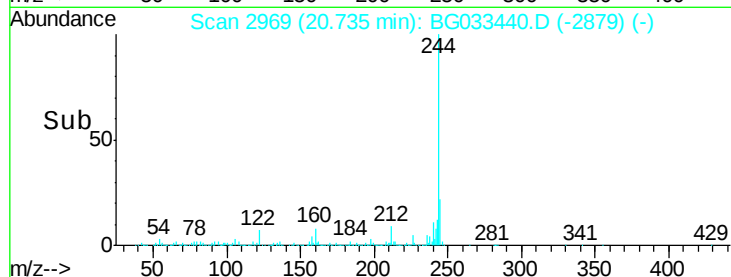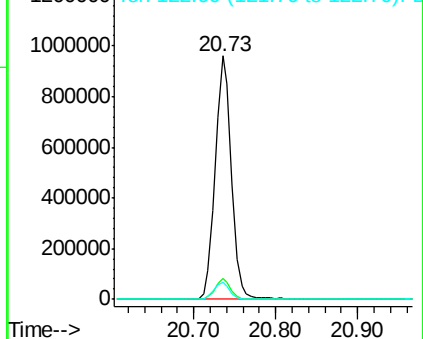

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.33 min Scan# 3921

Delta R.T. -0.01 min

Lab File: BG033440.D

Acq: 30 Mar 2018 3:44


Tgt Ion:264 Resp: 352567

Ion Ratio Lower Upper

264 100

260 23.7 17.4 26.0

265 20.3 17.7 26.5

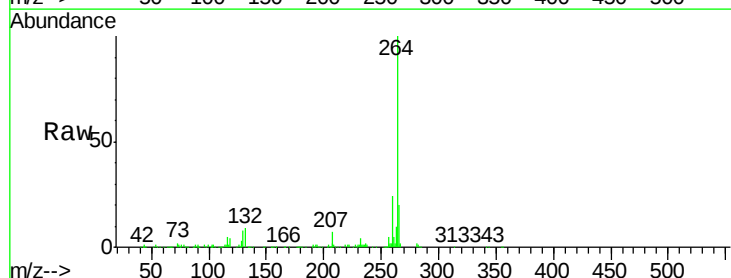

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

