


Data Path : Z:\HPCHEM1\BNA G\DATA\BG032918\
 Data File : BG033423.D
 Acq On : 29 Mar 2018 17:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 28 18:34:58 2018

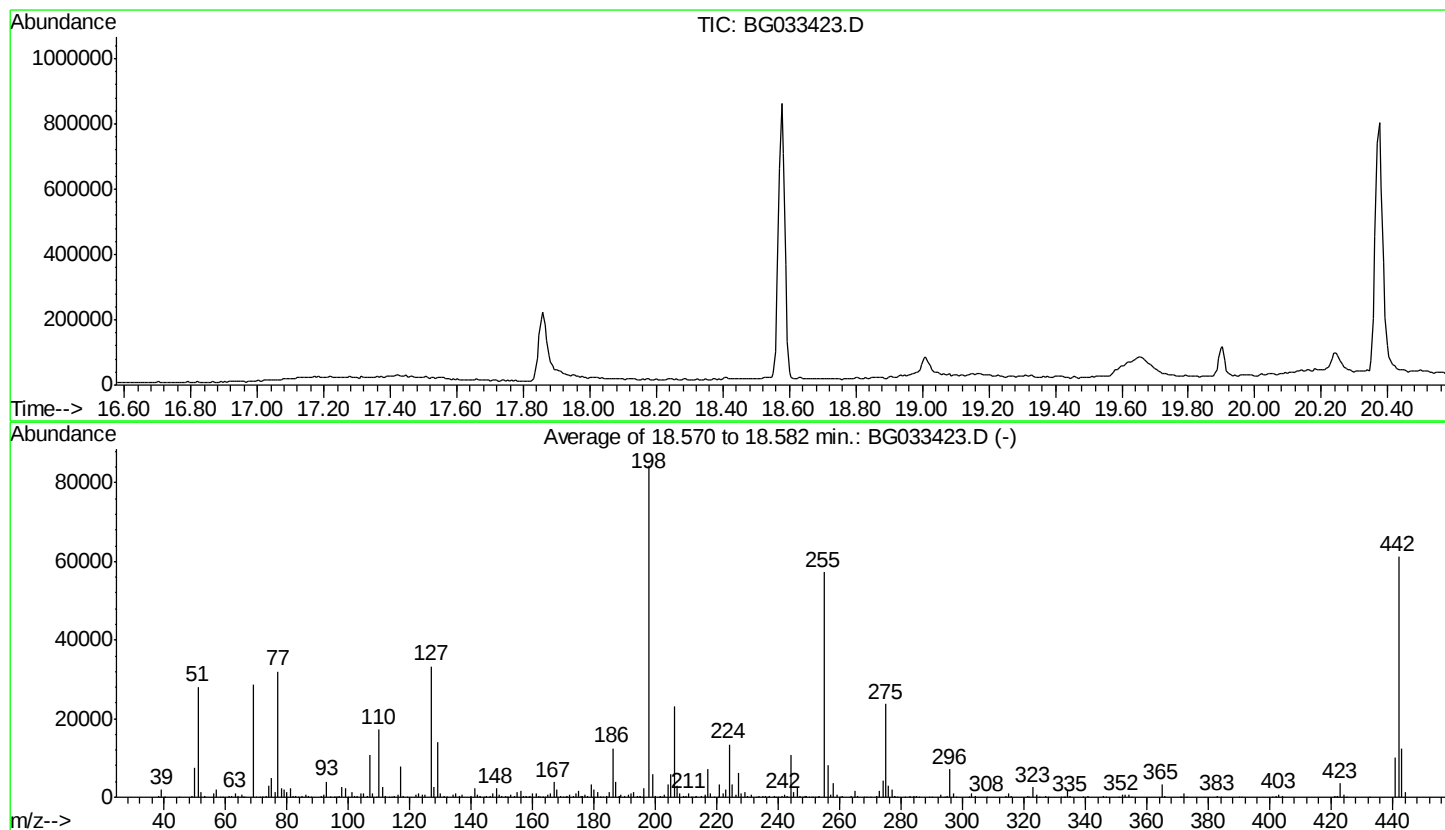

AutoFind: Scans 2601, 2602, 2603; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	28024	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.8	28557	PASS
70	69	0.00	2	0.3	87	PASS
127	198	10	80	39.4	33256	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84378	PASS
199	198	5	9	6.8	5739	PASS
275	198	10	60	28.2	23770	PASS
365	198	1	100	3.8	3233	PASS
441	443	0.01	100	81.2	10160	PASS
442	198	50	100	72.5	61133	PASS
443	442	15	24	20.5	12506	PASS