


Data Path : Z:\HPCHEM1\BNA G\Data\BG032918\
 Data File : BG033442.D
 Acq On : 30 Mar 2018 6:51
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 10 16:51:36 2018

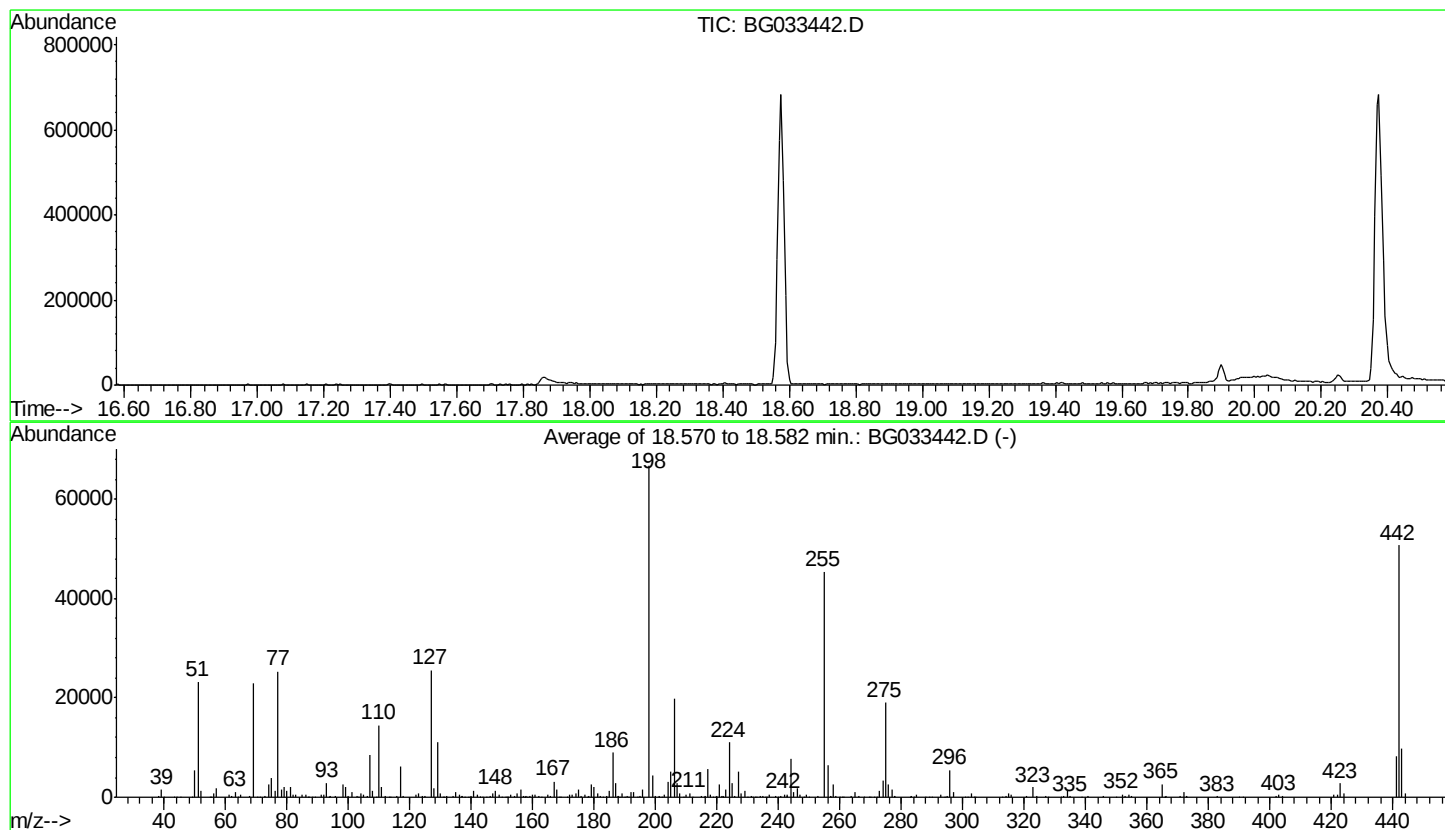

AutoFind: Scans 2601, 2602, 2603; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	23248	PASS
68	69	0.00	2	0.7	153	PASS
69	198	0.00	100	34.2	22821	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	38.4	25616	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66754	PASS
199	198	5	9	6.7	4468	PASS
275	198	10	60	28.5	19034	PASS
365	198	1	100	3.9	2594	PASS
441	443	0.01	100	82.1	8148	PASS
442	198	50	100	76.0	50736	PASS
443	442	15	24	19.6	9924	PASS