
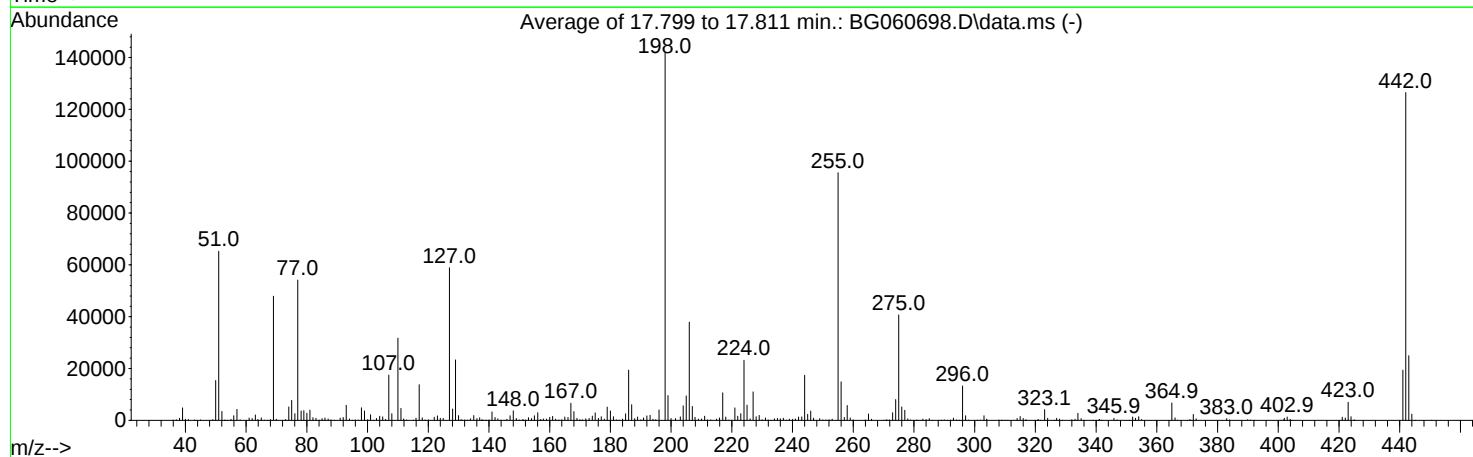


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032924\
Data File : BG060698.D
Acq On : 29 Mar 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 03:12:26 2024

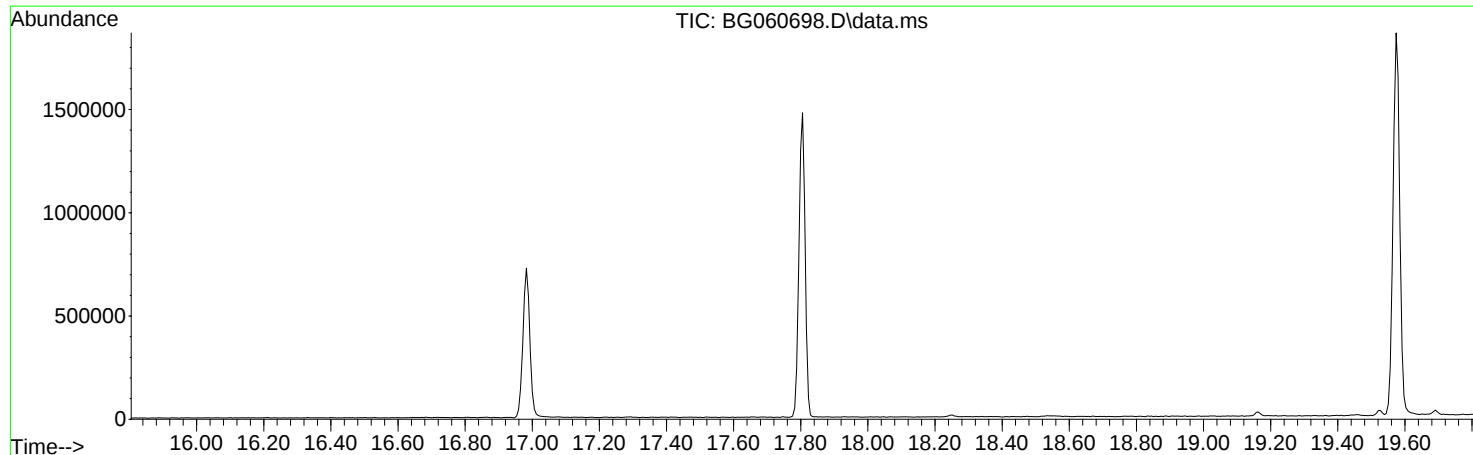




AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	65264	PASS
68	69	0.00	2	0.6	302	PASS
69	198	0.00	100	33.7	47883	PASS
70	69	0.00	2	0.9	435	PASS
127	198	10	80	41.5	58909	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	141936	PASS
199	198	5	9	6.7	9556	PASS
275	198	10	60	28.7	40672	PASS
365	198	1	100	4.8	6749	PASS
441	198	0.01	100	13.7	19378	PASS
442	442	50	100	100.0	126499	PASS
443	442	15	24	19.7	24920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032924\
Data File : BG060698.D
Acq On : 29 Mar 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 30 04:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

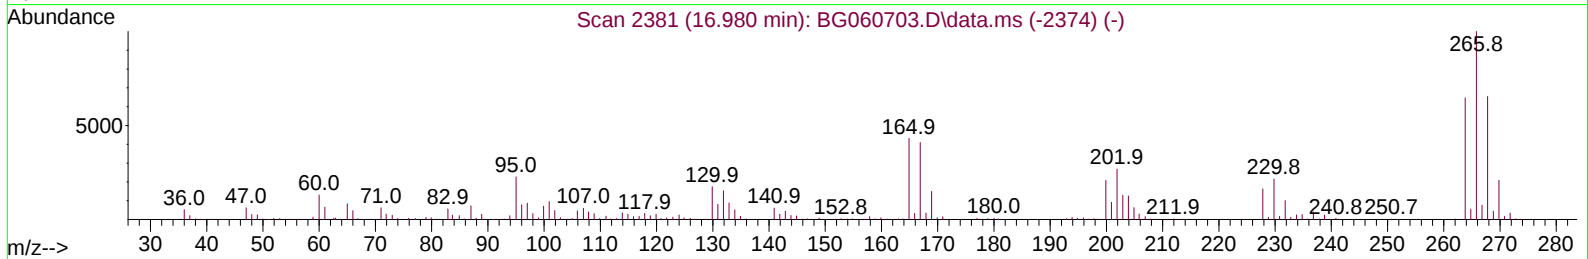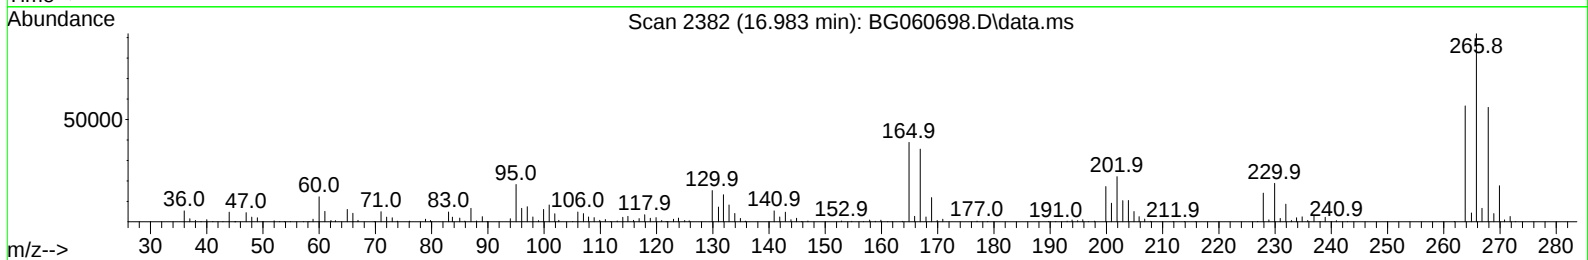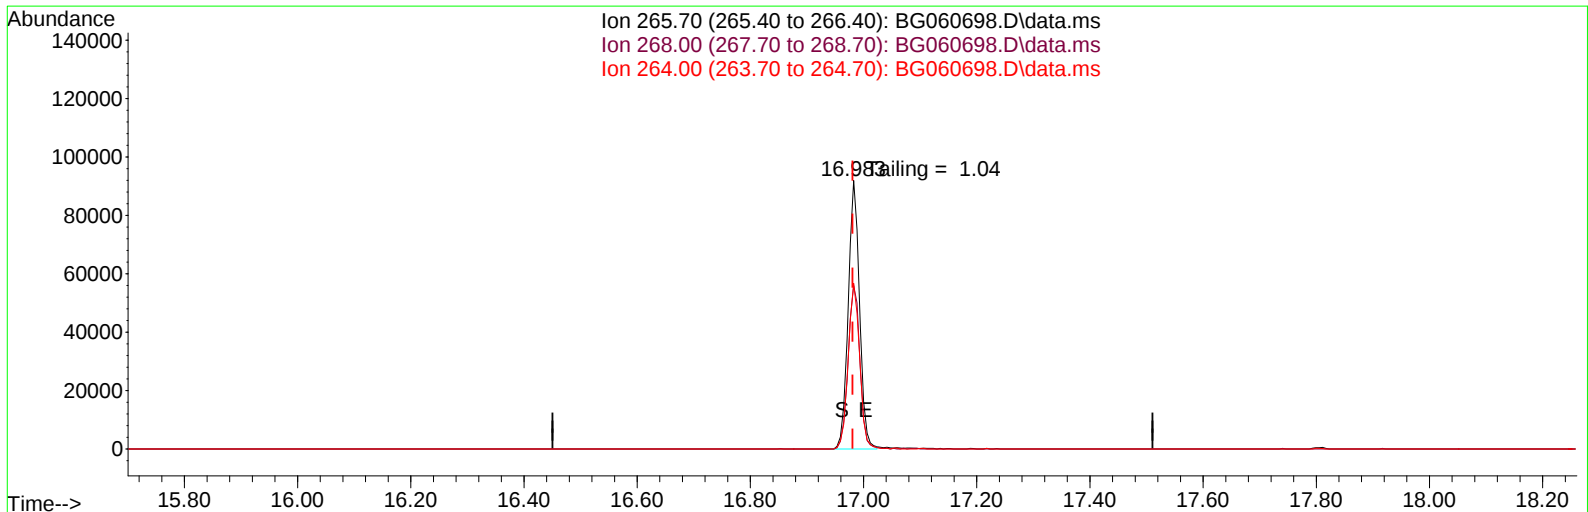

TIC: BG060698.D\data.ms

(70) Pentachlorophenol (C)

16.983min (+ 0.002) 0.00 ng




response 128649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	60.88
264.00	64.70	61.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG032924\
Data File : BG060698.D
Acq On : 29 Mar 2024 10:08
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 30 04:09:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG032924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 30 03:12:26 2024
Response via : Initial Calibration

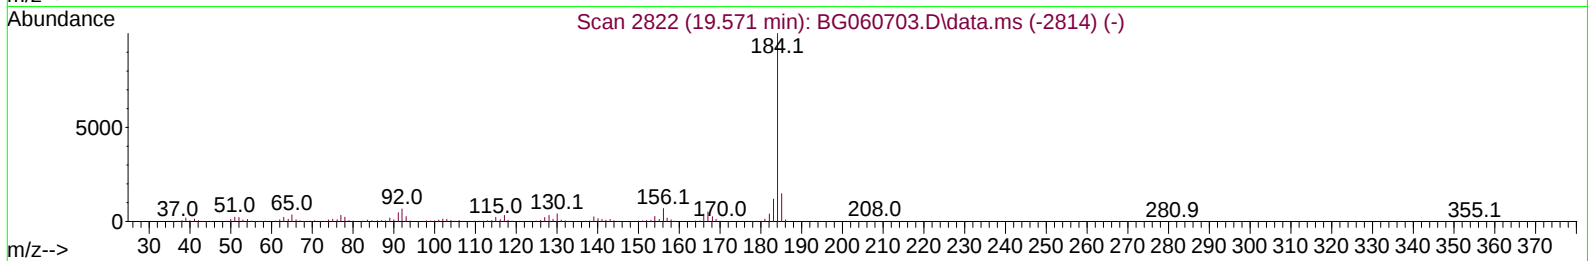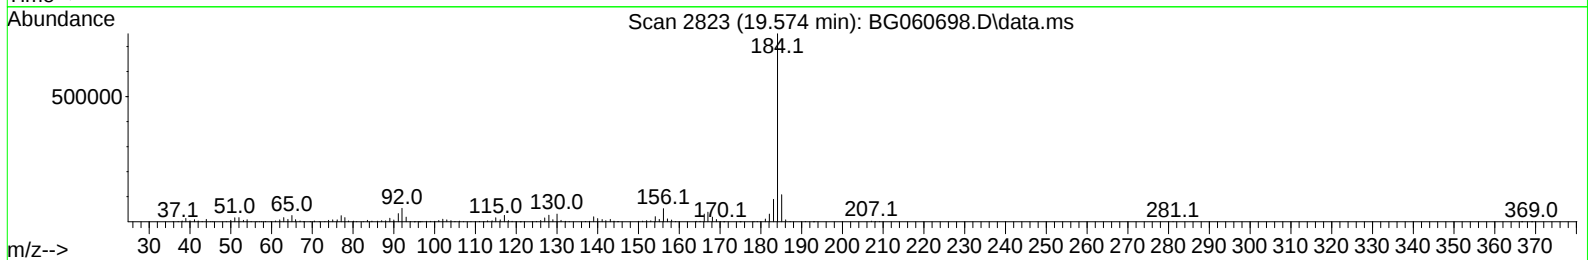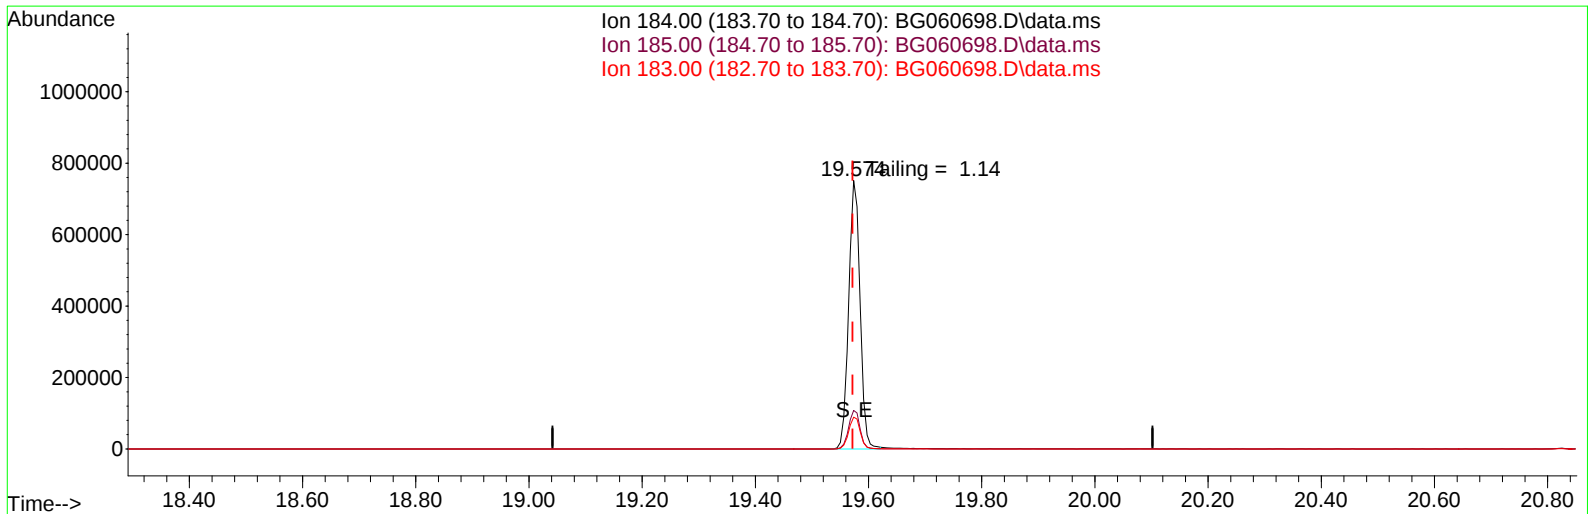

TIC: BG060698.D\data.ms

(77) Benzidine

19.574min (+ 0.002) 116890.72 ng

response 1052671

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.37
183.00	11.90	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/29/2024	BNA_G	<u>BG060698.D</u>
Compound Name	Response	Retention Time
DDT	420391	20.825
DDD	6236	20.432
DDE	110	20.349
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6346	426737	1.49

Instrument :
BNA_G
ClientSampleId :
DFTPP