

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
 Data File : BG021579.D
 Acq On : 30 Mar 2016 13:32
 Operator : UM/SJ
 Sample : H1910-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.979	22	24	25	rVB	706	424	0.15%	0.017%
2	3.144	50	52	53	rVB	663	372	0.13%	0.015%
3	3.173	55	57	60	rVB3	588	416	0.15%	0.017%
4	3.203	60	62	66	rBV3	550	398	0.14%	0.016%
5	3.385	91	93	97	rVV3	436	414	0.15%	0.017%
6	3.596	127	129	131	rBV2	471	315	0.11%	0.013%
7	3.702	144	147	149	rBV	316	306	0.11%	0.012%
8	3.849	169	172	174	rBV2	333	353	0.13%	0.014%
9	4.019	198	201	202	rBV	374	345	0.13%	0.014%
10	4.378	261	262	265	rBV2	302	329	0.12%	0.013%
11	4.519	284	286	289	rVB2	384	390	0.14%	0.016%
12	4.548	289	291	293	rBV	525	317	0.12%	0.013%
13	4.660	308	310	313	rVB2	770	678	0.25%	0.027%
14	4.689	313	315	316	rBV	477	453	0.16%	0.018%
15	4.760	324	327	332	rVB2	526	884	0.32%	0.036%
16	4.854	339	343	344	rBV	264	376	0.14%	0.015%
17	5.018	368	371	372	rVB	432	422	0.15%	0.017%
18	5.124	386	389	390	rBV	216	284	0.10%	0.011%
19	5.183	396	399	401	rBB	382	332	0.12%	0.013%
20	5.318	419	422	425	rBB2	355	515	0.19%	0.021%
21	5.353	426	428	430	rBV2	417	338	0.12%	0.014%
22	5.453	443	445	448	rVB2	497	359	0.13%	0.015%
23	7.374	763	772	780	rBB2	23363	44107	16.01%	1.784%
24	7.633	810	816	823	rBB	22460	38005	13.79%	1.537%
25	8.050	881	887	894	rBB	31547	50932	18.48%	2.060%
26	8.843	1017	1022	1032	rBB	16153	27122	9.84%	1.097%
27	9.219	1080	1086	1095	rBB	32443	55483	20.13%	2.244%
28	9.942	1203	1209	1216	rBB	27975	47484	17.23%	1.920%
29	10.565	1309	1315	1328	rBB	32690	59055	21.43%	2.388%
30	10.852	1358	1364	1371	rBV	48014	83518	30.31%	3.378%
31	11.017	1390	1392	1393	rBV	292	287	0.10%	0.012%
32	11.029	1393	1394	1397	rVB	375	315	0.11%	0.013%
33	13.485	1808	1812	1816	rBB	1663	1843	0.67%	0.075%
34	13.690	1844	1847	1849	rBB	595	530	0.19%	0.021%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
 Data File : BG021579.D
 Acq On : 30 Mar 2016 13:32
 Operator : UM/SJ
 Sample : H1910-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

35	14.066	1906	1911	1920	rBB	92187	132138	47.95%	5.344%
36	14.360	1955	1961	1970	rBV	95258	149120	54.12%	6.031%
37	14.666	2007	2013	2020	rBB2	84158	131823	47.84%	5.331%
38	15.124	2087	2091	2096	rBB2	1684	2555	0.93%	0.103%
39	15.653	2175	2181	2189	rBB	129214	199933	72.56%	8.086%
40	15.782	2199	2203	2211	rBB	36405	53833	19.54%	2.177%
41	15.899	2219	2223	2225	rBB	710	804	0.29%	0.033%
42	16.375	2300	2304	2305	rBB	356	361	0.13%	0.015%
43	16.493	2321	2324	2326	rBB	312	365	0.13%	0.015%
44	16.875	2387	2389	2392	rBB	494	444	0.16%	0.018%
45	17.409	2473	2480	2486	rBV2	121188	177755	64.51%	7.189%
46	17.503	2490	2496	2505	rVV2	148265	225969	82.00%	9.139%
47	17.568	2505	2507	2511	rVB	375	468	0.17%	0.019%
48	18.349	2637	2640	2644	rBB2	499	645	0.23%	0.026%
49	18.402	2645	2649	2651	rBV	286	468	0.17%	0.019%
50	18.602	2681	2683	2685	rBV	230	286	0.10%	0.012%
51	18.831	2719	2722	2723	rBV	490	458	0.17%	0.019%
52	19.066	2760	2762	2764	rBV	452	468	0.17%	0.019%
53	19.131	2770	2773	2774	rBV	409	369	0.13%	0.015%
54	19.389	2815	2817	2818	rBV	431	433	0.16%	0.018%
55	19.431	2820	2824	2827	rBV	1511	1921	0.70%	0.078%
56	19.507	2835	2837	2839	rBV	491	356	0.13%	0.014%
57	19.530	2839	2841	2843	rVB	454	419	0.15%	0.017%
58	19.554	2843	2845	2846	rVB	559	364	0.13%	0.015%
59	19.572	2846	2848	2850	rBV	786	721	0.26%	0.029%
60	19.630	2857	2858	2860	rBV	672	566	0.21%	0.023%
61	19.783	2877	2884	2891	rBV2	188643	275558	100.00%	11.144%
62	19.883	2900	2901	2904	rBV2	522	553	0.20%	0.022%
63	19.924	2906	2908	2910	rBV2	487	310	0.11%	0.013%
64	19.983	2916	2918	2919	rBV	631	458	0.17%	0.019%
65	20.077	2931	2934	2935	rBV2	428	391	0.14%	0.016%
66	20.118	2939	2941	2942	rVB	653	304	0.11%	0.012%
67	20.136	2942	2944	2946	rBV2	852	691	0.25%	0.028%
68	20.183	2950	2952	2954	rVB2	866	538	0.20%	0.022%
69	20.200	2954	2955	2956	rVB	840	296	0.11%	0.012%
70	20.218	2956	2958	2960	rBV2	930	864	0.31%	0.035%
71	20.259	2963	2965	2966	rVB2	891	424	0.15%	0.017%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
 Data File : BG021579.D
 Acq On : 30 Mar 2016 13:32
 Operator : UM/SJ
 Sample : H1910-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
 Title : SVOA CALIBRATION

72	20.271	2966	2967	2968	rBV	804	474	0.17%	0.019%
73	20.371	2982	2984	2986	rBV3	738	768	0.28%	0.031%
74	20.441	2994	2996	2997	rVB2	690	384	0.14%	0.016%
75	20.471	2999	3001	3002	rVV2	1185	1008	0.37%	0.041%
76	20.512	3005	3008	3011	rBV4	1087	1457	0.53%	0.059%
77	20.547	3011	3014	3015	rBV3	592	615	0.22%	0.025%
78	20.565	3015	3017	3021	rVV3	1008	1267	0.46%	0.051%
79	20.635	3027	3029	3032	rVB2	924	672	0.24%	0.027%
80	21.105	3107	3109	3111	rBV2	1093	929	0.34%	0.038%
81	21.311	3142	3144	3145	rBV2	1199	595	0.22%	0.024%
82	21.469	3169	3171	3173	rBV3	1392	1196	0.43%	0.048%
83	21.516	3175	3179	3184	rBV6	3405	5664	2.06%	0.229%
84	21.663	3198	3204	3213	rVB	133672	211564	76.78%	8.556%
85	22.127	3281	3283	3284	rBV2	1629	762	0.28%	0.031%
86	23.872	3577	3580	3581	rBV3	2169	2525	0.92%	0.102%
87	24.648	3702	3712	3722	rBV	92405	248852	90.31%	10.064%
88	24.871	3735	3750	3760	rBV2	72658	205740	74.66%	8.321%
89	26.270	3986	3988	3990	rBV2	1861	1630	0.59%	0.066%
90	26.669	4054	4056	4057	rBV2	1643	803	0.29%	0.032%
91	27.198	4144	4146	4147	rBV2	2190	1880	0.68%	0.076%
92	27.216	4147	4149	4150	rVV2	2461	1873	0.68%	0.076%
93	29.824	4591	4593	4595	rBV2	1687	824	0.30%	0.033%


Sum of corrected areas: 2472612

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
Data File : BG021579.D
Acq On : 30 Mar 2016 13:32
Operator : UM/SJ
Sample : H1910-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG5

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

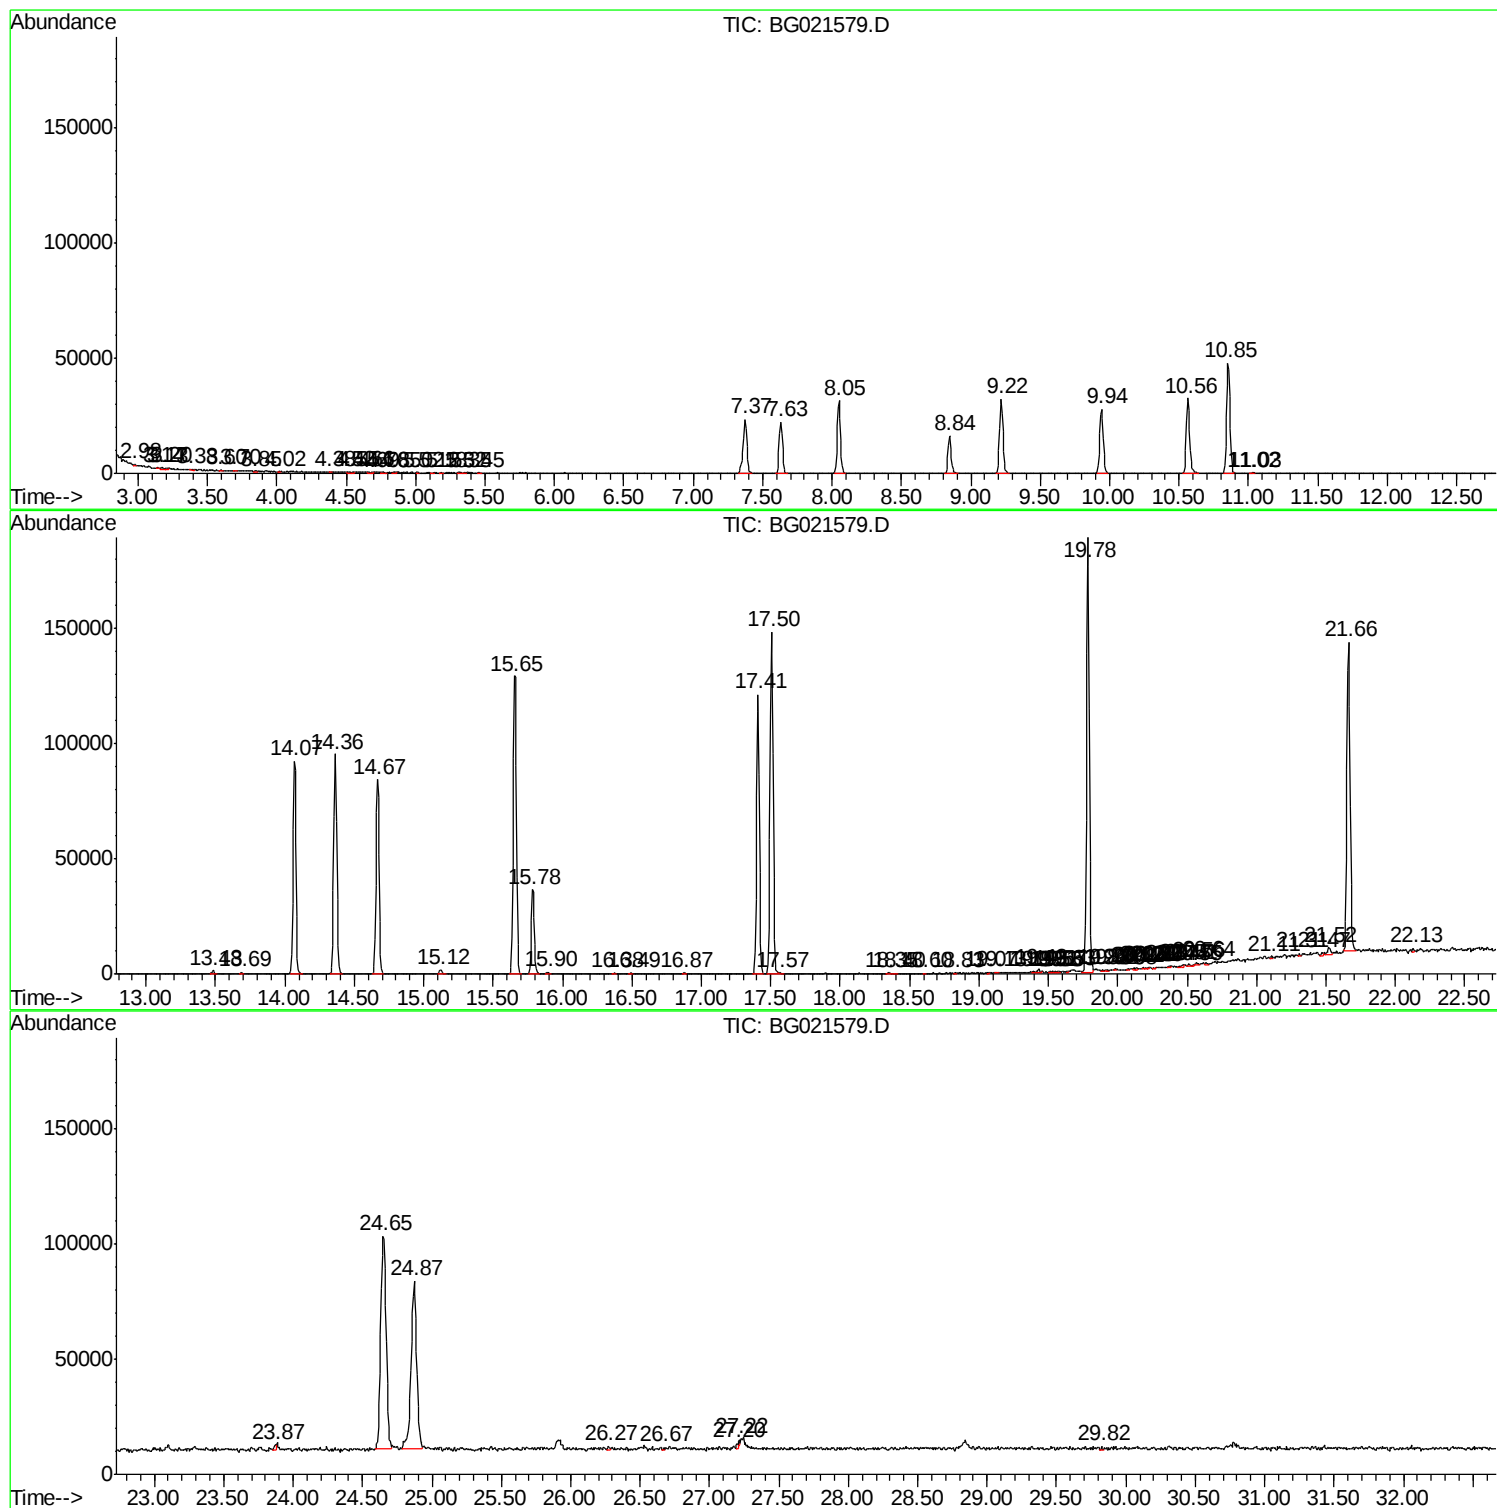

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
Data File : BG021579.D
Acq On : 30 Mar 2016 13:32
Operator : UM/SJ
Sample : H1910-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG5

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG033016\
Data File : BG021579.D
Acq On : 30 Mar 2016 13:32
Operator : UM/SJ
Sample : H1910-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AG5

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc