

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG033017\
 Data File : BG026509.D
 Acq On : 30 Mar 2017 23:21
 Operator : SJ/MA
 Sample : I2448-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 31 01:09:22 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 01:08:45 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 G9YC0

Manual Integrations
 APPROVED

mohammad
 3/31/2017 10:31:19 AM

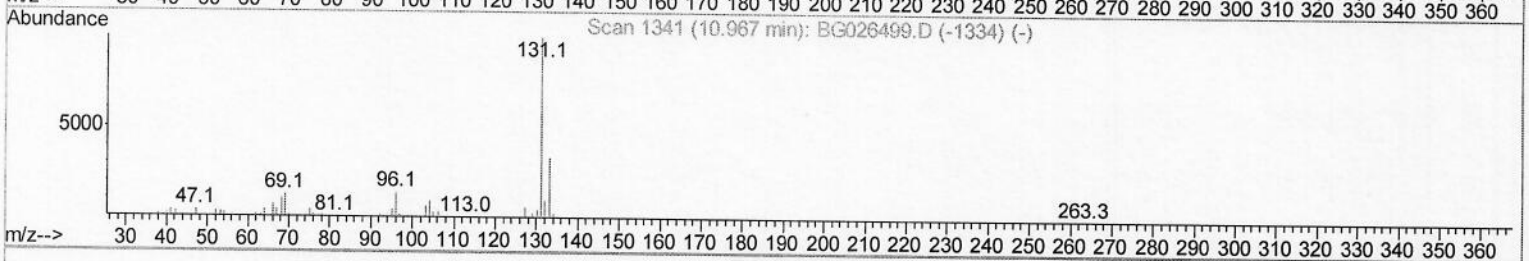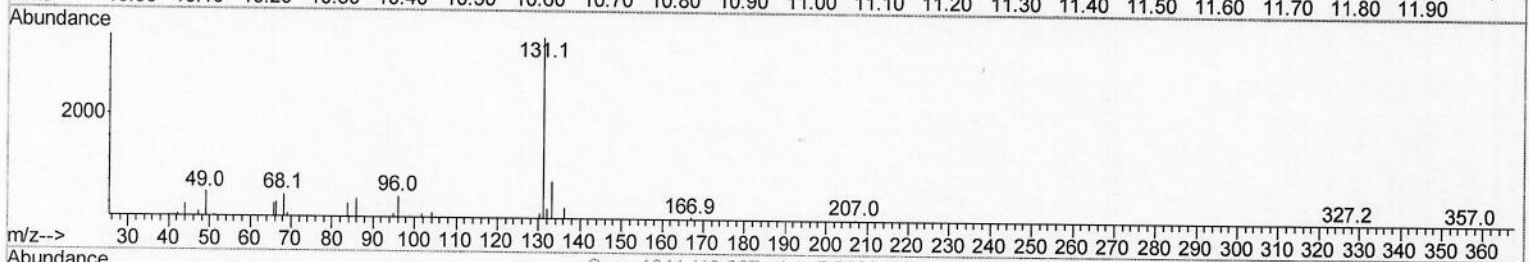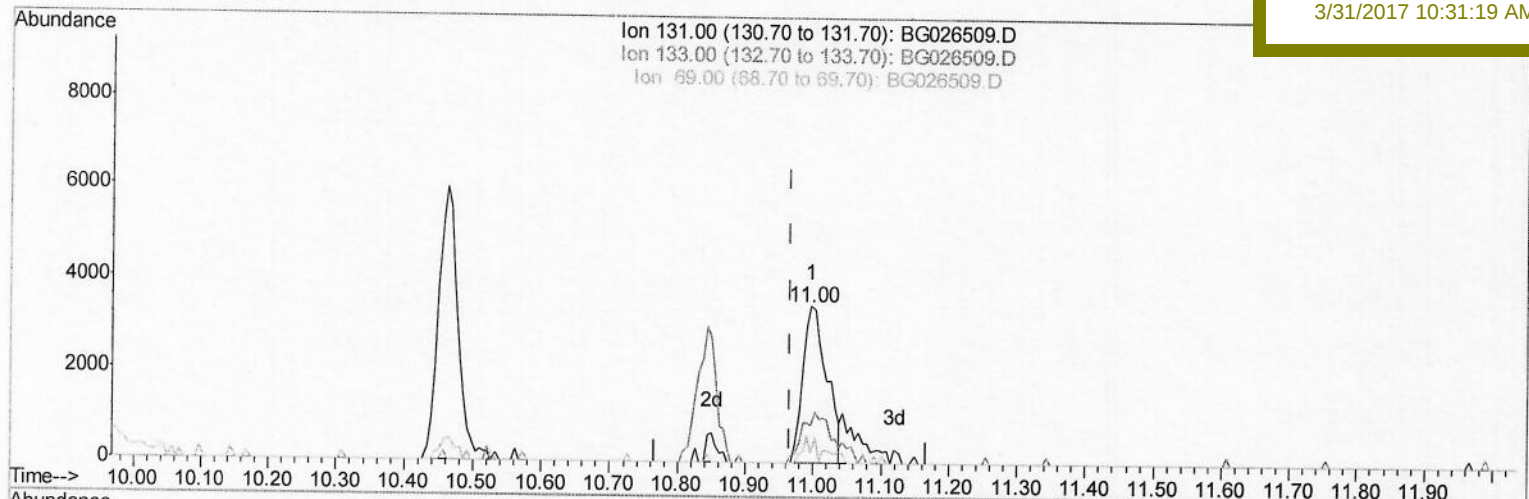

TIC: BG026509.D

(29) 4-Chloroaniline-d4 (S)
 10.996min (+0.030) 0.72ng/ul
 response 8494

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	24.21#
69.00	16.20	6.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG033017\
 Data File : BG026509.D
 Acq On : 30 Mar 2017 23:21
 Operator : SJ/MA
 Sample : I2448-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 31 01:09:22 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 01:08:45 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 G9YC0

Manual Integrations
 APPROVED

mohammad
 3/31/2017 10:31:19 AM

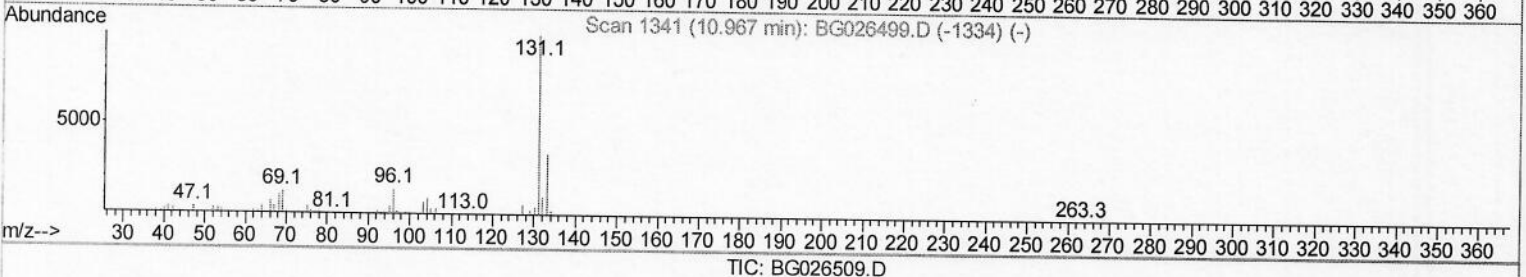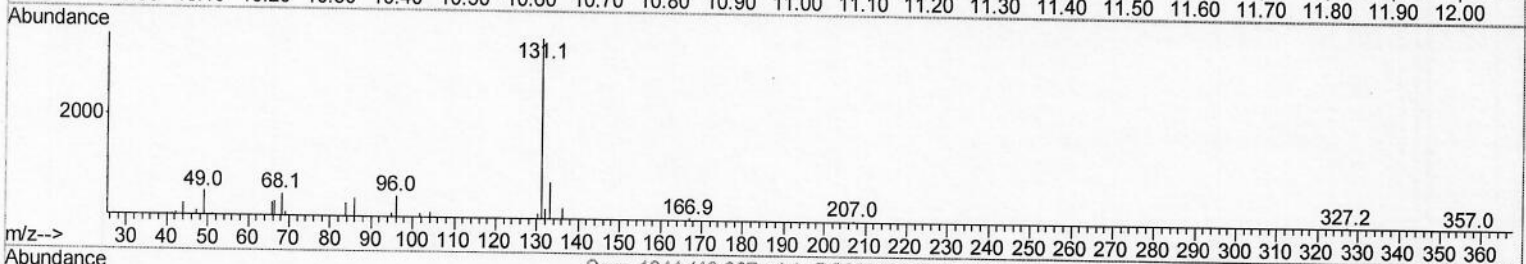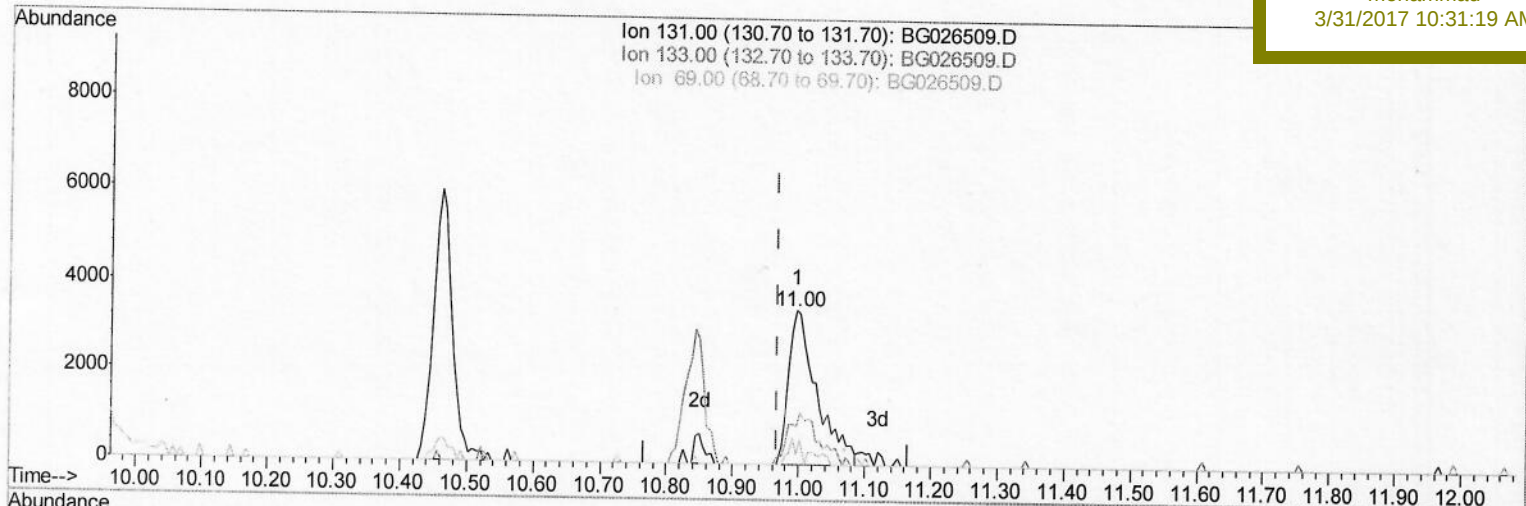

(29) 4-Chloroaniline-d4 (S)

10.996min (+0.030) 0.87ng/ul m

response 10235

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	24.21#
69.00	16.20	6.60#
0.00	0.00	0.00

S.J
03/31/2017

Data Path : Z:\HPCHEM1\BNA G\DATA\BG033017\
 Data File : BG026509.D
 Acq On : 30 Mar 2017 23:21
 Operator : SJ/MA
 Sample : I2448-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 31 01:23:34 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 01:08:45 2017
 Response via : Initial Calibration

Instrument :
 BNA_G
 Client Sample ID :
 G9YC0

Manual Integrations
 APPROVED

mohammad
 3/31/2017 10:31:19 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	185817	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	768361	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.65	164	445398	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.38	188	1068795	20.00	ng/ul	0.00
77) Chrysene-d12	21.63	240	1307354	20.00	ng/ul	0.00
85) Perylene-d12	24.80	264	1309484	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	21782	5.61	ng/uL	0.00
5) Phenol-d5	7.21	99	105613	7.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	282050	36.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	361730	29.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	207830	18.85	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	212701	38.73	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	257207	39.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	394658	33.41	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	10235m	0.87	ng/ul	0.03
43) Dimethylphthalate-d6	14.05	166	1325008	38.42	ng/ul	0.00
46) Acenaphthylene-d8	14.34	160	1594988	37.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	42575	6.35	ng/ul	0.00
57) Fluorene-d10	15.63	176	1221737	38.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.75	200	244156	35.53	ng/ul	0.00
70) Anthracene-d10	17.48	188	1905136	39.25	ng/ul	0.00
78) Pyrene-d10	19.76	212	2183164	37.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.59	264	2324874	41.32	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

S.S
 03/31/2017

Data Path : Z:\HPCHEM1\BNA G\DATA\BG033017\
Data File : BG026509.D
Acq On : 30 Mar 2017 23:21
Operator : SJ/MA
Sample : I2448-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Mar 31 01:23:34 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 01:08:45 2017
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
G9YC0

Manual Integrations
APPROVED

mohammad
3/31/2017 10:31:19 AM

