
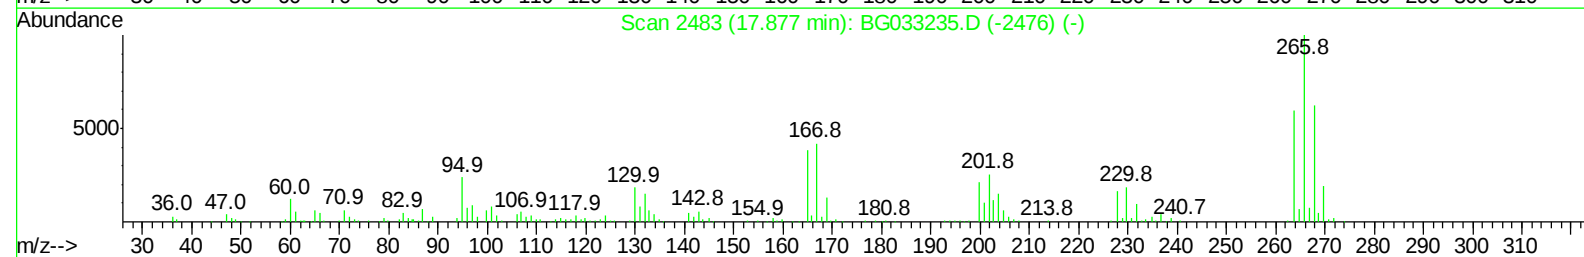
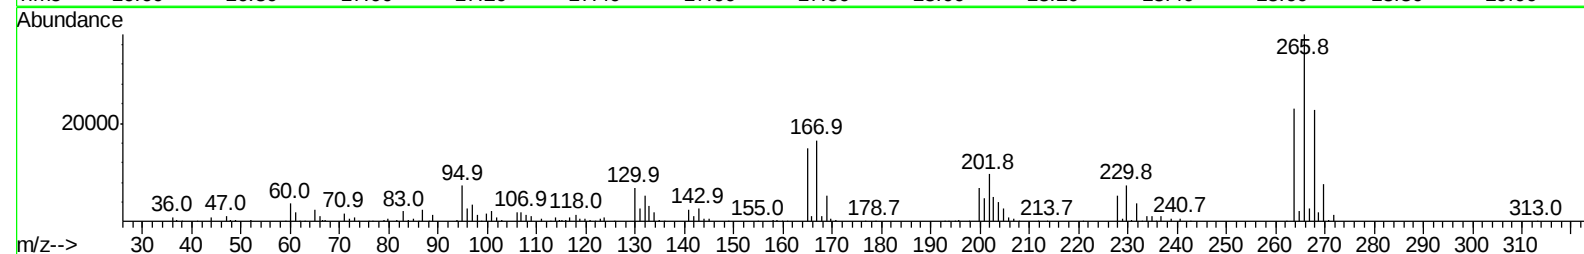


Data Path : U:\HPCHEM1\BNA G\Data\BG033018\
Data File : BG033449.D
Acq On : 30 Mar 2018 15:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:30:44 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

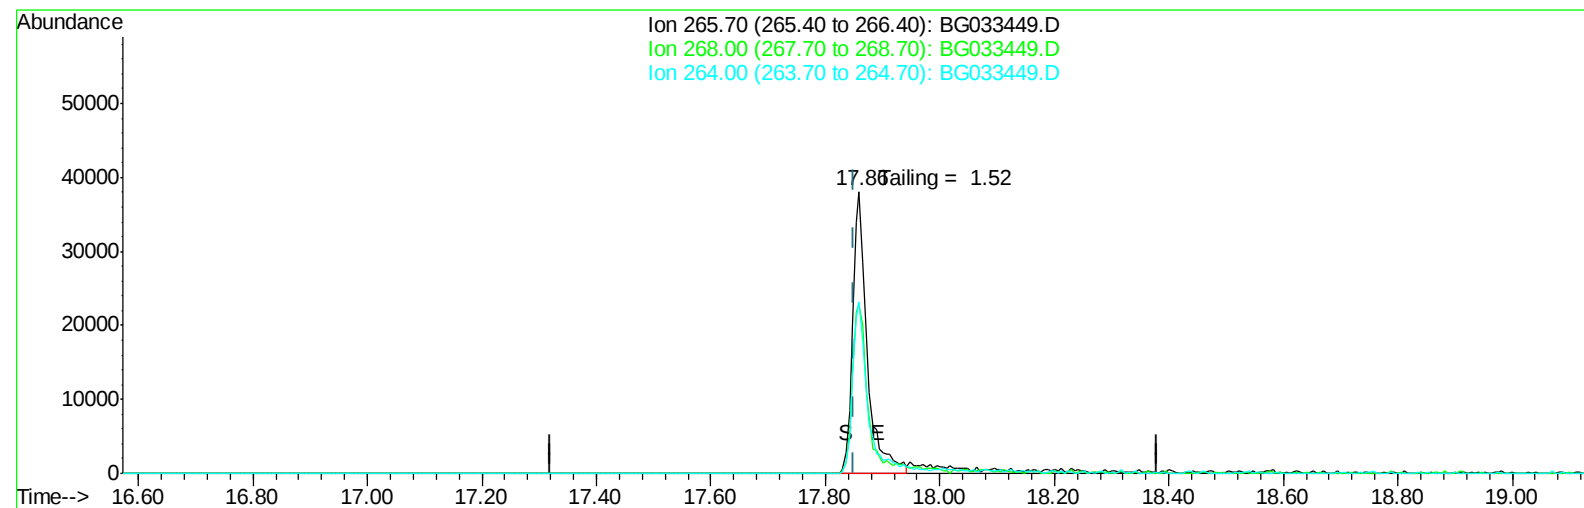

TIC: BG033449.D

(69) Pentachlorophenol (C)




17.860min (+0.009) 18338.68ng

response 67706

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.11
264.00	62.00	60.70
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\Data\BG033018\
Data File : BG033449.D
Acq On : 30 Mar 2018 15:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:30:44 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

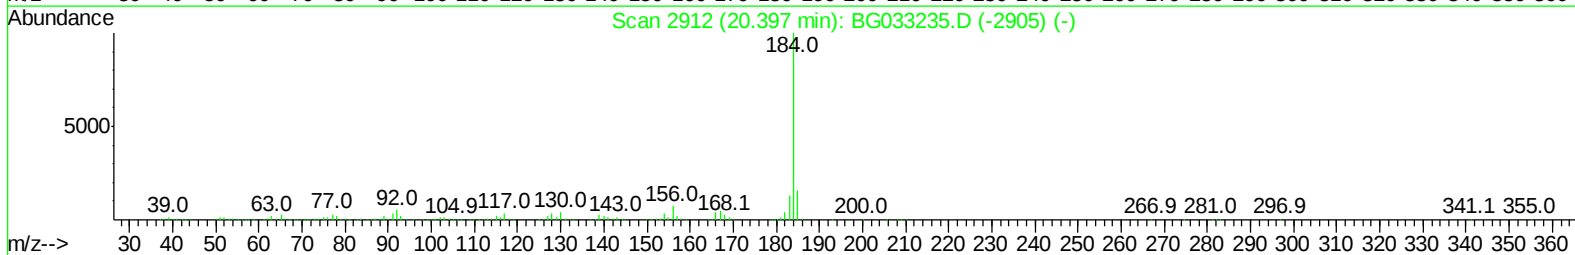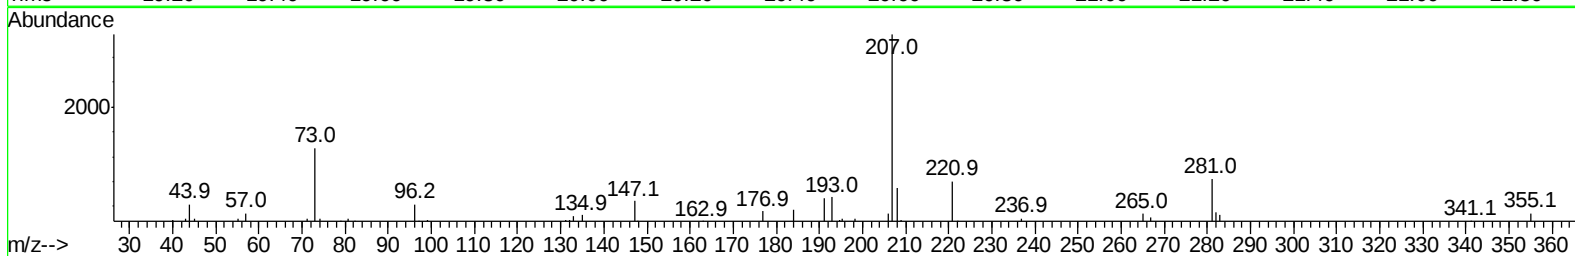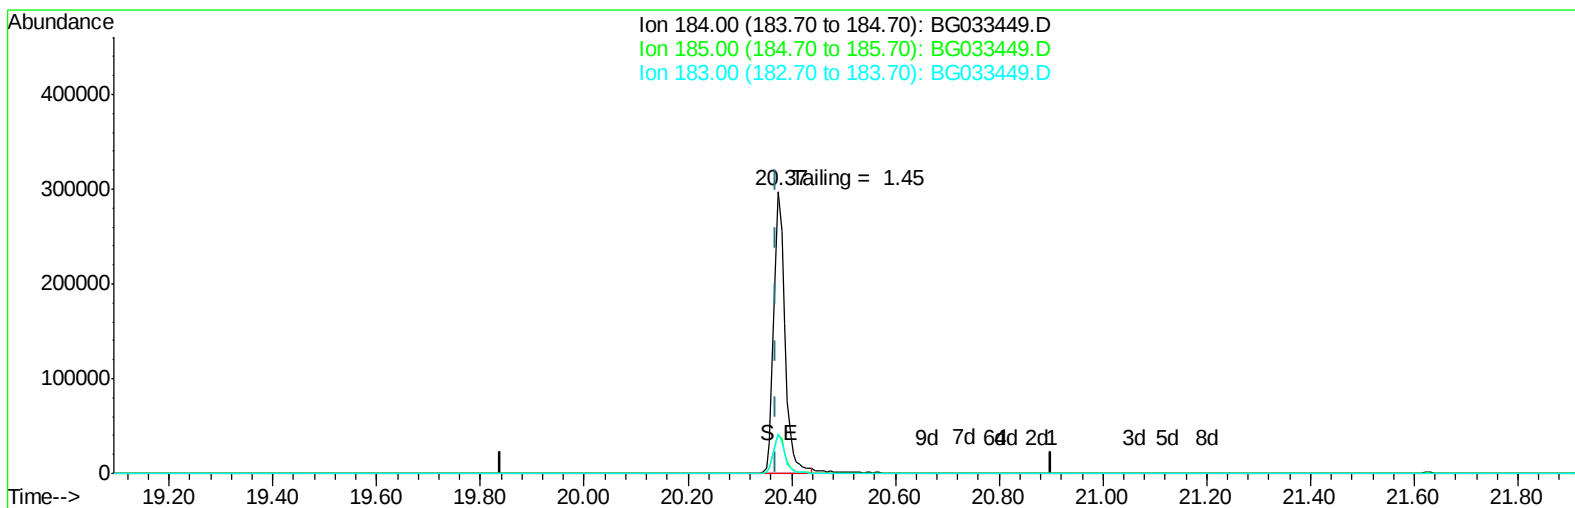

TIC: BG033449.D

(76) Benzidine

20.903min (+0.532) 237.05ng

response 360

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00