
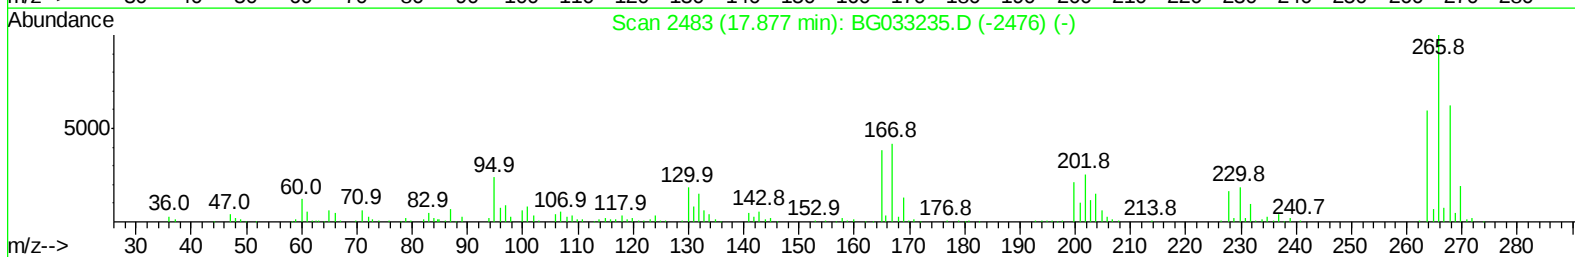
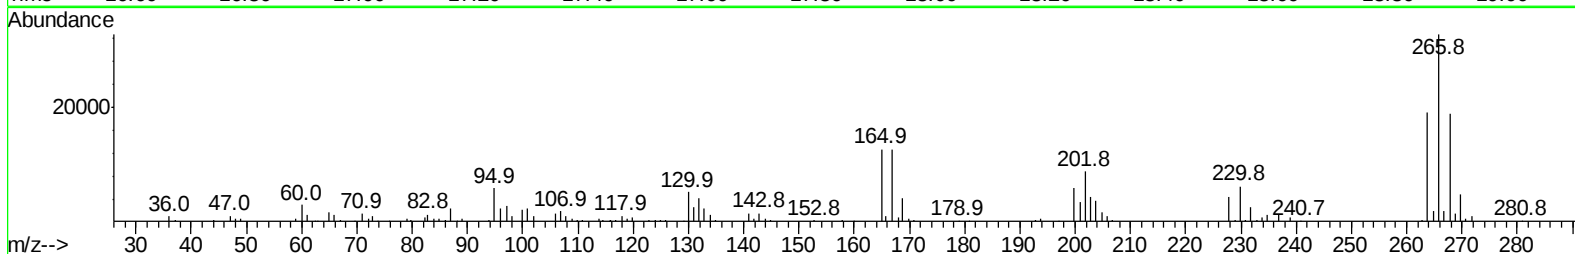


Data Path : U:\HPCHEM1\BNA G\Data\BG033018\
Data File : BG033468.D
Acq On : 31 Mar 2018 4:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:31:44 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

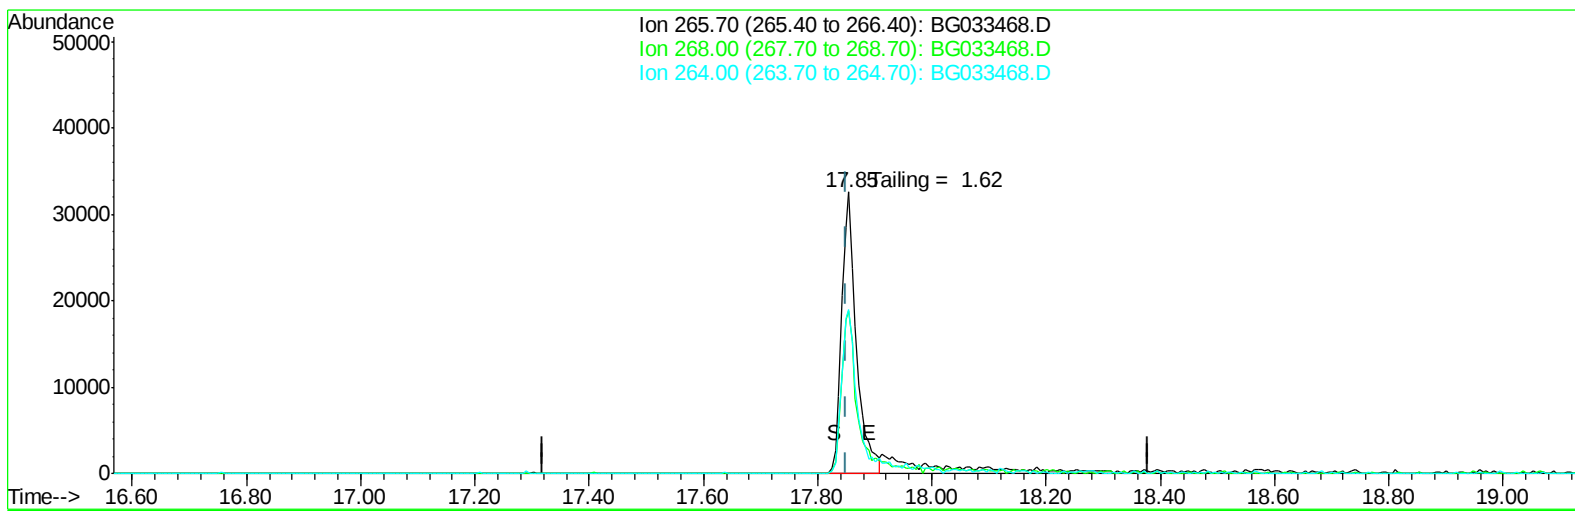

TIC: BG033468.D

(69) Pentachlorophenol (C)




17.854min (+0.004) 12570.36ng

response 58600

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.08
264.00	62.00	58.42
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\Data\BG033018\
 Data File : BG033468.D
 Acq On : 31 Mar 2018 4:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 02:31:44 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 18:34:58 2018
 Response via : Initial Calibration

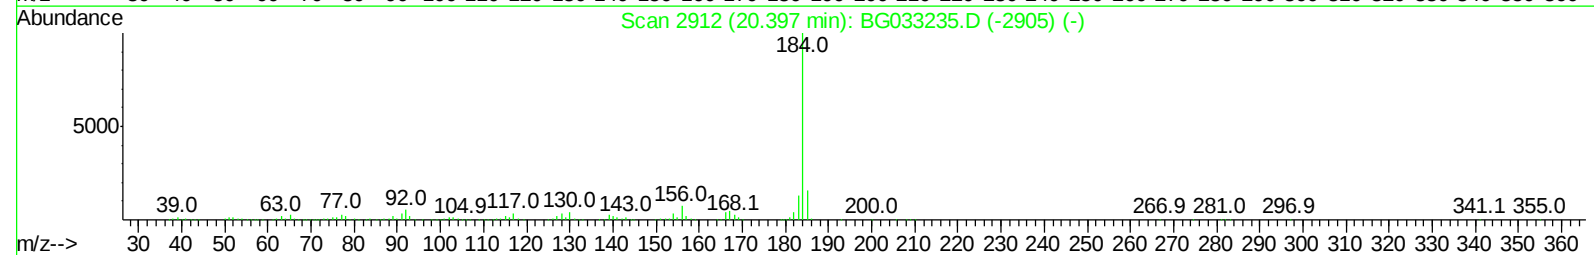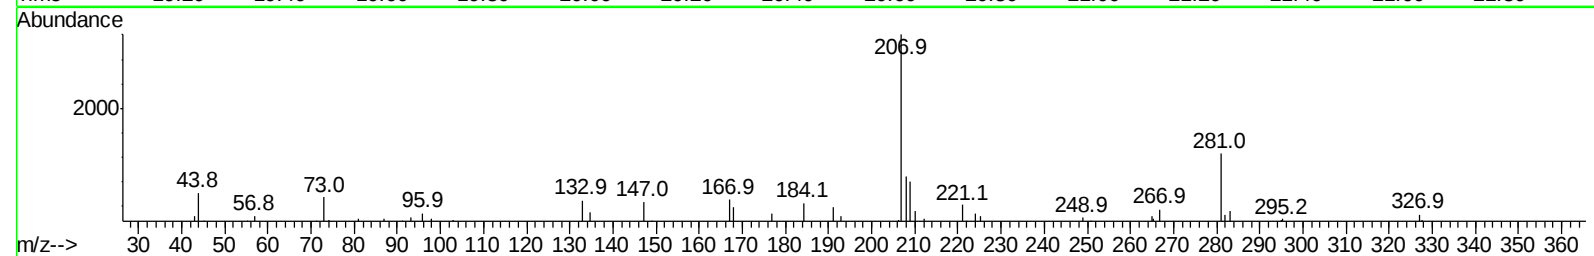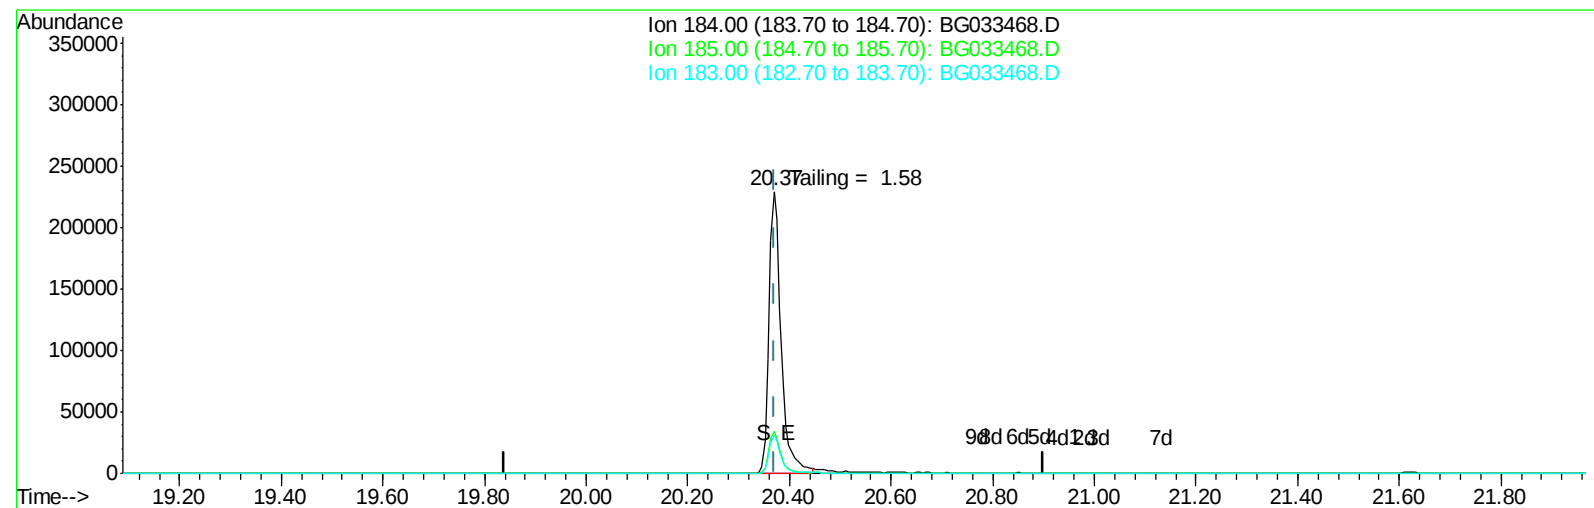

TIC: BG033468.D

(76) Benzidine

20.962min (+0.592) 141.57ng

response 215

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00