

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG033018\
 Data File : BG033460.D
 Acq On : 30 Mar 2018 22:39
 Operator : SJ/JU
 Sample : J1755-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-02-032818

Quant Time: Mar 31 02:33:36 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 28 18:34:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.87	152	29982	20.00	ng	-0.01
21) Naphthalene-d8	11.75	136	133137	20.00	ng	-0.01
38) Acenaphthene-d10	15.48	164	109302	20.00	ng	0.00
63) Phenanthrene-d10	18.21	188	317411	20.00	ng	0.00
75) Chrysene-d12	22.56	240	337920	20.00	ng	0.00
86) Perylene-d12	26.32	264	364662	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	6.29	112	255704	159.92	ng	0.00
7) Phenol-d6	7.98	99	358677	130.56	ng	0.00
23) Nitrobenzene-d5	10.06	82	298382	102.97	ng	-0.01
41) 2,4,6-Tribromophenol	16.96	330	266093	162.77	ng	0.00
44) 2-Fluorobiphenyl	14.11	172	727680	96.11	ng	0.00
78) Terphenyl-d14	20.73	244	1551519	98.19	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG033018\
Data File : BG033460.D
Acq On : 30 Mar 2018 22:39
Operator : SJ/JU
Sample : J1755-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-02-032818

Quant Time: Mar 31 02:33:36 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG031918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 28 18:34:58 2018
Response via : Initial Calibration

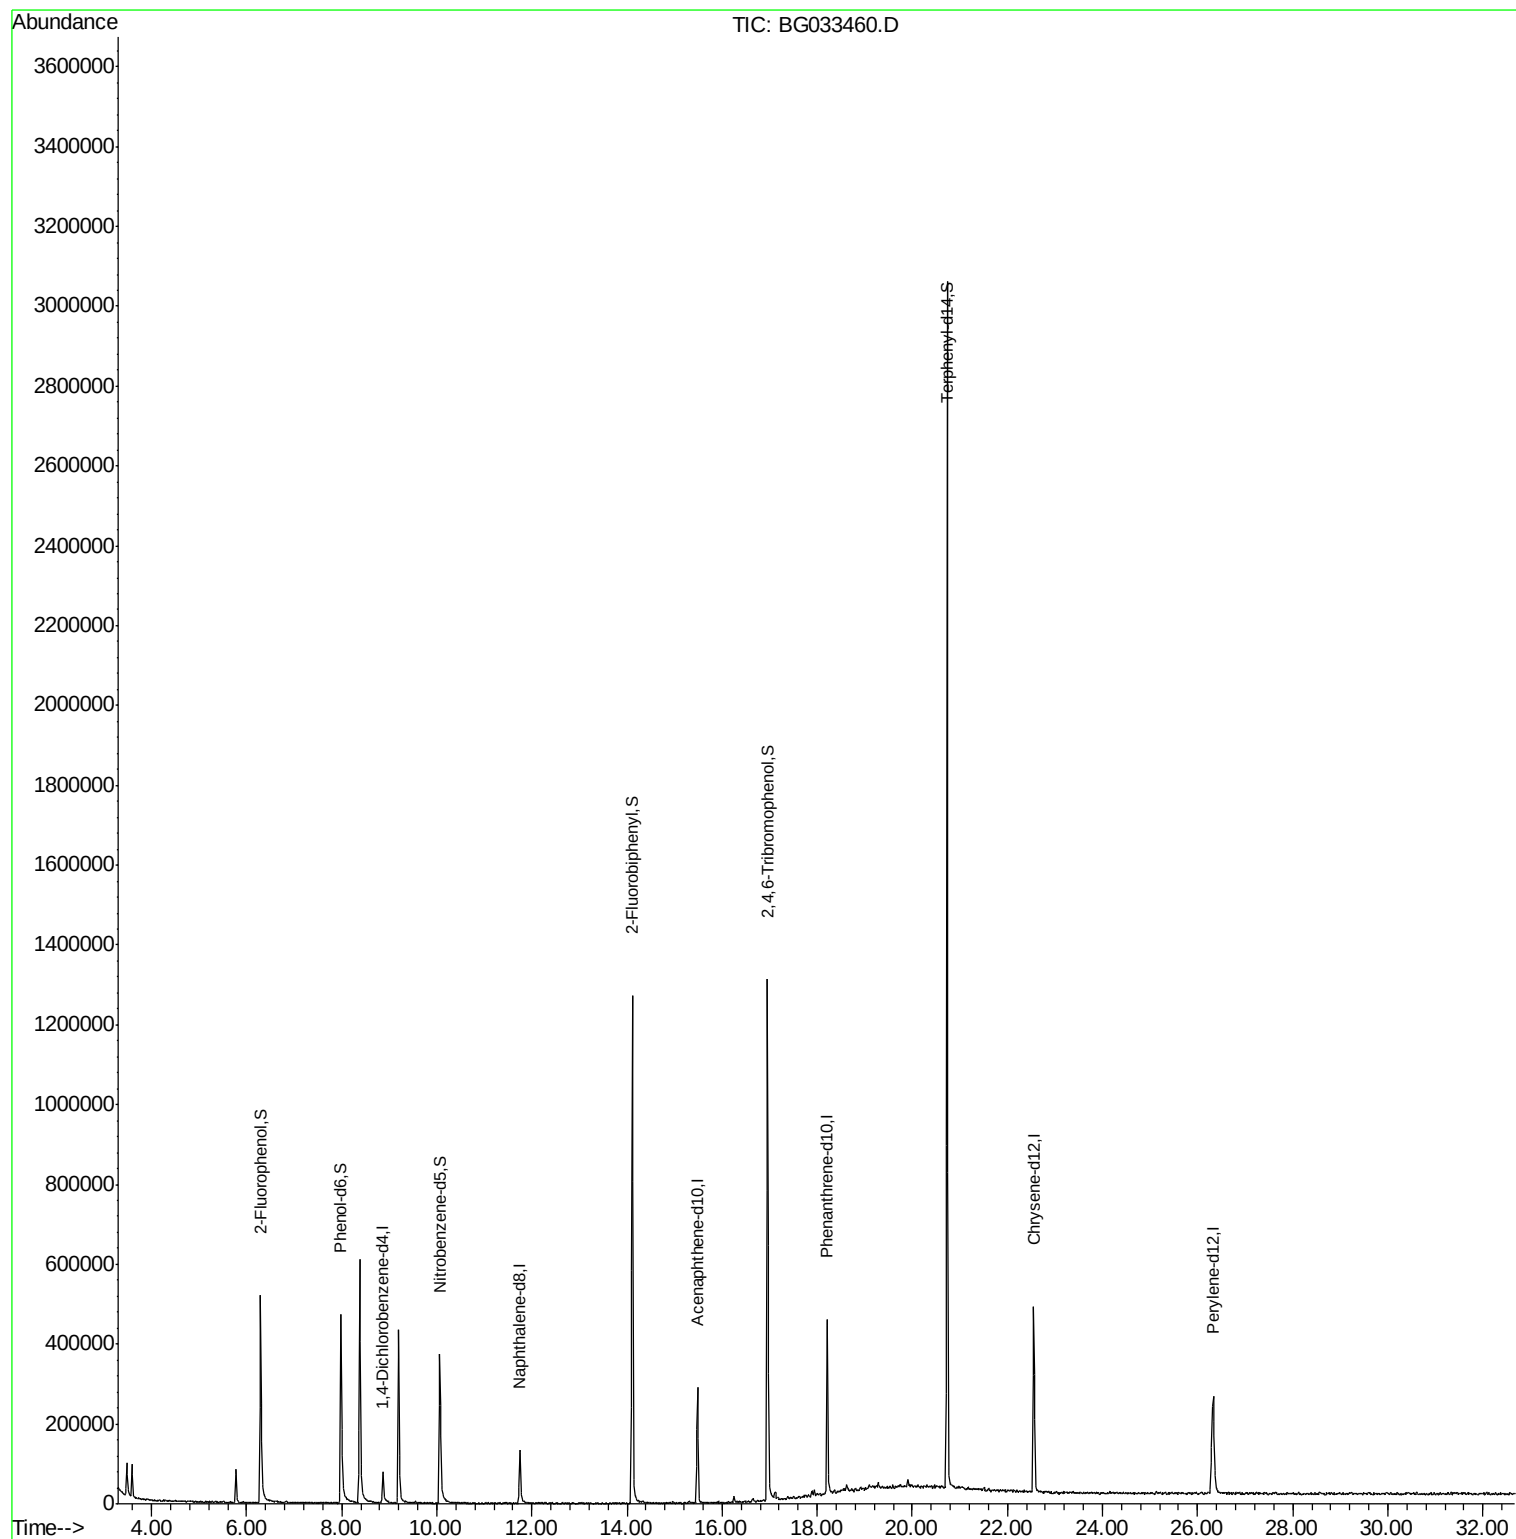

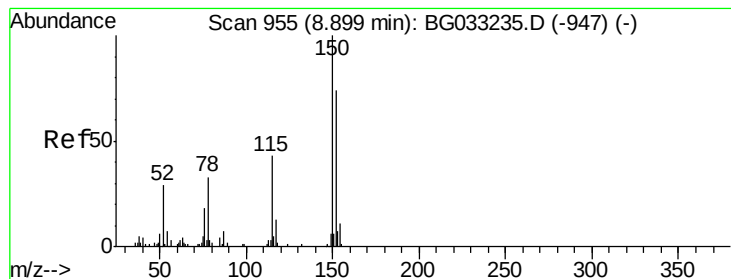

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.87 min Scan# 949

Delta R.T. -0.01 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39

Instrument :

BNA_G

ClientSampleId :

OK-02-032818


Tot Ion:152 Resp: 29982

Ion Ratio Lower Upper

152 100

150 164.0 126.6 189.8




115 62.5 53.0 79.4

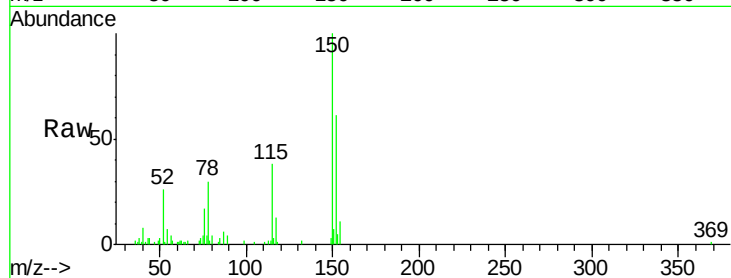

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

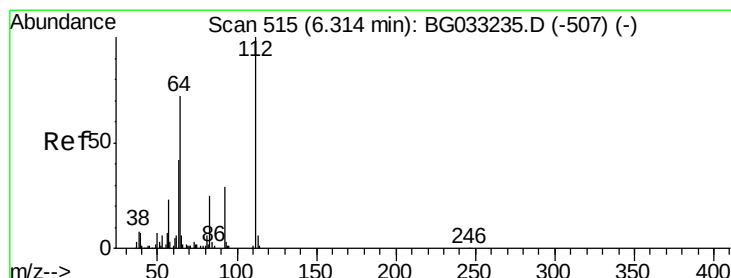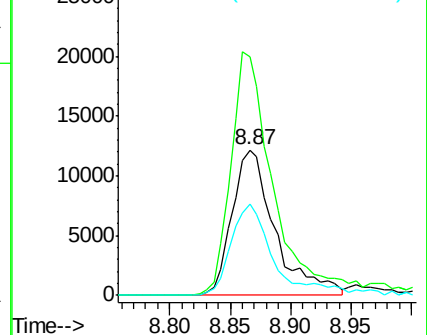

#5

2-Fluorophenol

Concen: 159.921 ng

RT: 6.29 min Scan# 511

Delta R.T. -0.00 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39


Tgt Ion:112 Resp: 255704

Ion Ratio Lower Upper

112 100

64 74.4 56.3 84.5



63 41.6 30.1 45.1

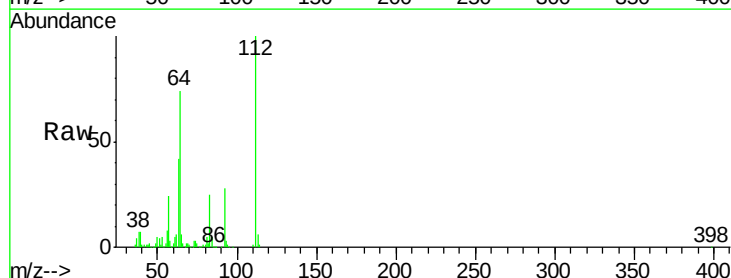


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

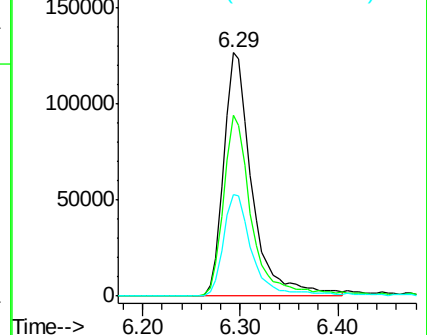



#7

Phenol-d6

Concen: 130.556 ng

RT: 7.98 min Scan# 798

Delta R.T. -0.00 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39

Instrument :

BNA_G

ClientSampleId :

OK-02-032818


Tot Ion: 99 Resp: 358677

Ion Ratio Lower Upper




99 100

42 21.0 14.1 21.1

71 39.2 26.1 39.1#

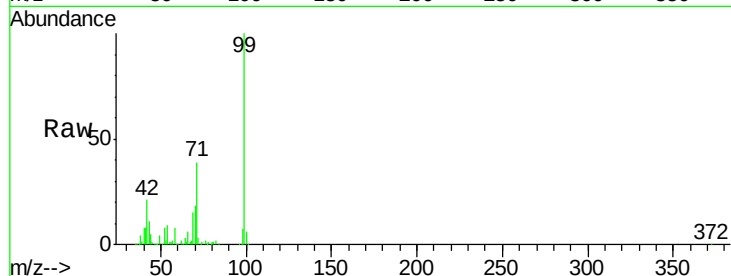

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

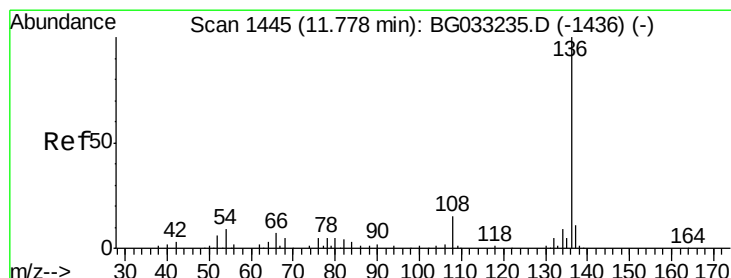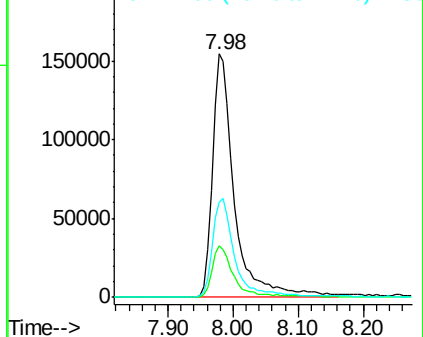

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.75 min Scan# 1439

Delta R.T. -0.01 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39

Tgt Ion: 136 Resp: 133137


Ion Ratio Lower Upper

136 100



137 10.4 9.2 13.8


54 9.0 10.3 15.5#

68 5.3 4.5 6.7

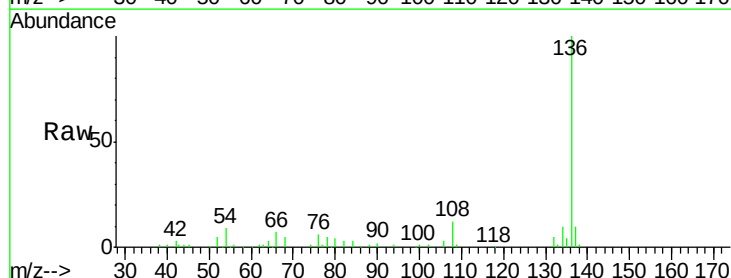

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC




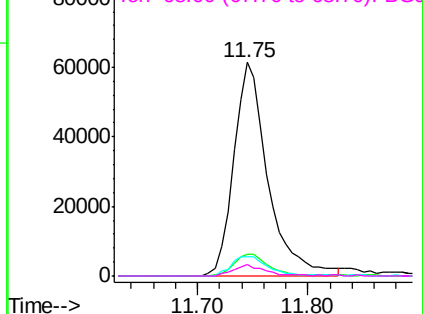


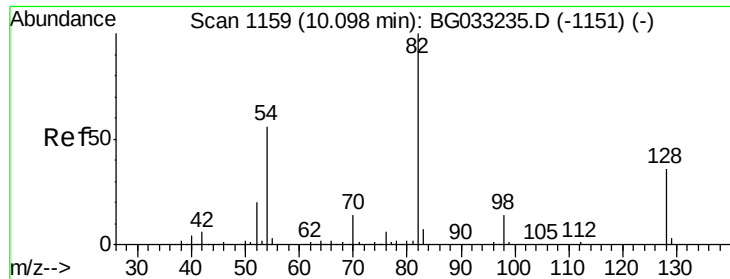

#23
 Nitrobenzene-d5
 Concen: 102.968 ng
 RT: 10.06 min Scan# 1153
 Delta R.T. -0.01 min
 Lab File: BG033460.D
 Acq: 30 Mar 2018 22:39




Instrument :
 BNA_G
 ClientSampleId :
 OK-02-032818


Tot Ion: 82 Resp: 298382
 Ion Ratio Lower Upper
 82 100
 128 38.1 29.7 44.5
 54 57.4 43.1 64.7

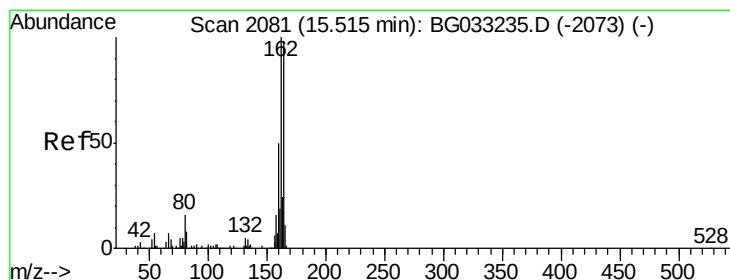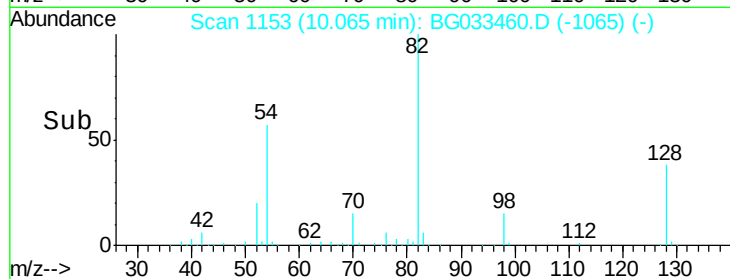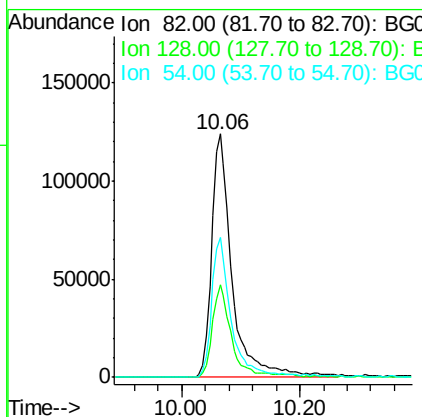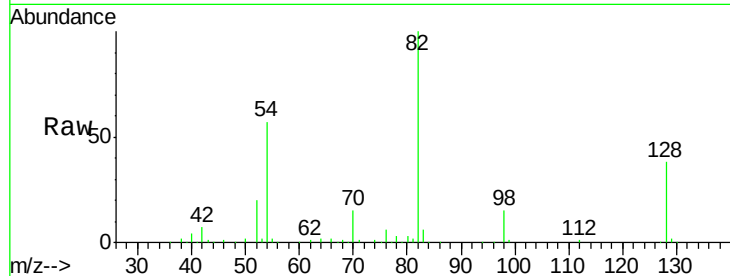

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.48 min Scan# 2075
 Delta R.T. -0.01 min
 Lab File: BG033460.D
 Acq: 30 Mar 2018 22:39

Tgt Ion: 164 Resp: 109302
 Ion Ratio Lower Upper
 164 100
 162 101.2 78.8 118.2
 160 46.4 35.4 53.0

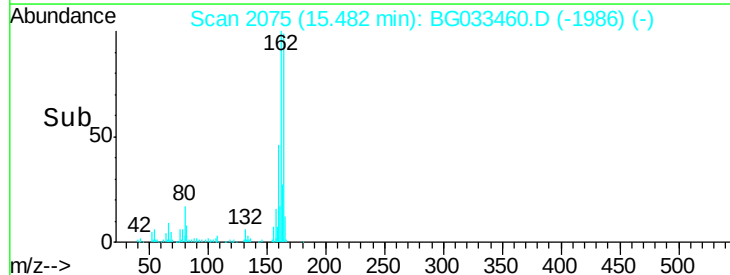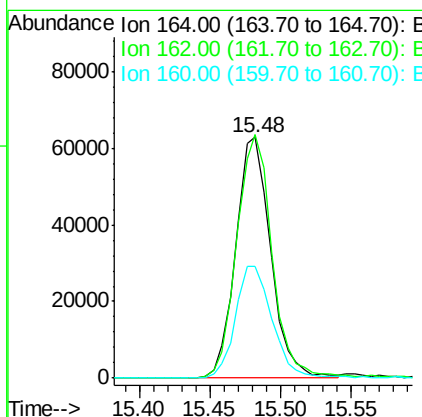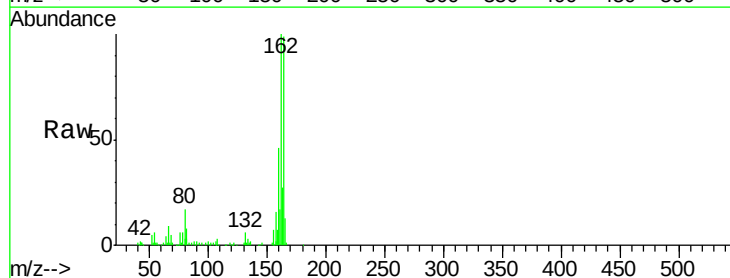


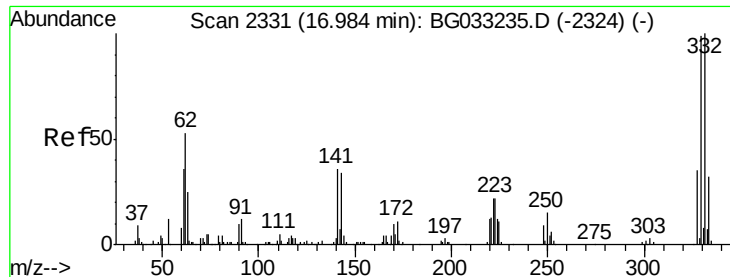




#41
 2,4,6-Tribromophenol
 Concen: 162.774 ng
 RT: 16.96 min Scan# 2326
 Delta R.T. -0.00 min
 Lab File: BG033460.D
 Acq: 30 Mar 2018 22:39

Instrument :
 BNA_G
 ClientSampleId :
 OK-02-032818

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	77.0	115.6
141	37.1	25.2	37.8

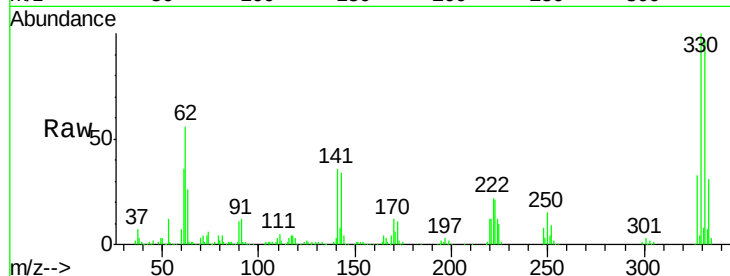


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

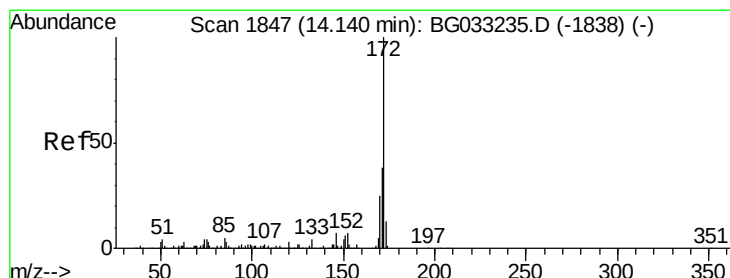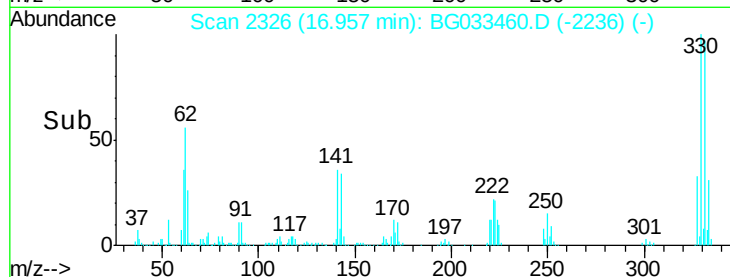
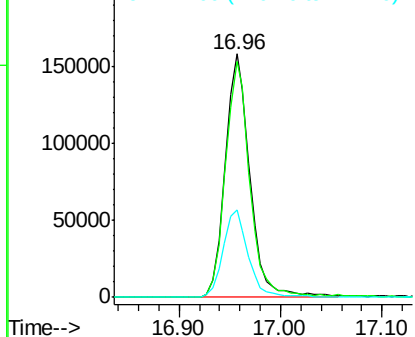



#44
 2-Fluorobiphenyl
 Concen: 96.110 ng
 RT: 14.11 min Scan# 1841
 Delta R.T. -0.01 min
 Lab File: BG033460.D
 Acq: 30 Mar 2018 22:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	30.0	45.0
170	24.2	19.5	29.3

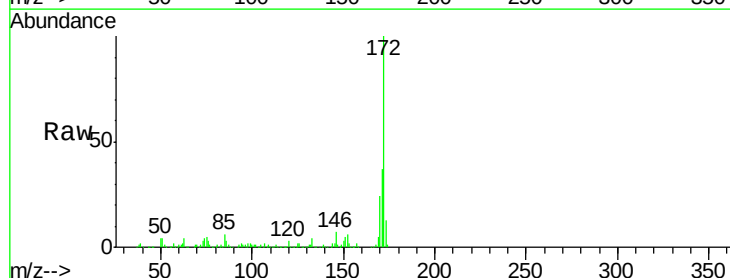

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

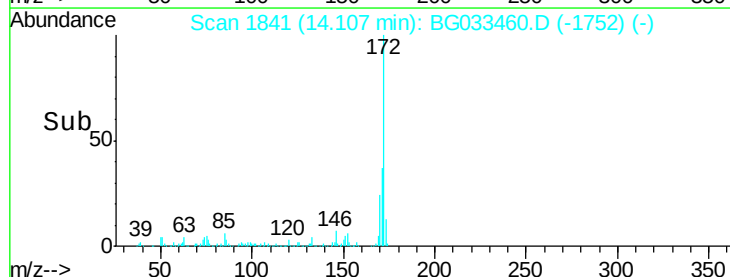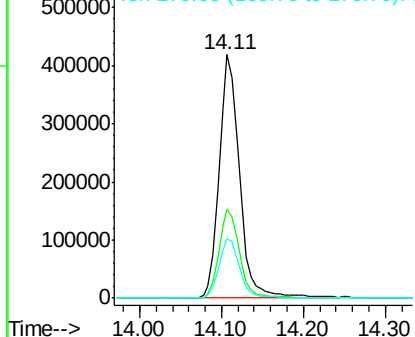



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 18.21 min Scan# 2539

Delta R.T. -0.01 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39

Instrument :

BNA_G

ClientSampleId :

OK-02-032818


Tot Ion:188 Resp: 317411

Ion Ratio Lower Upper

188 100

94 6.5 6.9 10.3#




80 8.6 7.7 11.5

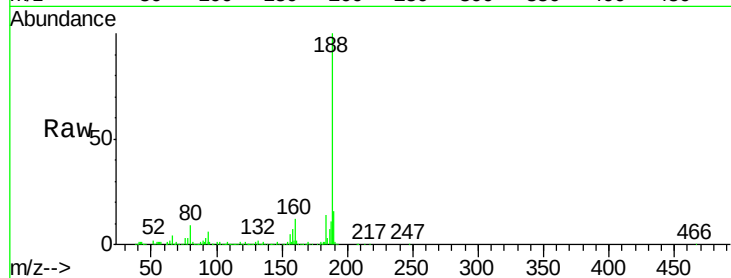

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

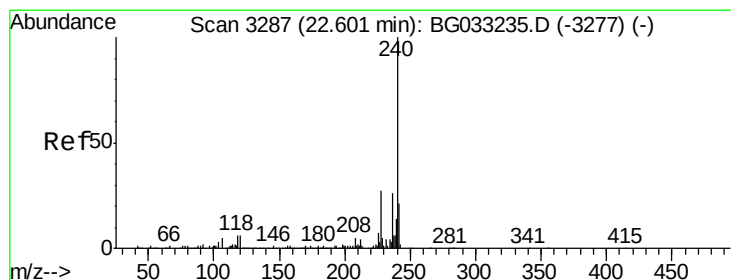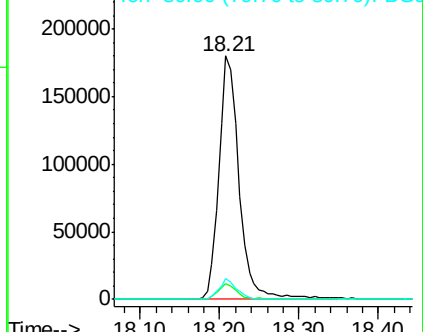

#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.56 min Scan# 3279

Delta R.T. -0.01 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39


Tgt Ion:240 Resp: 337920

Ion Ratio Lower Upper

240 100

120 6.4 6.8 10.2#



236 25.4 20.9 31.3

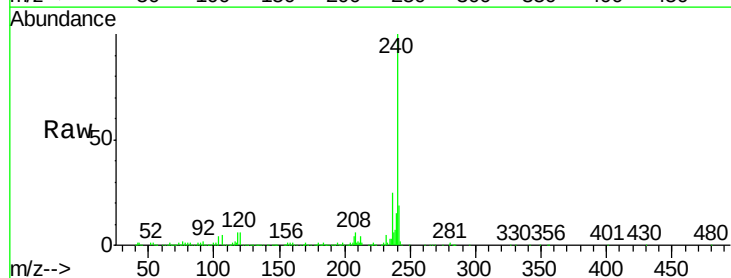


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

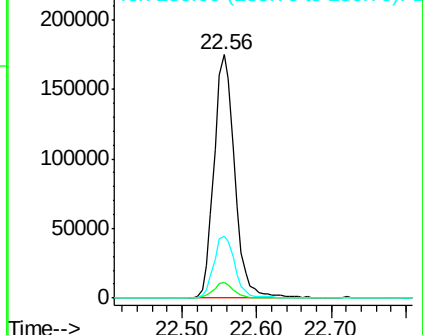



#78

Terphenyl-d14

Concen: 98.192 ng

RT: 20.73 min Scan# 2969

Delta R.T. -0.00 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39

Instrument :

BNA_G

ClientSampleId :

OK-02-032818


Tot Ion:244 Resp: 1551519

Ion Ratio Lower Upper




244 100

212 8.6 5.8 8.8

122 6.9 7.0 10.4#

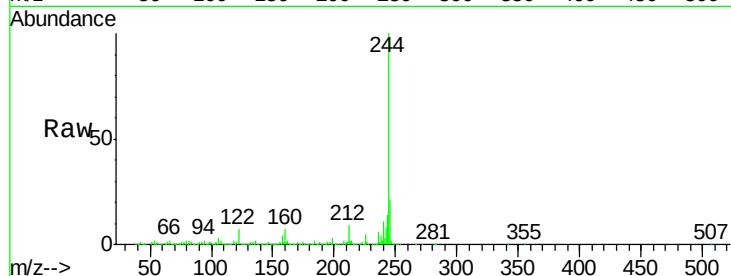

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

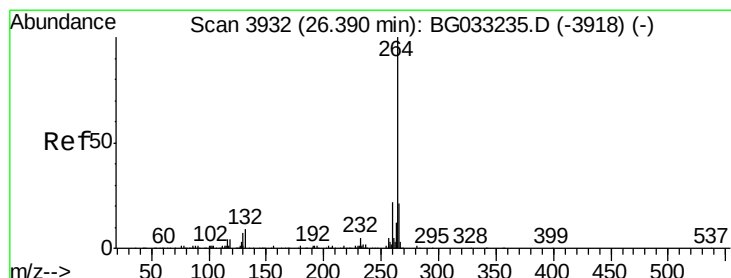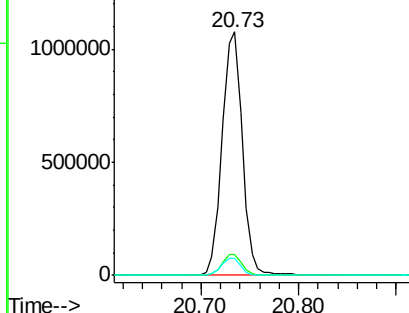

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.32 min Scan# 3920

Delta R.T. -0.01 min

Lab File: BG033460.D

Acq: 30 Mar 2018 22:39


Tgt Ion:264 Resp: 364662

Ion Ratio Lower Upper

264 100

260 22.7 17.4 26.0

265 22.5 17.7 26.5

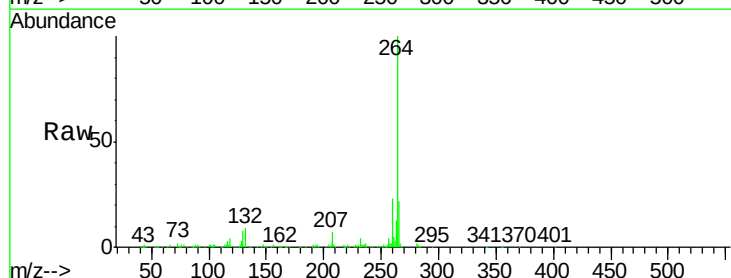

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

