


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG033018\
 Data File : BG033468.D
 Acq On : 31 Mar 2018 4:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG031918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 28 18:34:58 2018

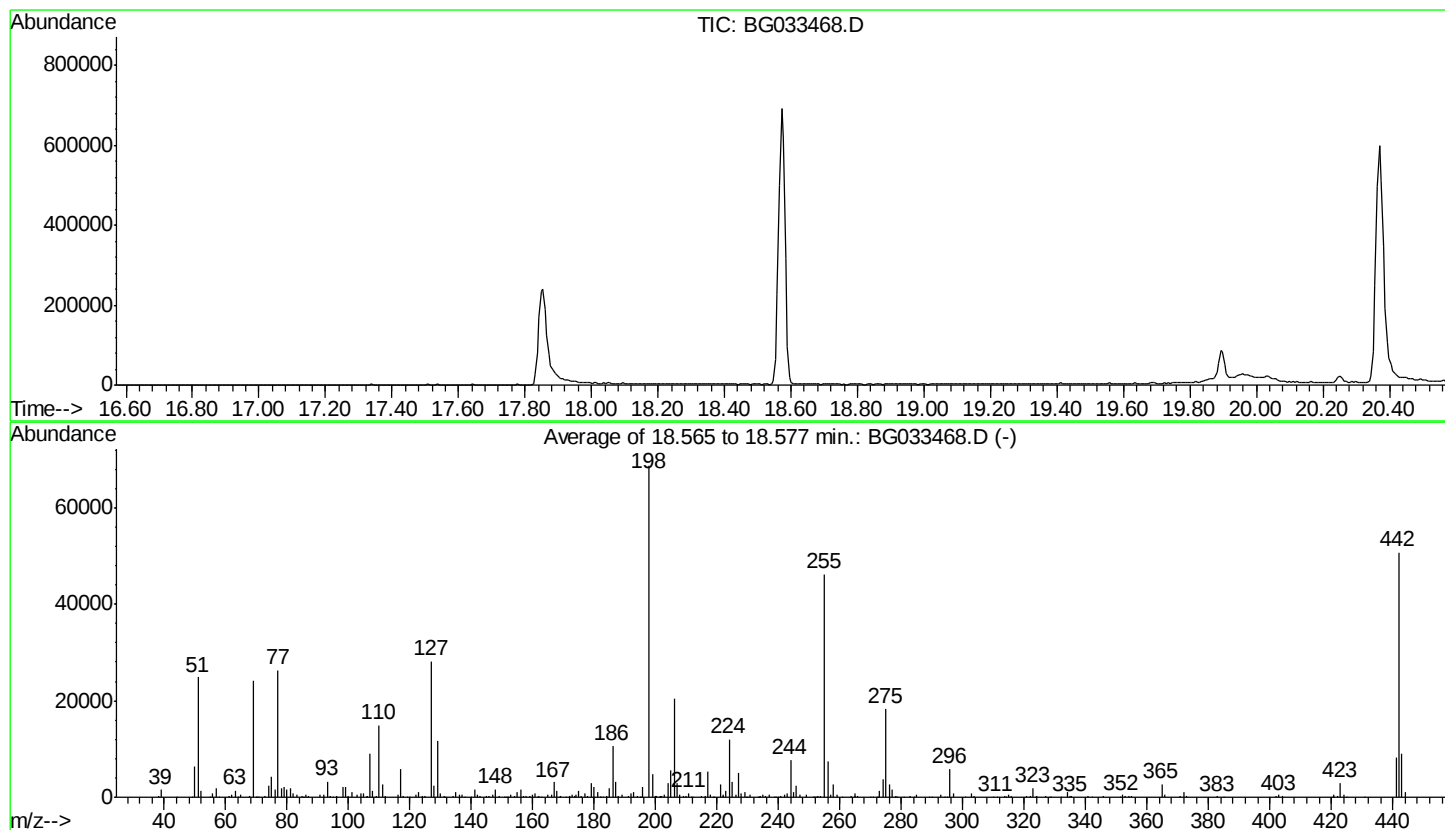

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	24893	PASS
68	69	0.00	2	1.6	389	PASS
69	198	0.00	100	35.1	24117	PASS
70	69	0.00	2	0.4	92	PASS
127	198	10	80	41.1	28218	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68722	PASS
199	198	5	9	7.0	4815	PASS
275	198	10	60	26.6	18314	PASS
365	198	1	100	3.9	2693	PASS
441	443	0.01	100	90.8	8169	PASS
442	198	50	100	73.8	50746	PASS
443	442	15	24	17.7	9001	PASS