
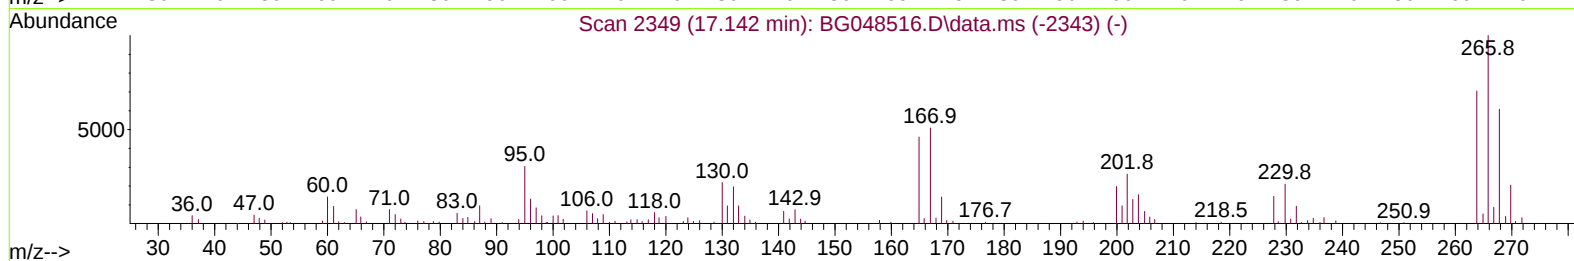
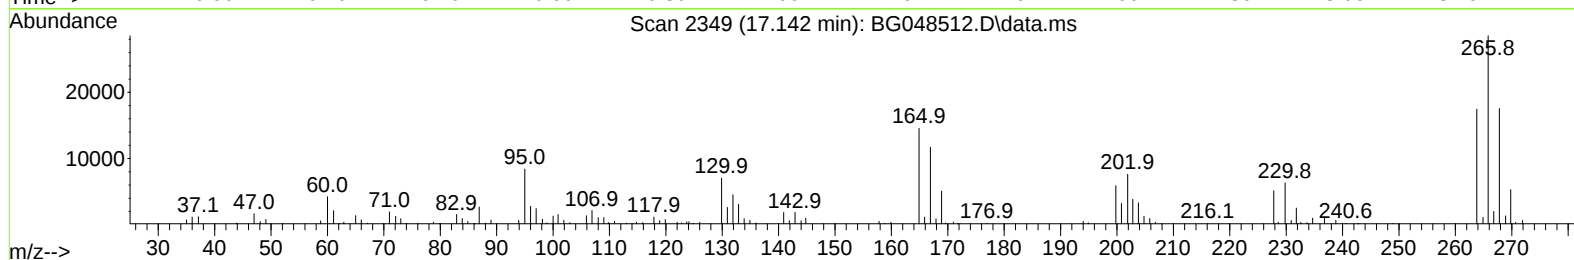


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033021\
Data File : BG048512.D
Acq On : 30 Mar 2021 16:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 02:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 01:49:35 2021
Response via : Initial Calibration

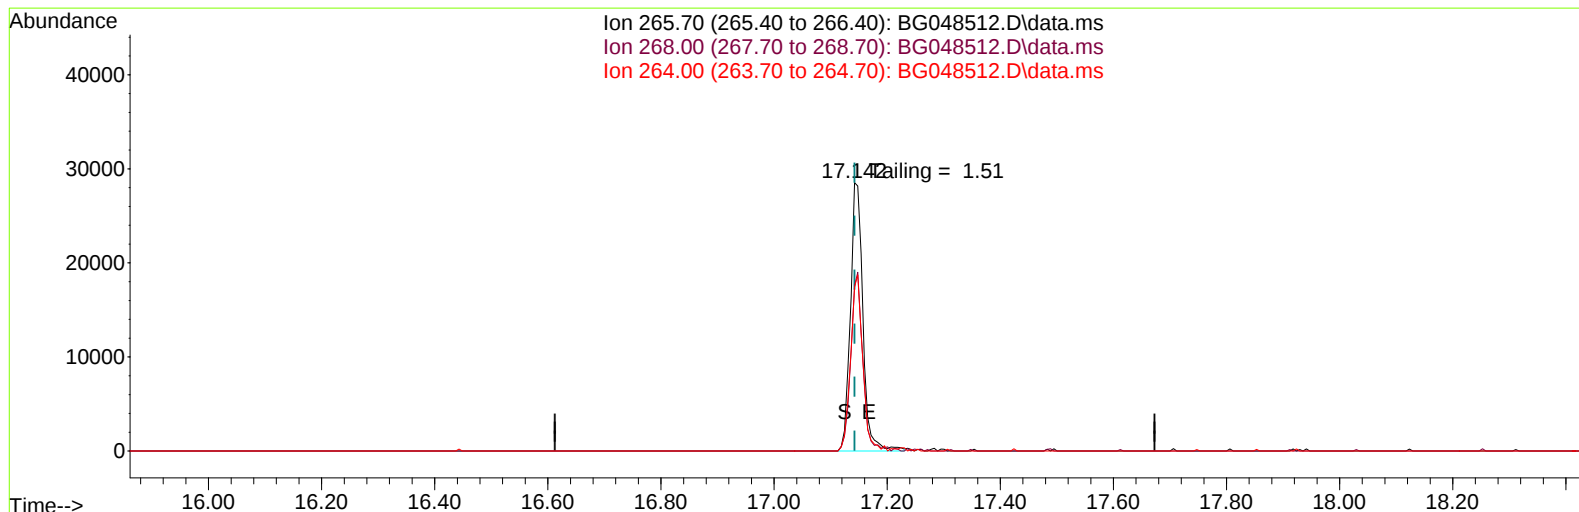

TIC: BG048512.D\data.ms

(70) Pentachlorophenol (C)




17.142min (-0.000) 31756.28 ng

response 43408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.48
264.00	70.50	61.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033021\
Data File : BG048512.D
Acq On : 30 Mar 2021 16:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 02:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 01:49:35 2021
Response via : Initial Calibration

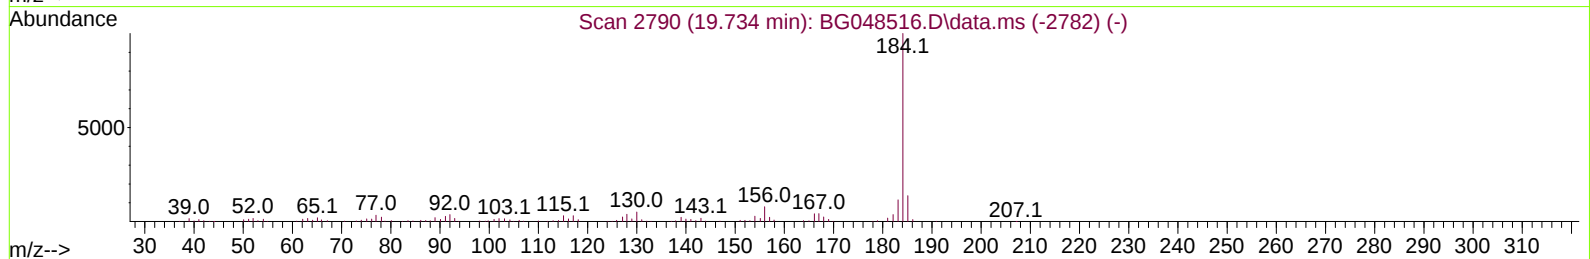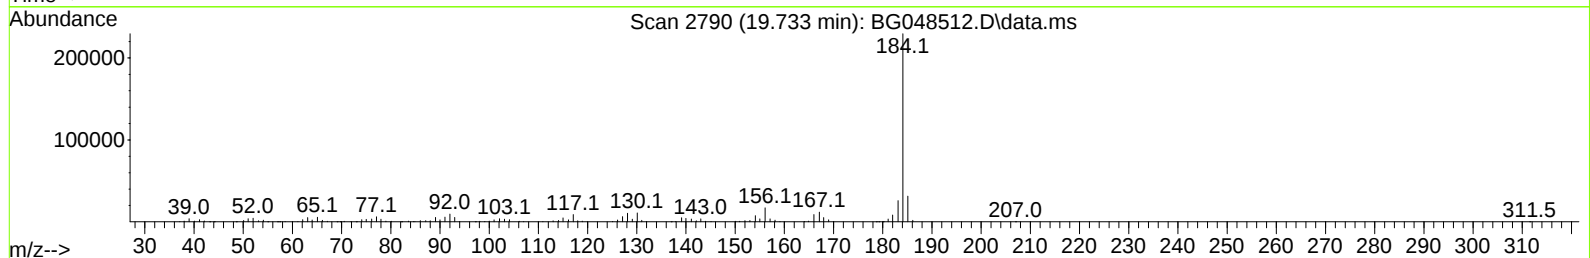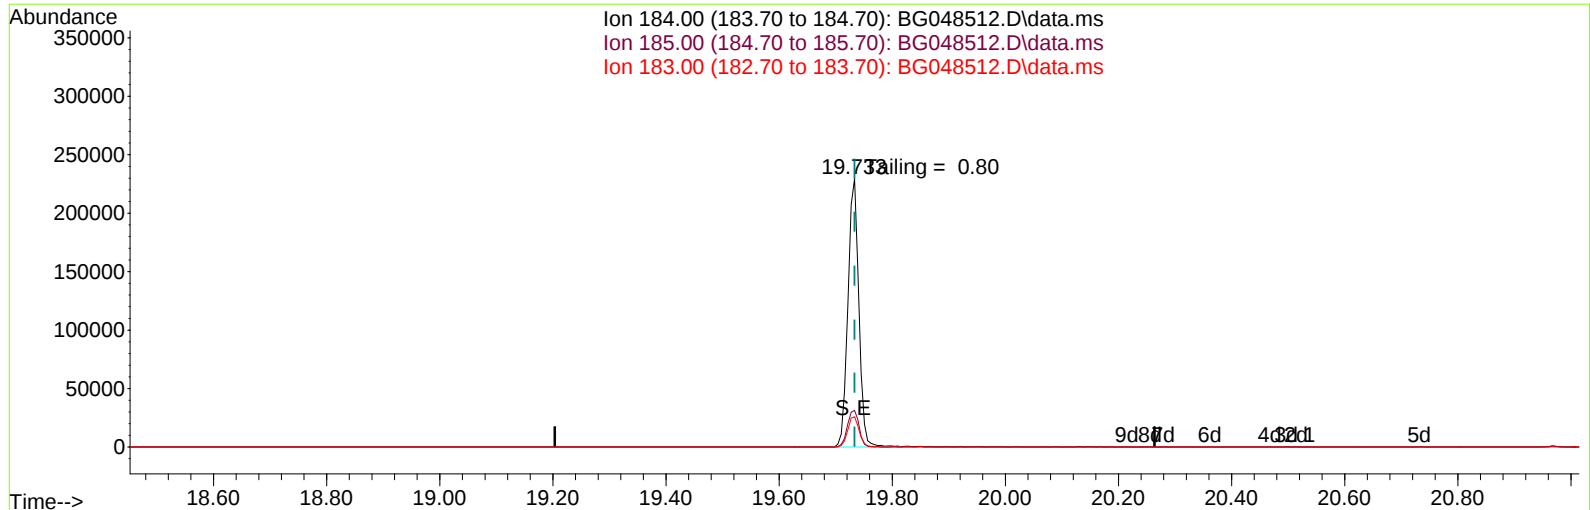

TIC: BG048512.D\data.ms

(77) Benzidine

19.733min (-0.000) 138892.93 ng m

response 310420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.67
183.00	11.50	11.30
0.00	0.00	0.00