
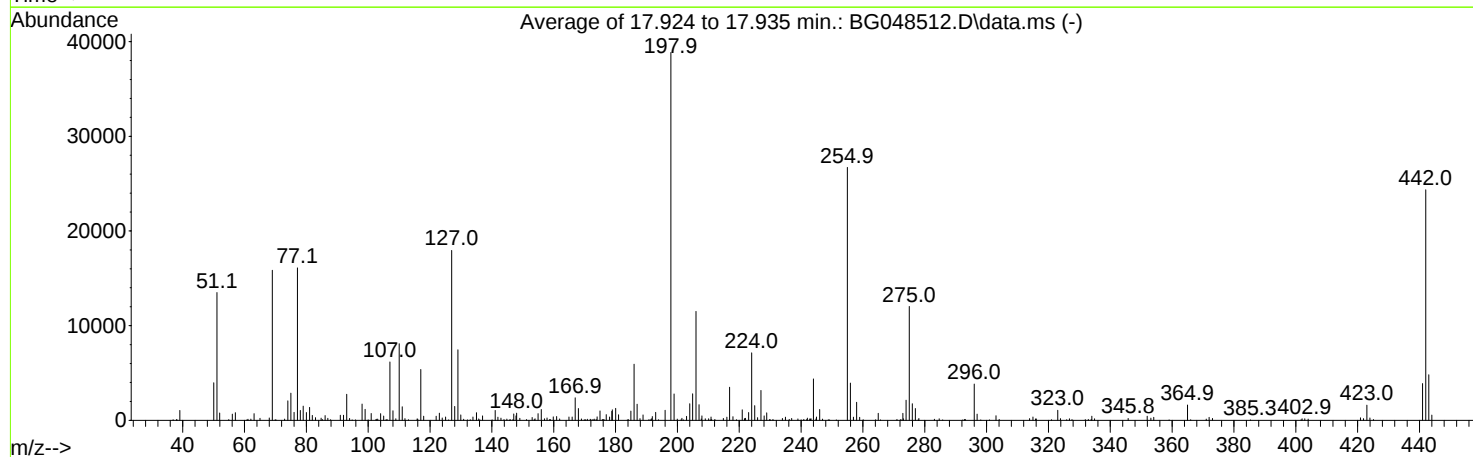


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033021\
 Data File : BG048512.D
 Acq On : 30 Mar 2021 16:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 31 01:49:35 2021

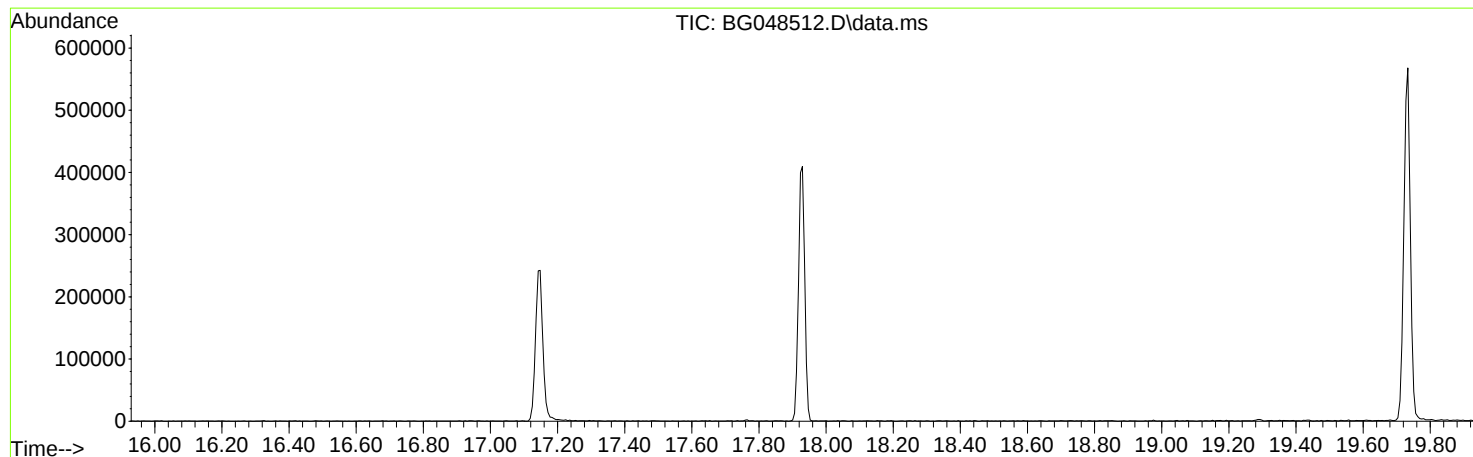




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	13507	PASS
68	69	0.00	2	1.6	258	PASS
69	198	0.00	100	40.8	15851	PASS
70	69	0.00	2	0.4	64	PASS
127	198	10	80	46.2	17953	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38848	PASS
199	198	5	9	7.2	2783	PASS
275	198	10	60	31.0	12024	PASS
365	198	1	100	4.2	1631	PASS
441	198	0.01	100	10.0	3887	PASS
442	198	50	100	62.7	24355	PASS
443	442	15	24	19.8	4812	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033021\
Data File : BG048512.D
Acq On : 30 Mar 2021 16:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 02:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 01:49:35 2021
Response via : Initial Calibration

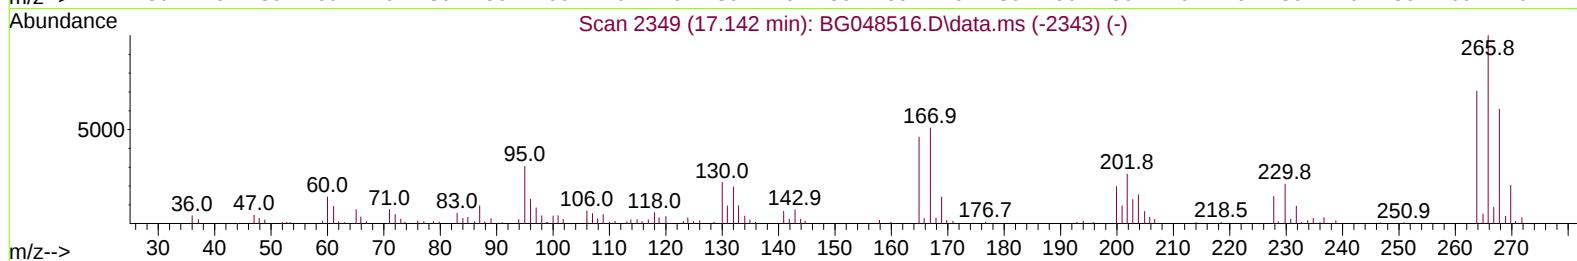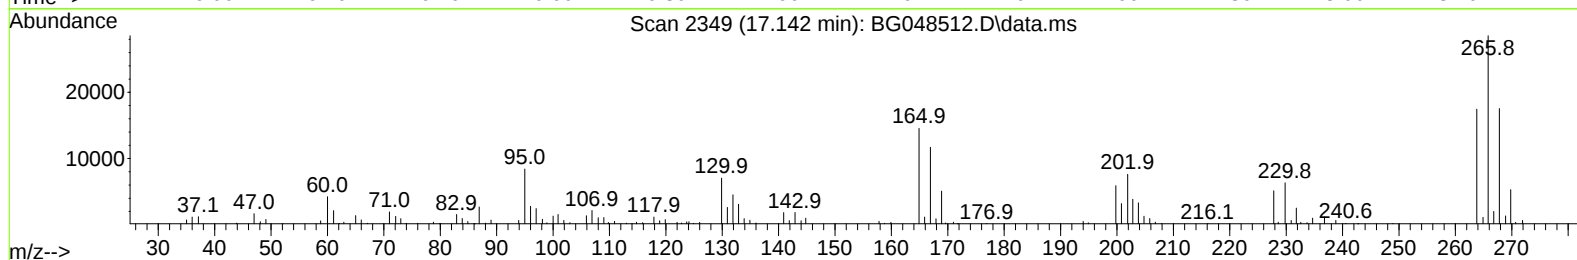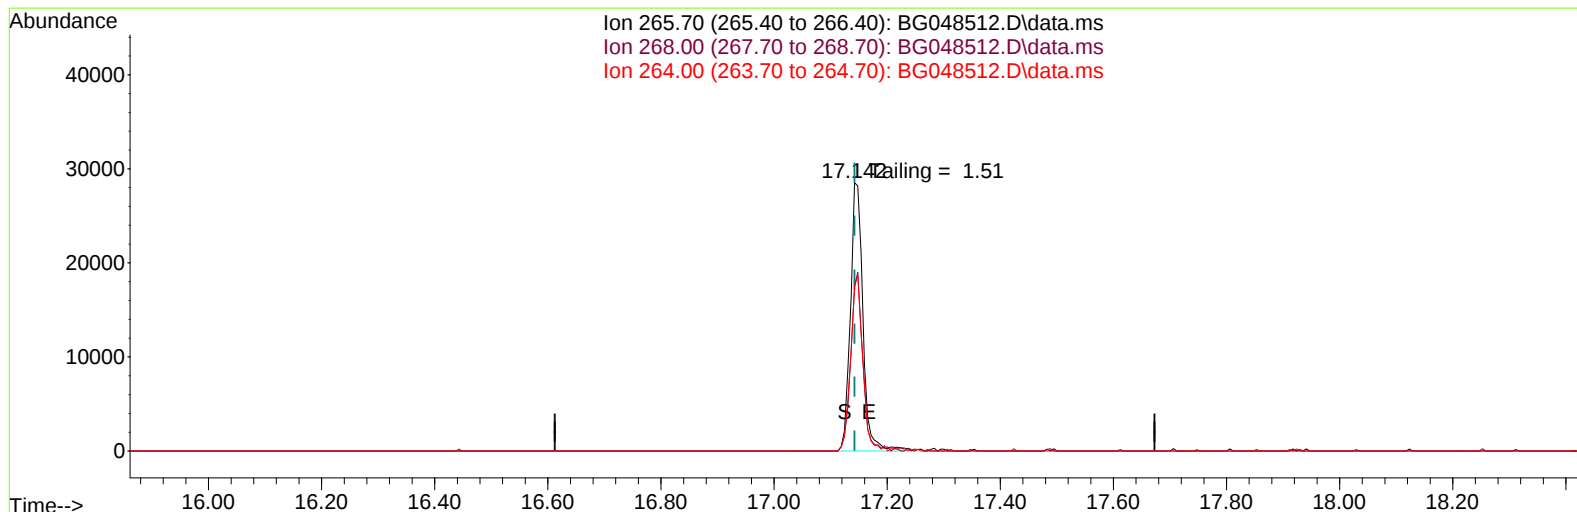

TIC: BG048512.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.000) 31756.28 ng




response 43408

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	61.48
264.00	70.50	61.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033021\
Data File : BG048512.D
Acq On : 30 Mar 2021 16:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 02:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 01:49:35 2021
Response via : Initial Calibration

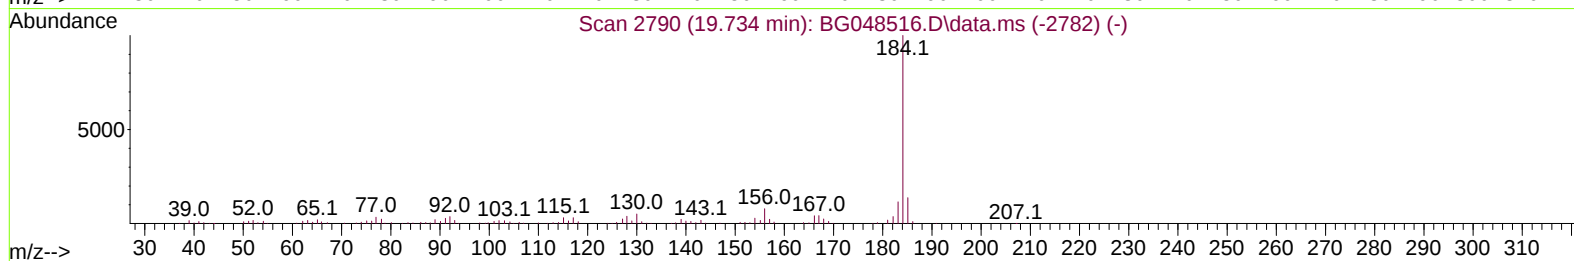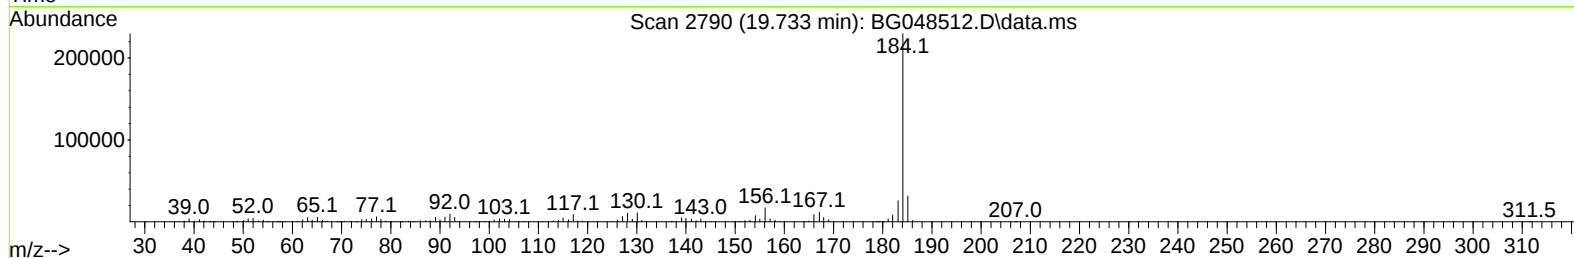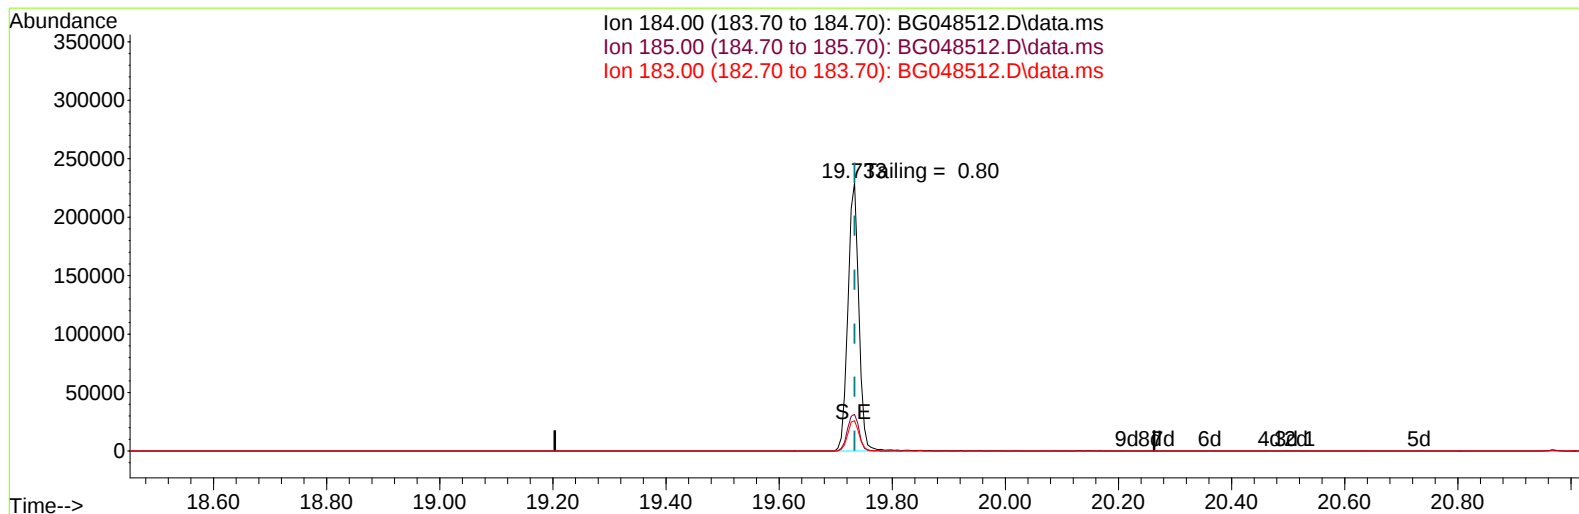

TIC: BG048512.D\data.ms

(77) Benzidine

19.733min (-0.000) 138892.93 ng m

response 310420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.67
183.00	11.50	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2021	BNA_G	BG048512.D
Compound Name	Response	Retention Time
DDT	154045	20.973
DDD	1486	20.515
DDE	57	20.021
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1543	155588	0.99