




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052950.D
 Acq On : 30 Mar 2022 15:30
 Operator : CG/JU
 Sample : N2068-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ40

Manual IntegrationsAPPROVED

Quant Time: Mar 31 09:17:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

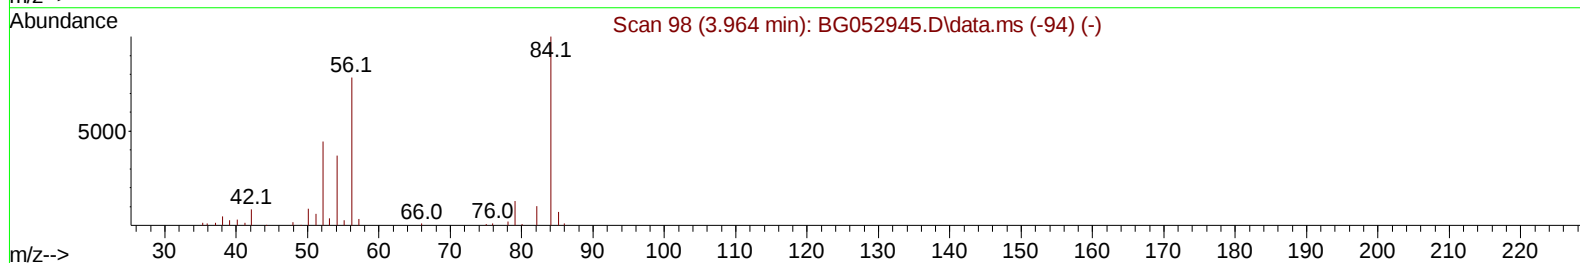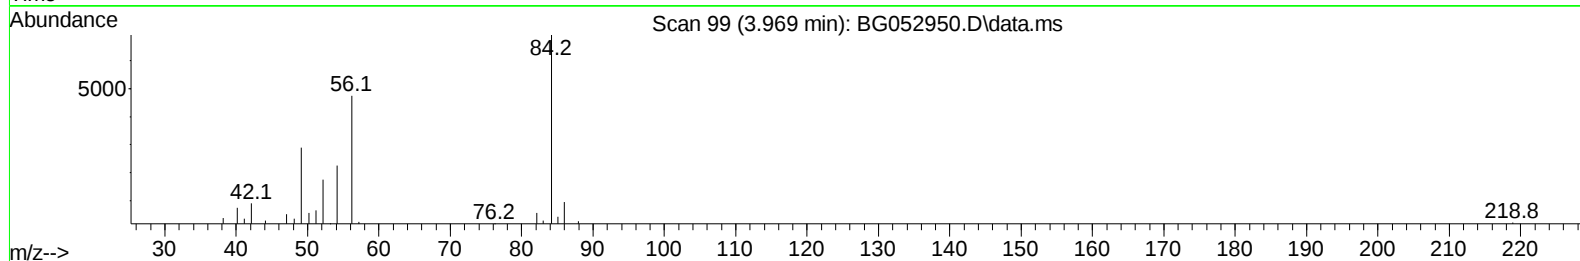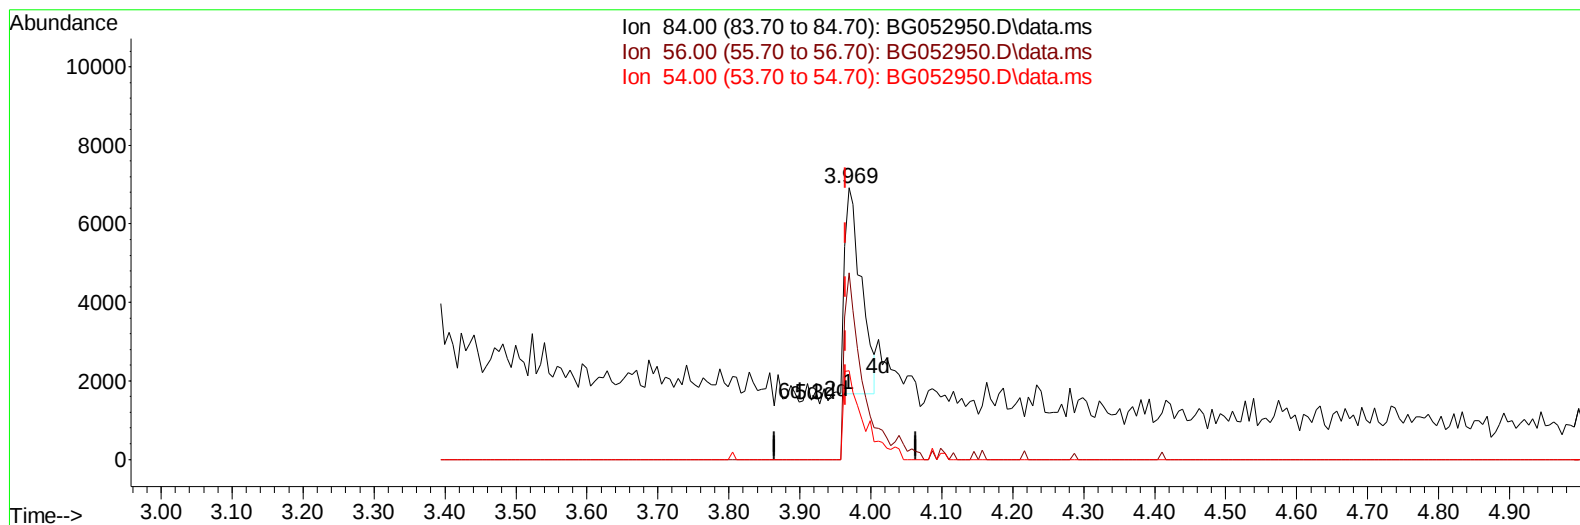

TIC: BG052950.D\data.ms

(4) Pyridine-d5 (S)

3.969min (+ 0.005) 5.16 ng/u1

response 8488

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	68.63
54.00	28.70	32.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052950.D
Acq On : 30 Mar 2022 15:30
Operator : CG/JU
Sample : N2068-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ40

Manual IntegrationsAPPROVED

Quant Time: Mar 31 09:17:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

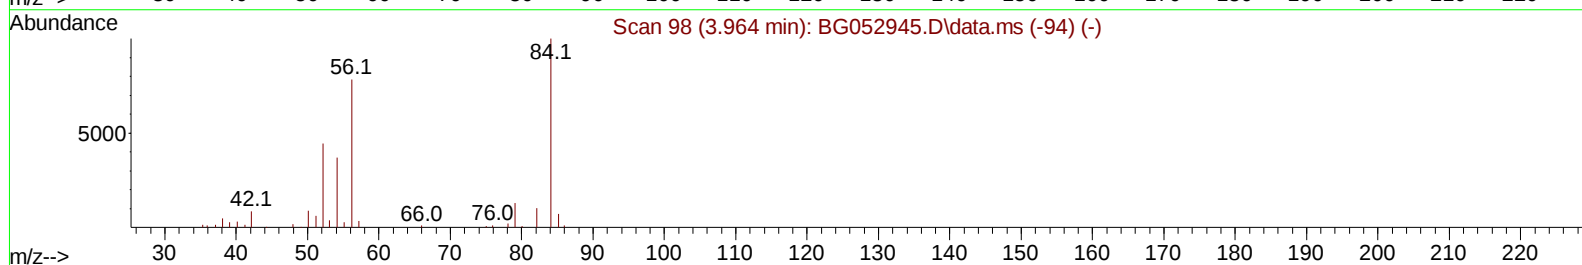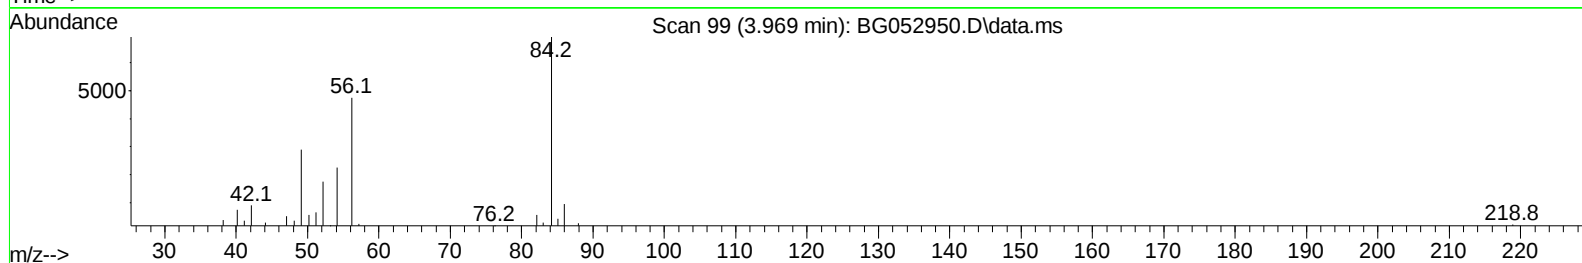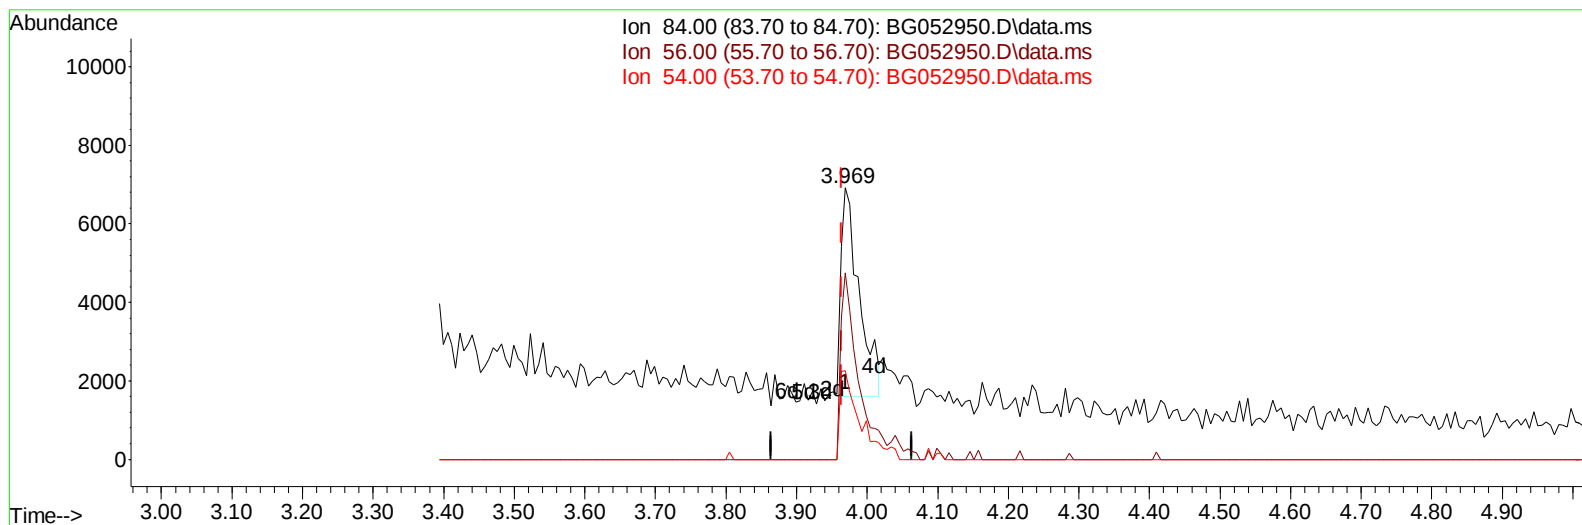

TIC: BG052950.D\data.ms

(4) Pyridine-d5 (S)

3.969min (+ 0.005) 5.75 ng/u1 m

response 9455

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	68.63
54.00	28.70	32.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052950.D
Acq On : 30 Mar 2022 15:30
Operator : CG/JU
Sample : N2068-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ40

Manual IntegrationsAPPROVED

Quant Time: Mar 31 09:17:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

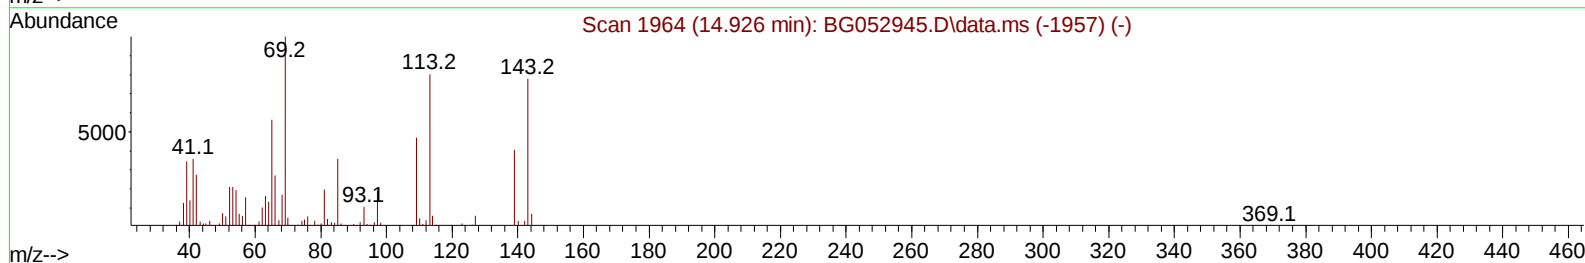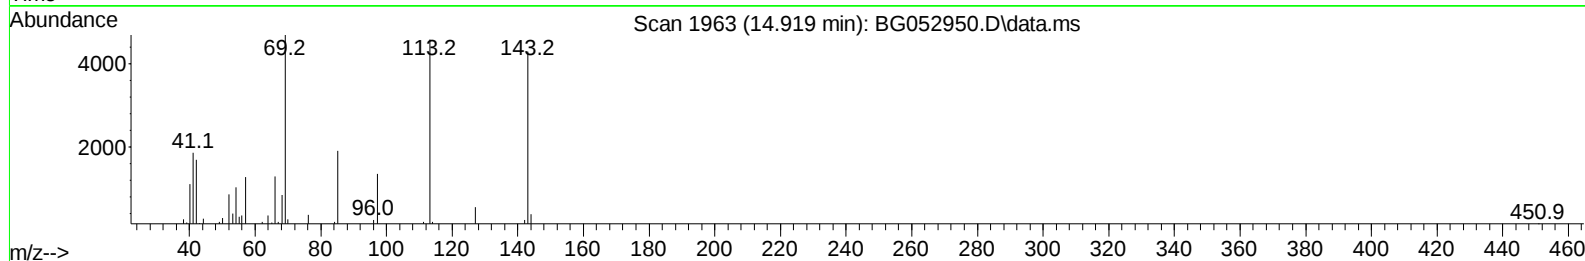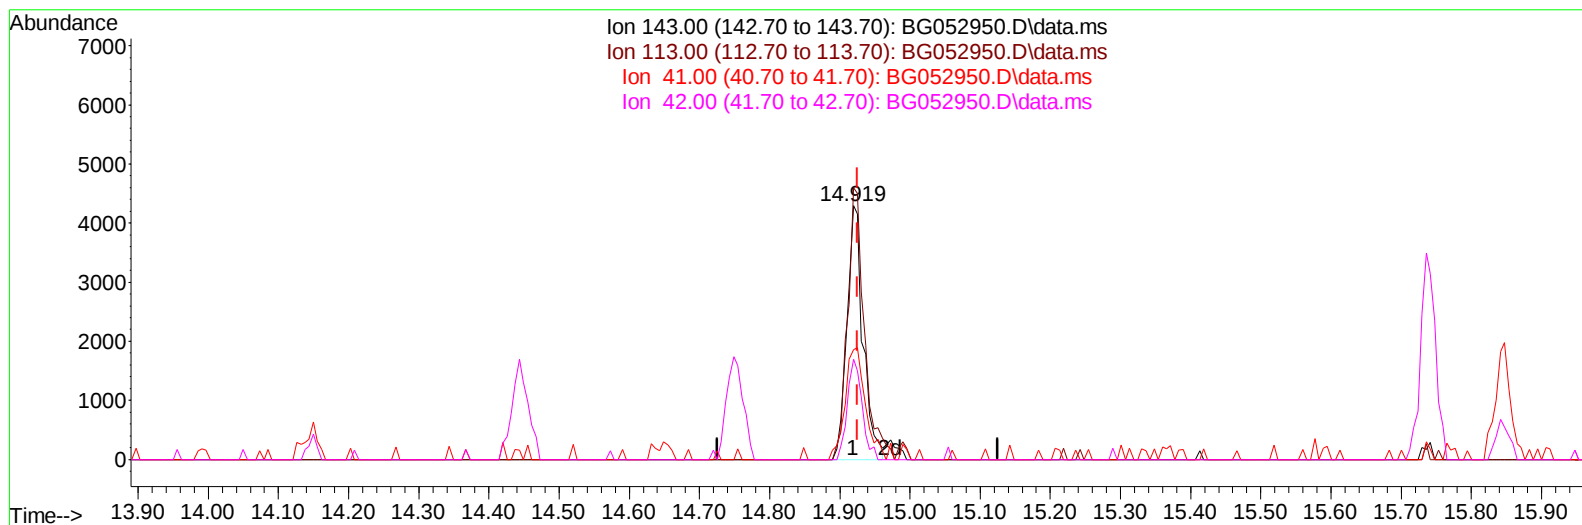

TIC: BG052950.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.919min (-0.006) 6.55 ng/u1

response 6864

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	106.96
41.00	47.20	43.33
42.00	29.40	39.37#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052950.D
Acq On : 30 Mar 2022 15:30
Operator : CG/JU
Sample : N2068-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ40

Manual IntegrationsAPPROVED

Quant Time: Mar 31 09:17:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

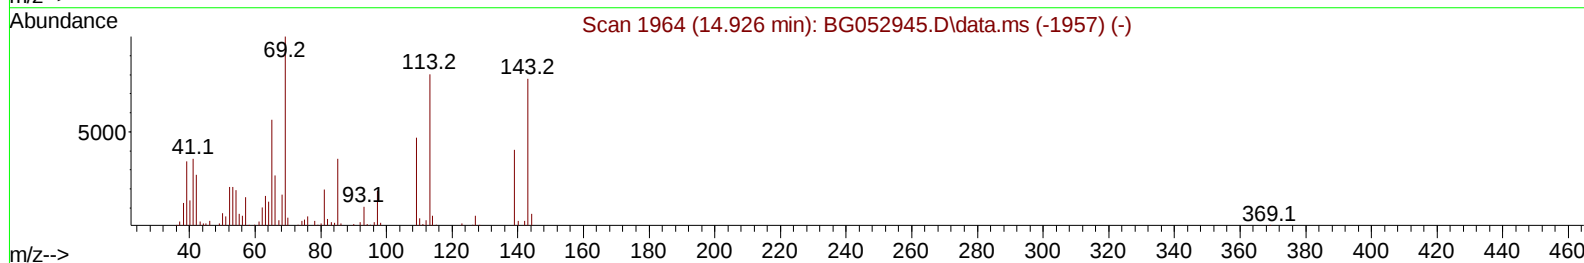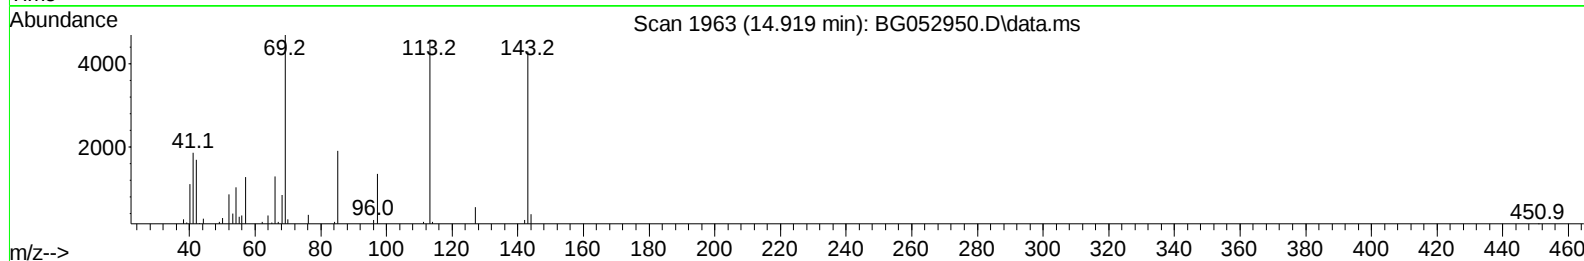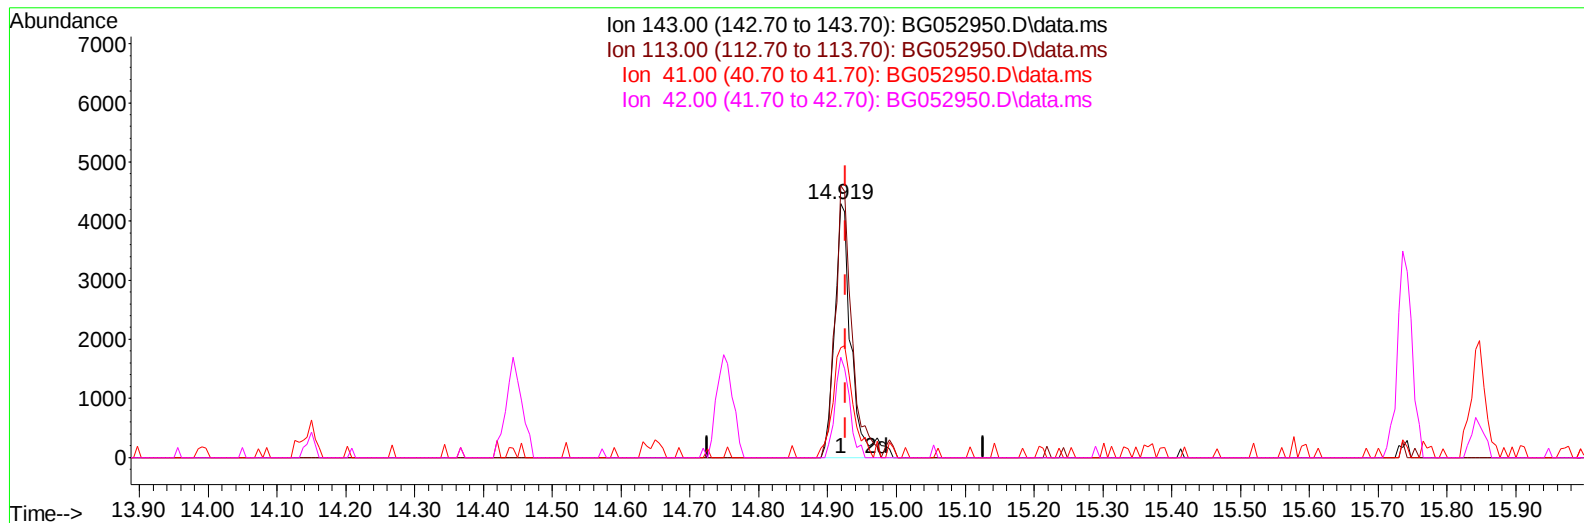

TIC: BG052950.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.919min (-0.006) 6.93 ng/ul m

response 7258

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	106.96
41.00	47.20	43.33
42.00	29.40	39.37#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052950.D
 Acq On : 30 Mar 2022 15:30
 Operator : CG/JU
 Sample : N2068-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ40

Manual IntegrationsAPPROVED

Quant Time: Mar 31 09:17:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	23268	20.000	ng/ul	0.00
20) Naphthalene-d8	10.942	136	98704	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.749	164	81078	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	199442	20.000	ng/ul	0.00
79) Chrysene-d12	21.775	240	225938	20.000	ng/ul	0.00
88) Perylene-d12	25.088	264	227226	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	2415	3.666	ng/uL	0.00
4) Pyridine-d5	3.969	84	9455m	5.749	ng/ul	0.00
7) Phenol-d5	7.277	99	14555	6.984	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	38821	30.500	ng/ul	0.00
11) 2-Chlorophenol-d4	7.664	132	30893	21.832	ng/ul	0.00
15) 4-Methylphenol-d8	8.827	113	27437	18.175	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	22107	31.114	ng/ul	0.00
24) 2-Nitrophenol-d4	10.020	143	22959	30.636	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.555	165	42143	25.849	ng/ul	0.00
31) 4-Chloroaniline-d4	11.066	131	42384	19.670	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	196635	31.569	ng/ul	0.00
49) Acenaphthylene-d8	14.443	160	206008	27.218	ng/ul	0.00
54) 4-Nitrophenol-d4	14.919	143	7258m	6.931	ng/ul	0.00
60) Fluorene-d10	15.742	176	170545	31.183	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.847	200	33782	33.284	ng/ul	0.00
73) Anthracene-d10	17.592	188	306901	33.045	ng/ul	0.00
81) Pyrene-d10	19.877	212	399641	31.619	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.859	264	403849	34.397	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052950.D
Acq On : 30 Mar 2022 15:30
Operator : CG/JU
Sample : N2068-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ40

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Mar 31 09:17:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

