




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052954.D
Acq On : 30 Mar 2022 18:05
Operator : CG/JU
Sample : N2068-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYX0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

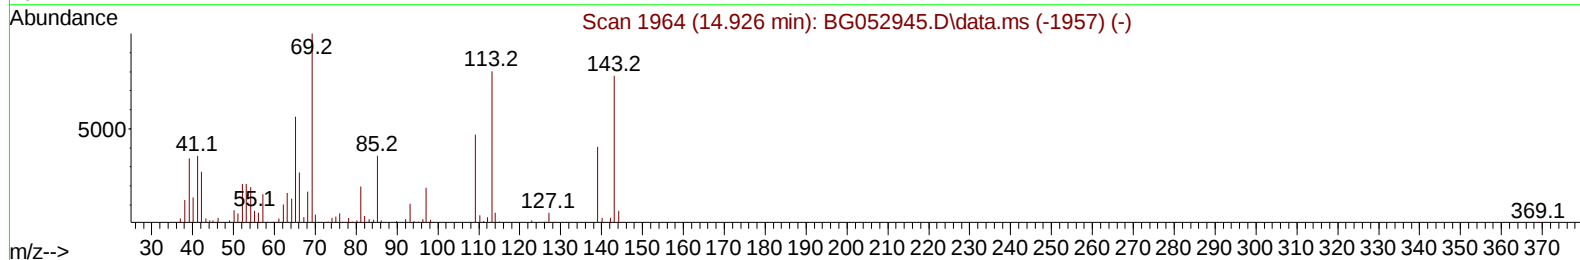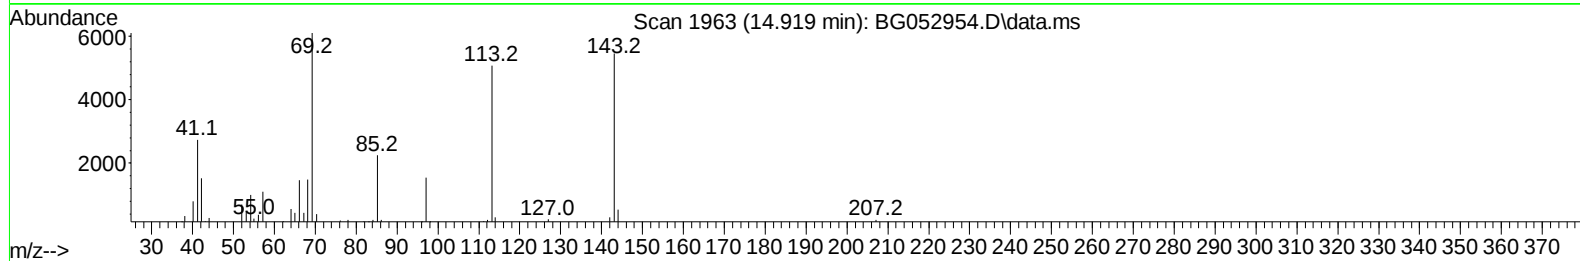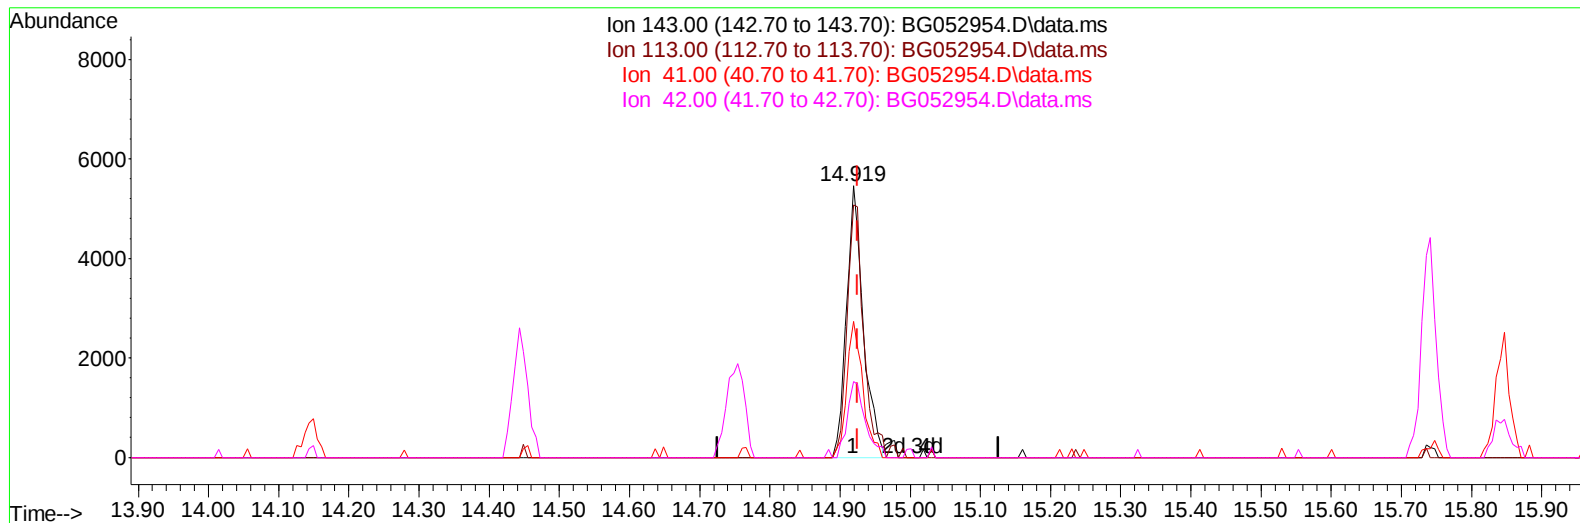

TIC: BG052954.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.919min (-0.007) 7.45 ng/u1

response 9115

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	92.94
41.00	47.20	50.10
42.00	29.40	27.87




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052954.D
Acq On : 30 Mar 2022 18:05
Operator : CG/JU
Sample : N2068-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYX0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

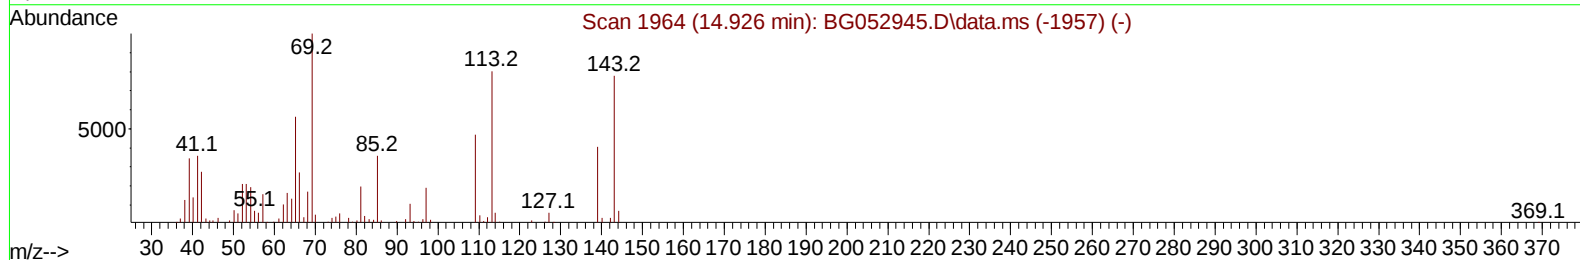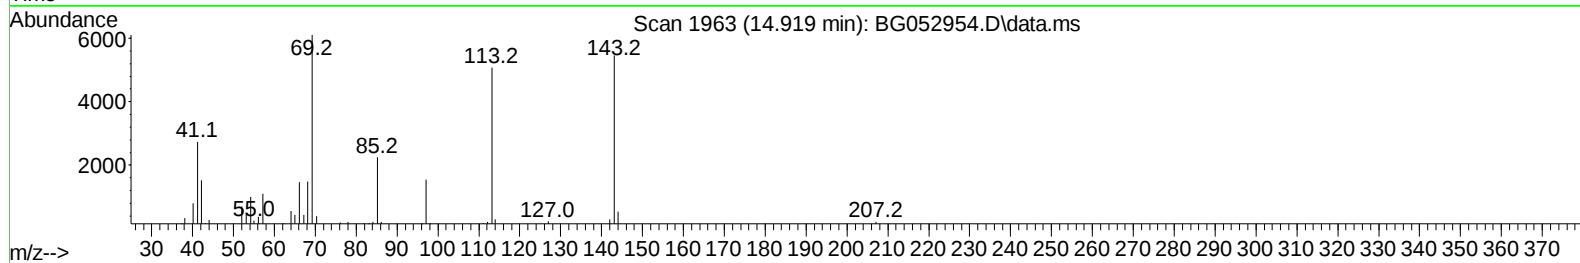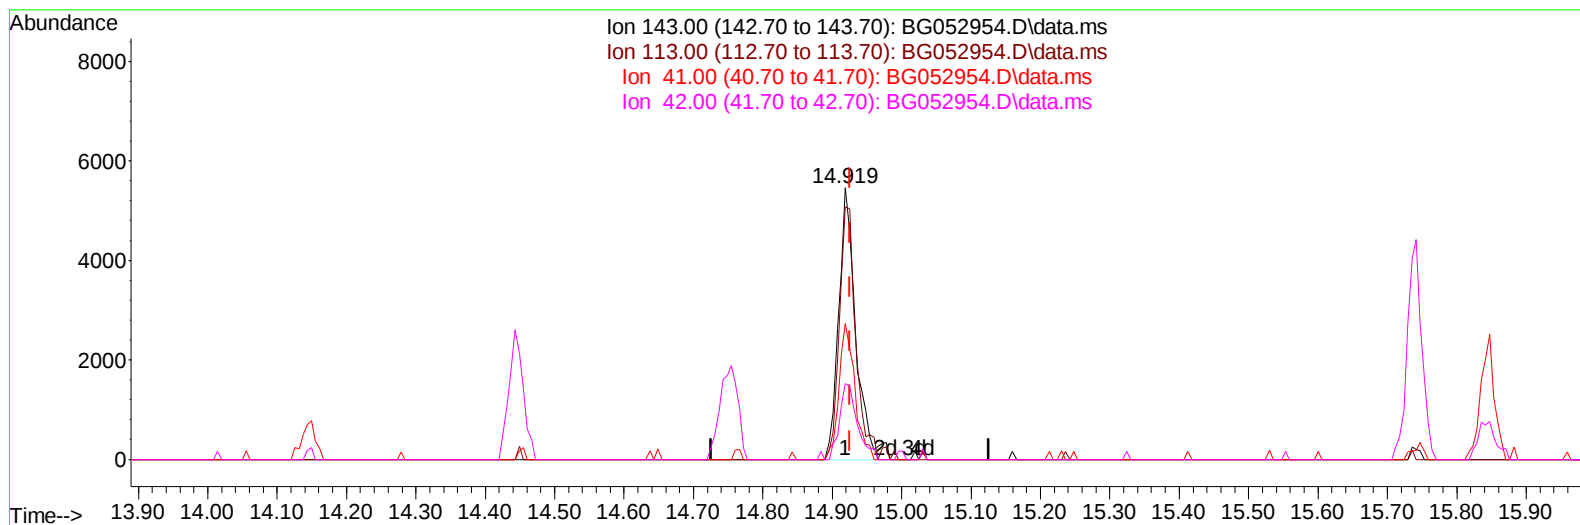

TIC: BG052954.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.919min (-0.007) 7.72 ng/ul m

response 9440

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	92.94
41.00	47.20	50.10
42.00	29.40	27.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052954.D
 Acq On : 30 Mar 2022 18:05
 Operator : CG/JU
 Sample : N2068-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYX0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	30736	20.000	ng/ul	0.00
20) Naphthalene-d8	10.948	136	126212	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.754	164	94700	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	229941	20.000	ng/ul	0.00
79) Chrysene-d12	21.774	240	255507	20.000	ng/ul	0.00
88) Perylene-d12	25.082	264	259702	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.552	96	4204	4.831	ng/uL	0.00
4) Pyridine-d5	3.975	84	10311	4.747	ng/ul	0.01
7) Phenol-d5	7.276	99	18668	6.781	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	55924	33.262	ng/ul	0.00
11) 2-Chlorophenol-d4	7.658	132	45215	24.189	ng/ul	0.00
15) 4-Methylphenol-d8	8.827	113	31112	15.602	ng/ul	0.00
21) Nitrobenzene-d5	9.291	128	31208	34.350	ng/ul	0.00
24) 2-Nitrophenol-d4	10.014	143	33682	35.149	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.560	165	57964	27.804	ng/ul	0.00
31) 4-Chloroaniline-d4	11.065	131	67784	24.601	ng/ul	0.00
46) Dimethylphthalate-d6	14.149	166	252342	34.685	ng/ul	0.00
49) Acenaphthylene-d8	14.449	160	272993	30.880	ng/ul	0.00
54) 4-Nitrophenol-d4	14.919	143	9440m	7.717	ng/ul	0.00
60) Fluorene-d10	15.741	176	223377	34.968	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.847	200	45420	38.815	ng/ul	0.00
73) Anthracene-d10	17.592	188	402359	37.577	ng/ul	0.00
81) Pyrene-d10	19.877	212	506639	35.445	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.858	264	499402	37.216	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052954.D
Acq On : 30 Mar 2022 18:05
Operator : CG/JU
Sample : N2068-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYX0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

