




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052957.D
Acq On : 30 Mar 2022 20:00
Operator : CG/JU
Sample : N2120-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHT0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

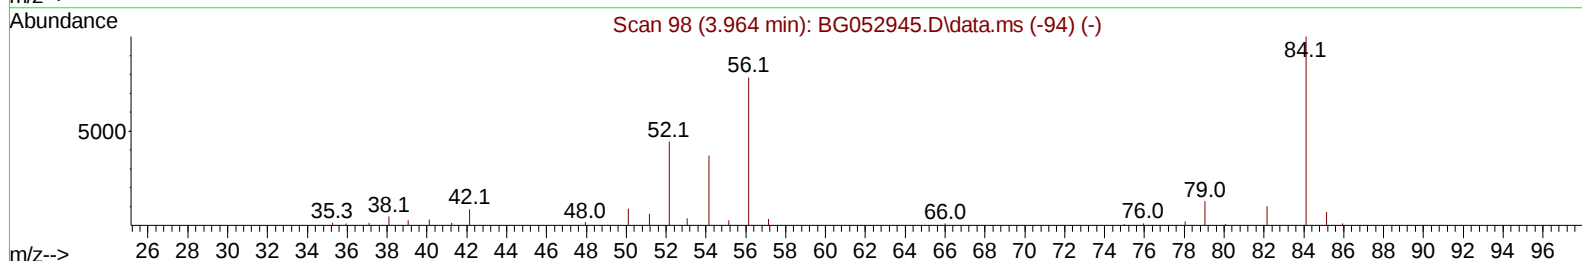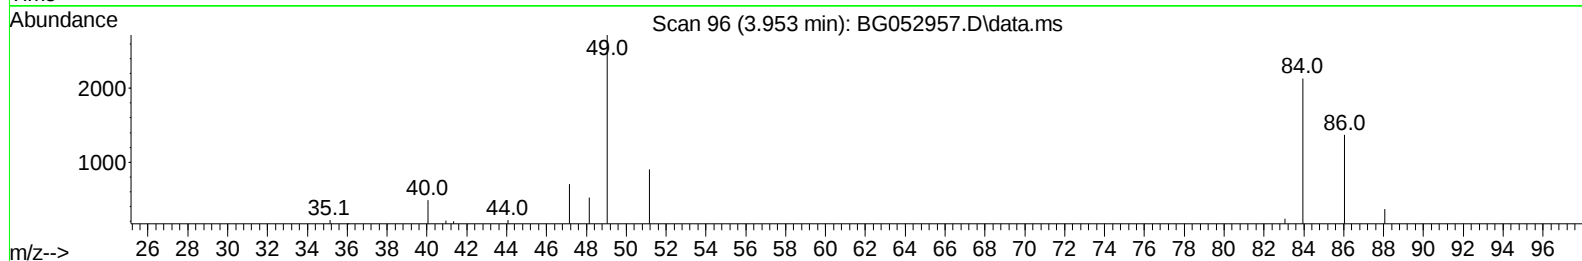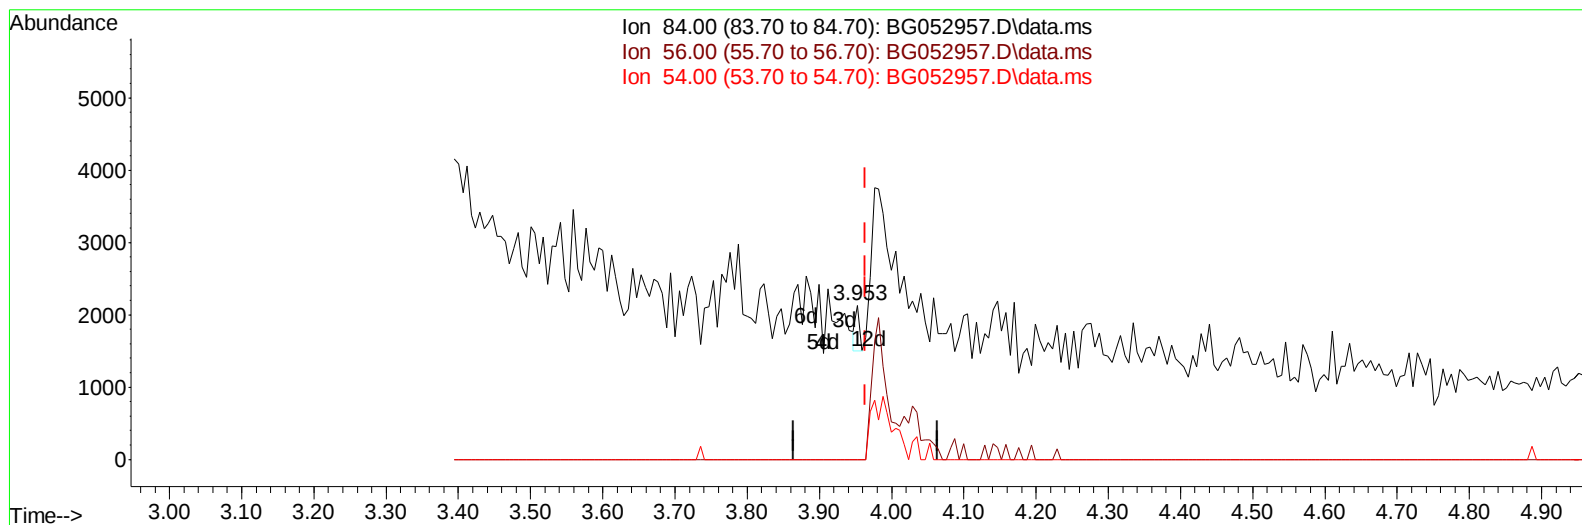

TIC: BG052957.D\data.ms

(4) Pyridine-d5 (S)

3.953min (-0.011) 0.13 ng/u1

response 223

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	0.00#
54.00	28.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052957.D
 Acq On : 30 Mar 2022 20:00
 Operator : CG/JU
 Sample : N2120-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 3

Instrument :
 BNA_G
 ClientSampleId :
 COHT0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

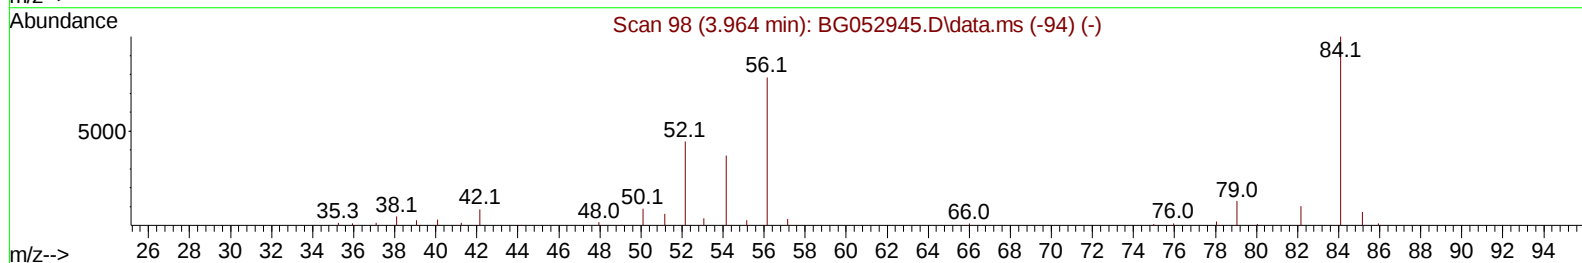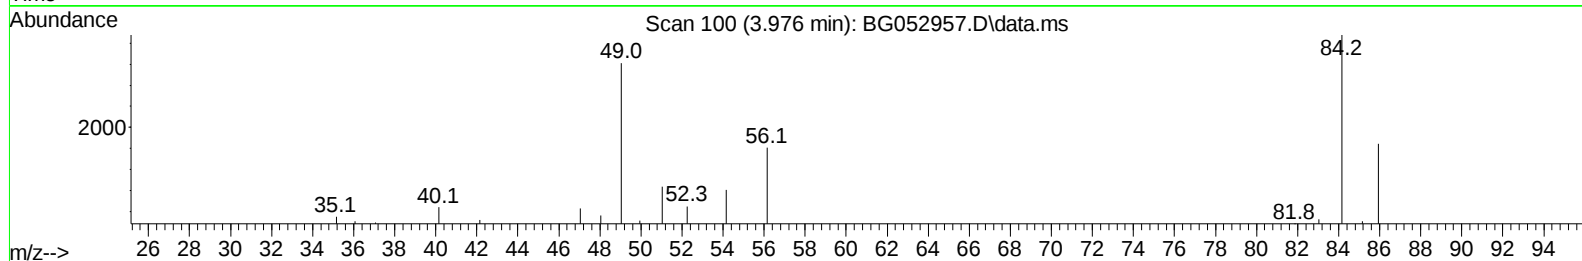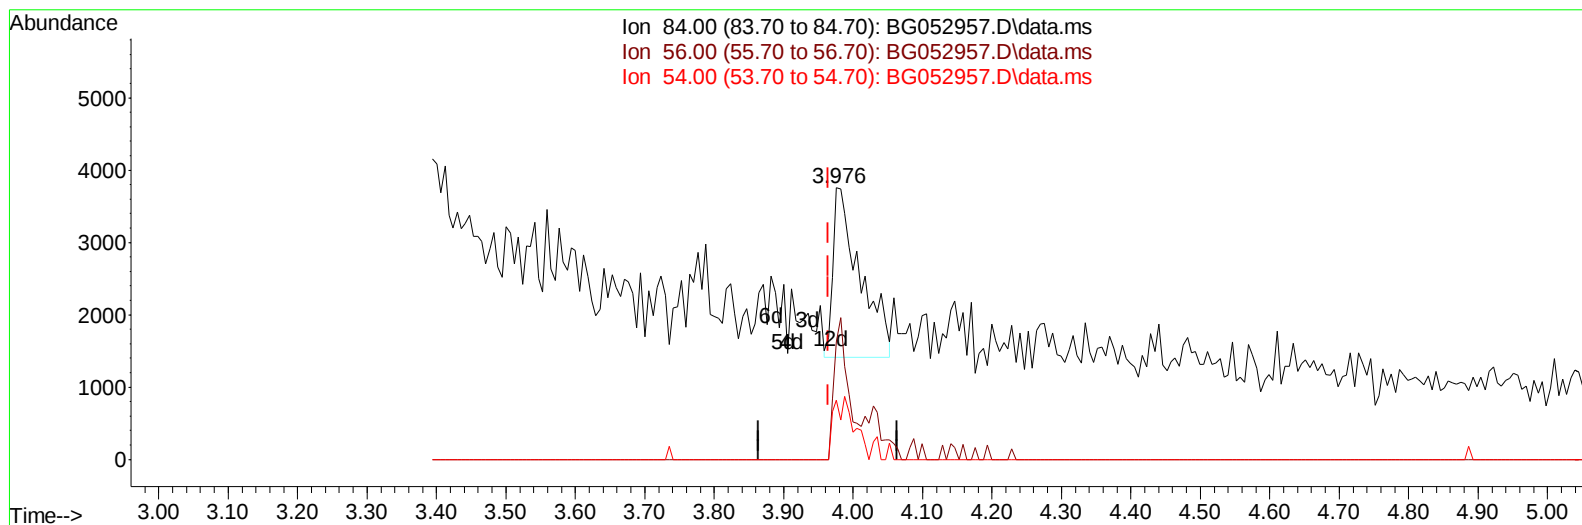

TIC: BG052957.D\data.ms

(4) Pyridine-d5 (S)

3.976min (+ 0.012) 3.73 ng/u1 m

response 6328

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.20	43.21#
54.00	28.70	21.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052957.D
Acq On : 30 Mar 2022 20:00
Operator : CG/JU
Sample : N2120-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHT0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

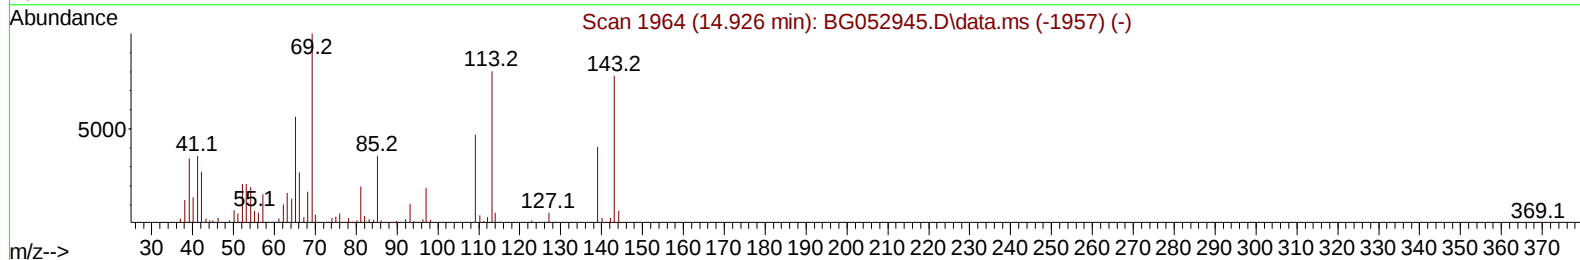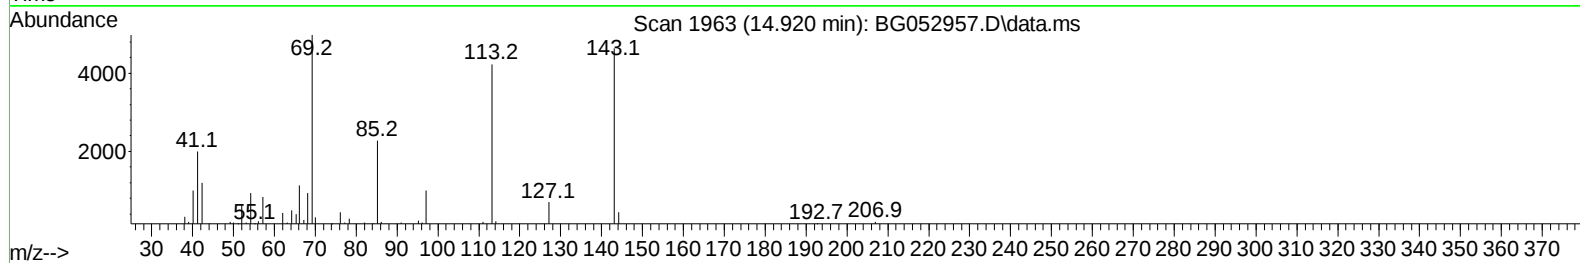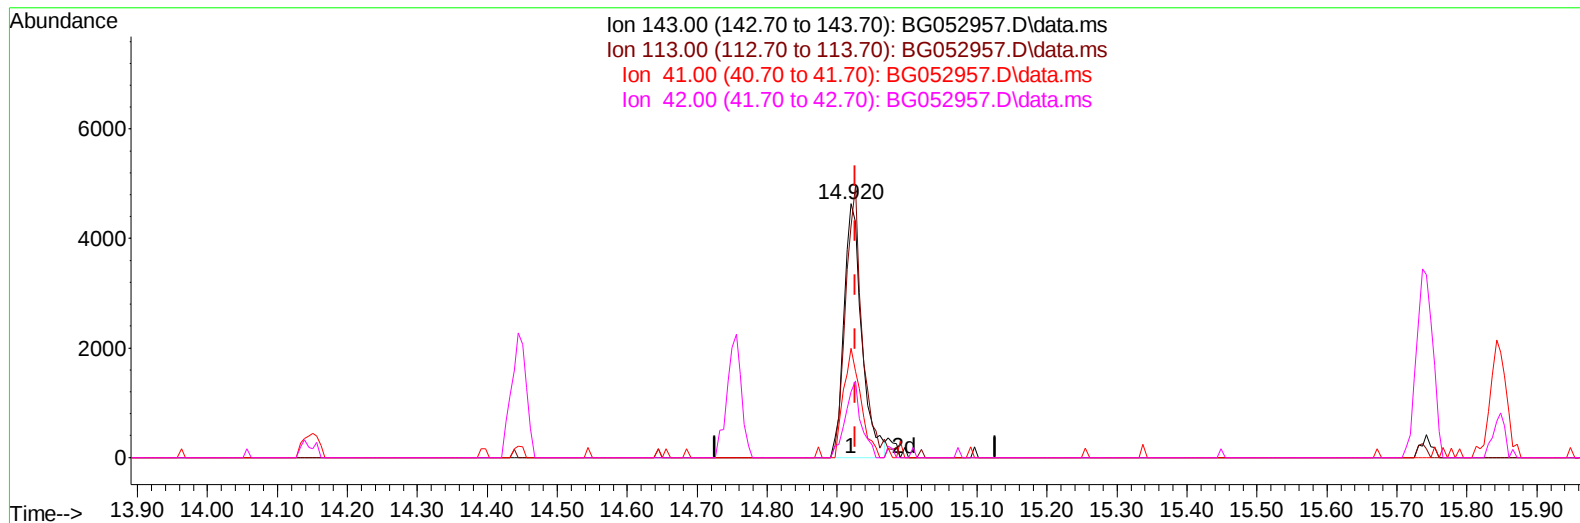

TIC: BG052957.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.920min (-0.006) 8.08 ng/u1

response 8224

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	91.22
41.00	47.20	43.10
42.00	29.40	25.94




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052957.D
Acq On : 30 Mar 2022 20:00
Operator : CG/JU
Sample : N2120-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHT0

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:53:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

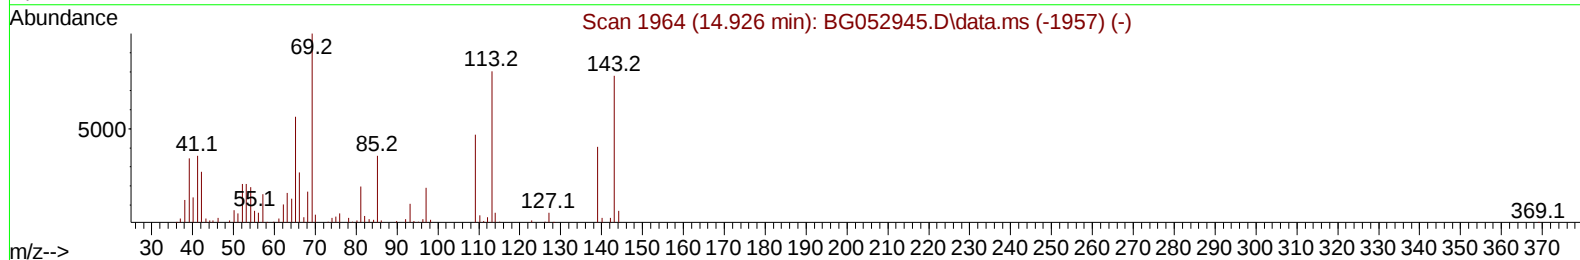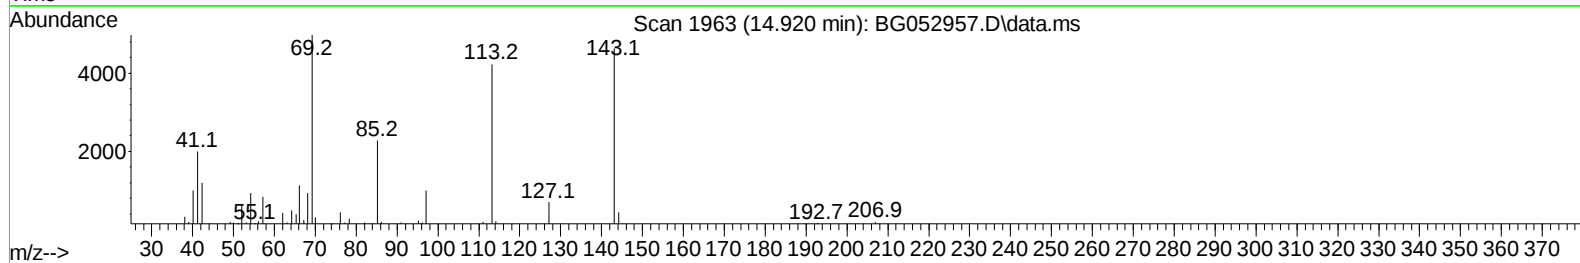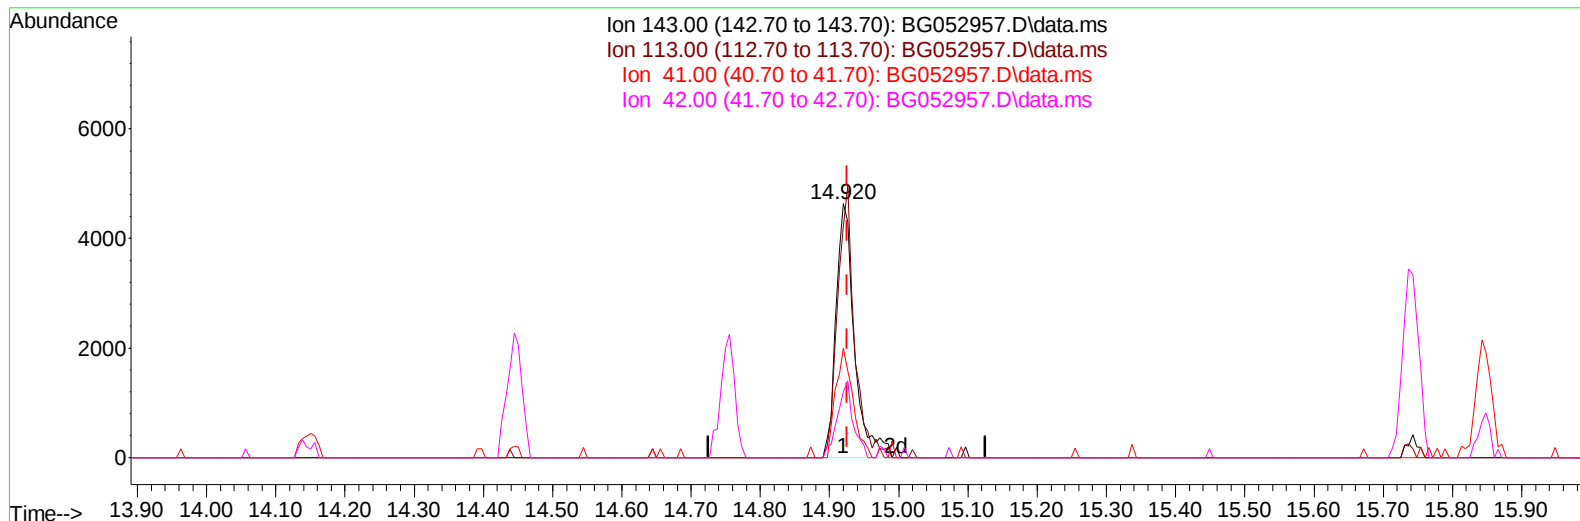

TIC: BG052957.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.920min (-0.006) 8.38 ng/ul m

response 8529

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	91.22
41.00	47.20	43.10
42.00	29.40	25.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052957.D
 Acq On : 30 Mar 2022 20:00
 Operator : CG/JU
 Sample : N2120-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 COHT0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Mar 31 00:53:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	23999	20.000	ng/ul	0.00
20) Naphthalene-d8	10.943	136	100575	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.750	164	78822	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.493	188	203779	20.000	ng/ul	0.00
79) Chrysene-d12	21.775	240	234628	20.000	ng/ul	0.00
88) Perylene-d12	25.083	264	230141	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	3522	5.184	ng/uL	0.00
4) Pyridine-d5	3.976	84	6328m	3.731	ng/ul	0.01
7) Phenol-d5	7.277	99	14626	6.804	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.448	67	46809	35.656	ng/ul	0.00
11) 2-Chlorophenol-d4	7.659	132	36219	24.816	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	26382	16.943	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128	25573	35.323	ng/ul	0.00
24) 2-Nitrophenol-d4	10.021	143	27713	36.292	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.555	165	47236	28.434	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	29129	13.267	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	224646	37.098	ng/ul	0.00
49) Acenaphthylene-d8	14.444	160	240843	32.731	ng/ul	0.00
54) 4-Nitrophenol-d4	14.920	143	8529m	8.377	ng/ul	0.00
60) Fluorene-d10	15.742	176	201288	37.858	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	40215	38.779	ng/ul	0.00
73) Anthracene-d10	17.593	188	379832	40.028	ng/ul	0.00
81) Pyrene-d10	19.872	212	499460	38.052	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.860	264	495125	41.637	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052957.D
Acq On : 30 Mar 2022 20:00
Operator : CG/JU
Sample : N2120-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
COHT0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Mar 31 00:53:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

