




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052960.D
Acq On : 30 Mar 2022 22:35
Operator : CG/JU
Sample : PB143705BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK705

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:54:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

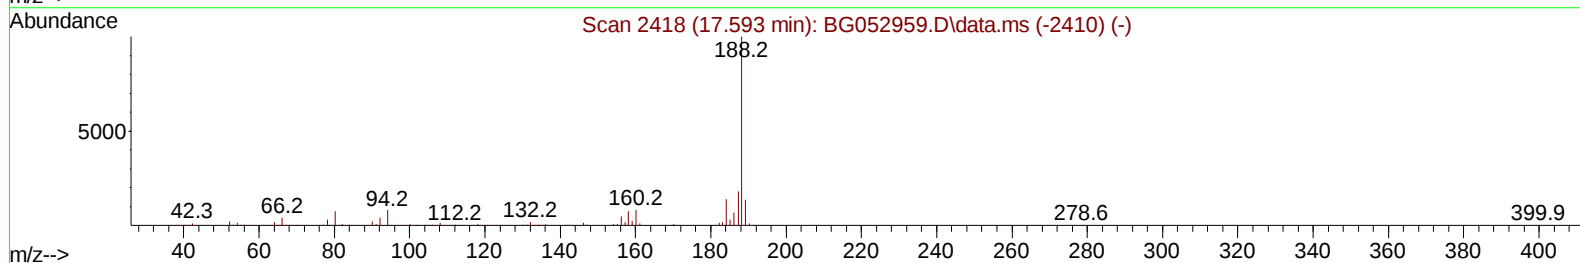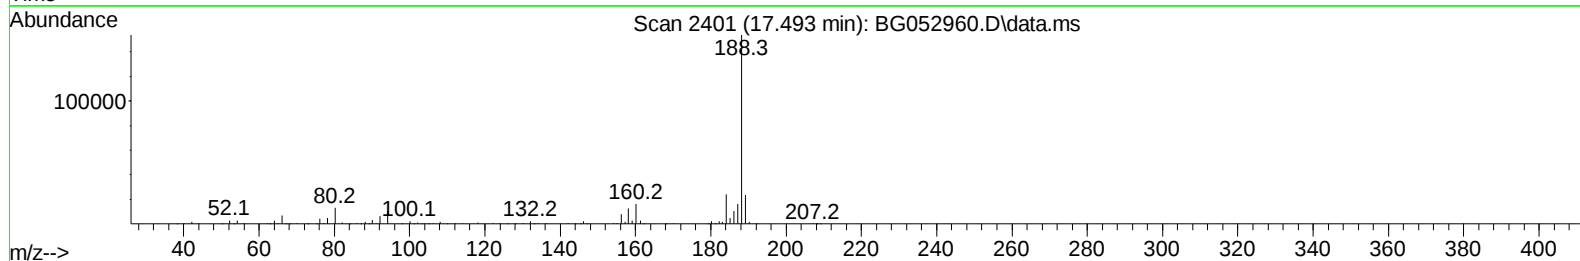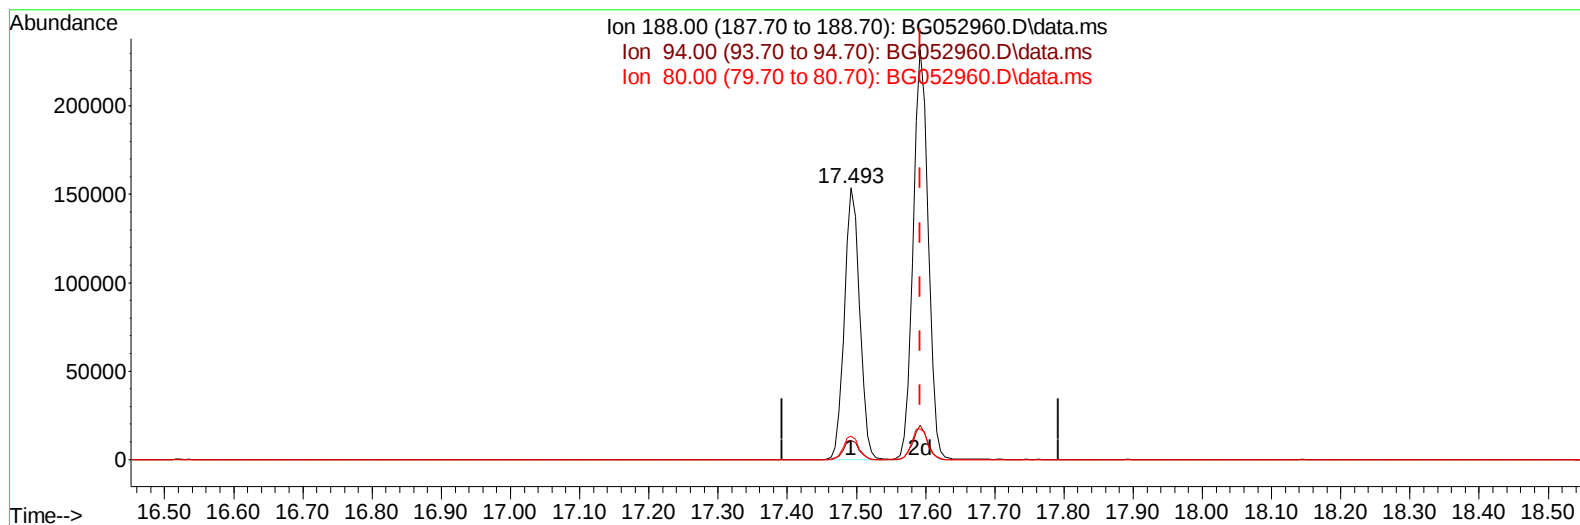

TIC: BG052960.D\data.ms

(73) Anthracene-d10 (S)

17.493min (-0.100) 21.47 ng/u1

response 234124

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	6.88
80.00	9.50	8.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052960.D
 Acq On : 30 Mar 2022 22:35
 Operator : CG/JU
 Sample : PB143705BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK705

Manual IntegrationsAPPROVED

Quant Time: Mar 31 00:54:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

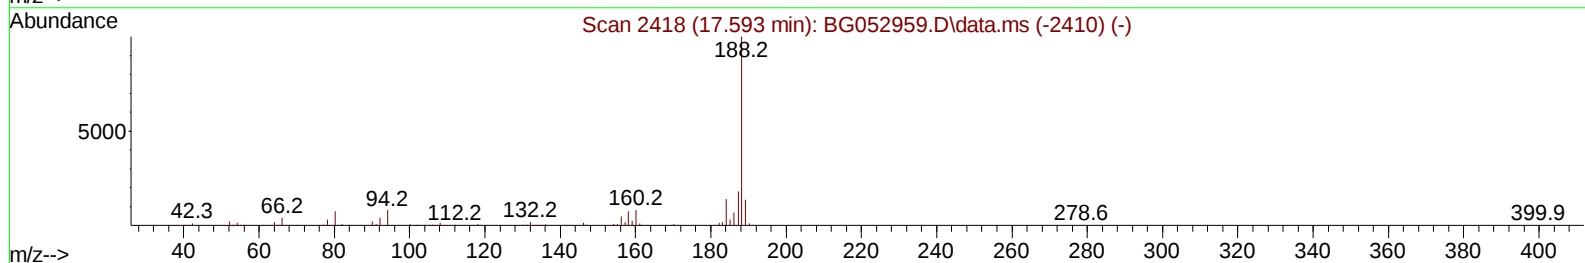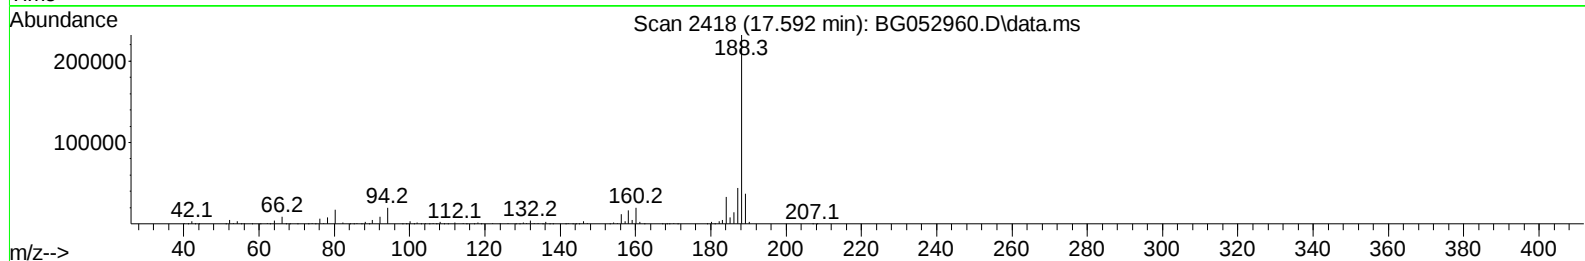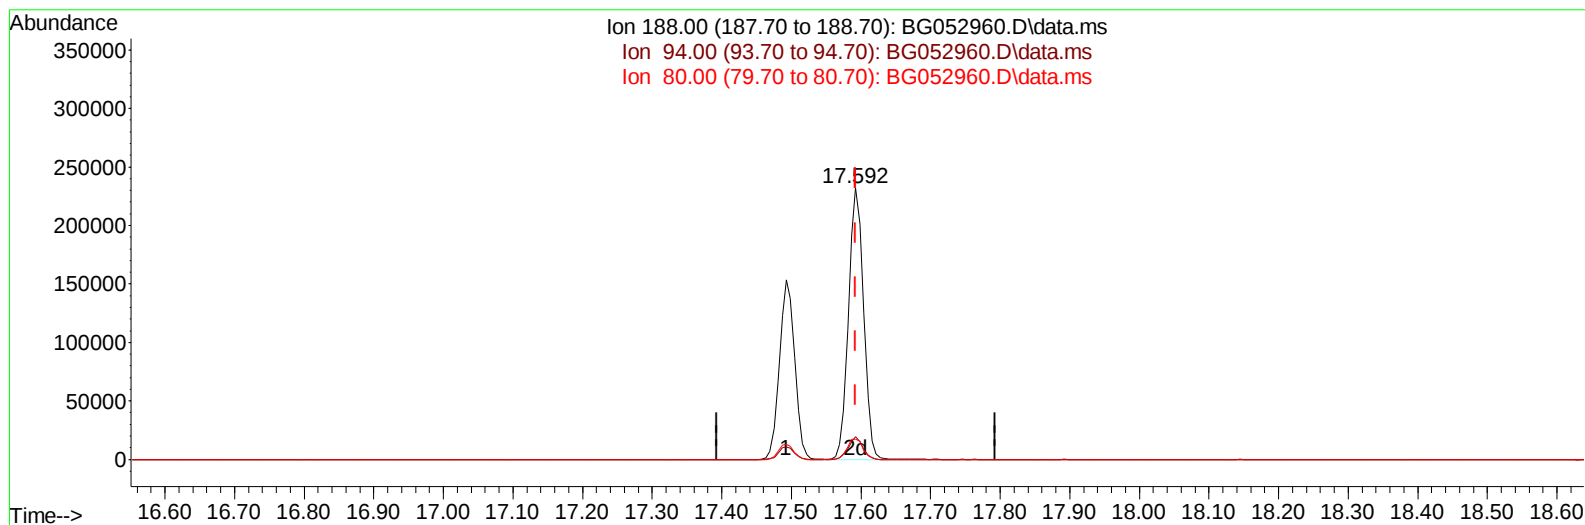

TIC: BG052960.D\data.ms

(73) Anthracene-d10 (S)

17.592min (-0.000) 32.10 ng/u1 m

response 350004

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.90	8.43
80.00	9.50	7.38#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052960.D
 Acq On : 30 Mar 2022 22:35
 Operator : CG/JU
 Sample : PB143705BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK705

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Mar 31 00:54:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	27725	20.000	ng/ul	# 0.00
20) Naphthalene-d8	10.943	136	118199	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.749	164	95006	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.493	188	234124	20.000	ng/ul	0.00
79) Chrysene-d12	21.775	240	250112	20.000	ng/ul	0.00
88) Perylene-d12	25.082	264	247661	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	4537	5.780	ng/uL	0.00
4) Pyridine-d5	3.964	84	54569	27.848	ng/ul	0.00
7) Phenol-d5	7.277	99	72870	29.345	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	48435	31.936	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	50253	29.804	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	57278	31.842	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	28135	33.067	ng/ul	0.00
24) 2-Nitrophenol-d4	10.014	143	31175	34.738	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.555	165	55507	28.431	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	80724	31.284	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	239869	32.864	ng/ul	0.00
49) Acenaphthylene-d8	14.444	160	256764	28.950	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	37545	30.595	ng/ul	0.00
60) Fluorene-d10	15.742	176	199790	31.175	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.842	200	37935	31.839	ng/ul	0.00
73) Anthracene-d10	17.592	188	350004m	32.104	ng/ul	0.00
81) Pyrene-d10	19.872	212	436595	31.204	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.853	264	416136	32.519	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052960.D
Acq On : 30 Mar 2022 22:35
Operator : CG/JU
Sample : PB143705BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK705

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/31/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Mar 31 00:54:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

