




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052971.D
 Acq On : 31 Mar 2022 9:17
 Operator : CG/JU
 Sample : PB143753BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK753

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:16:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

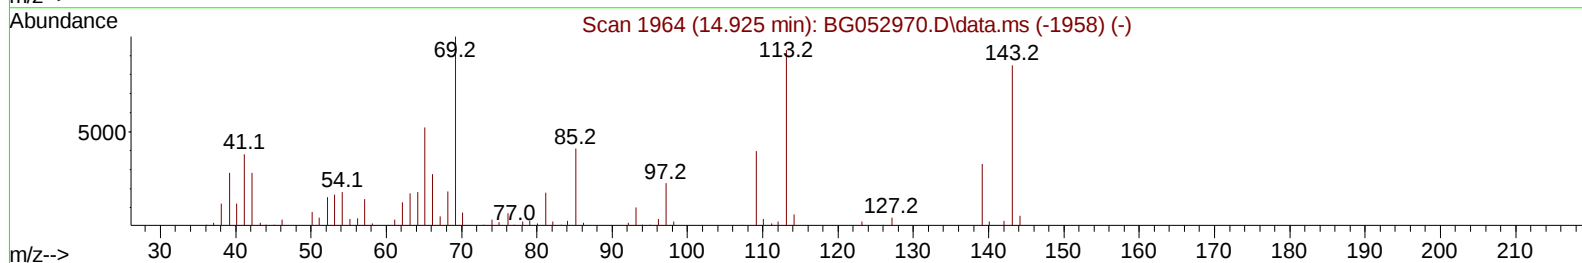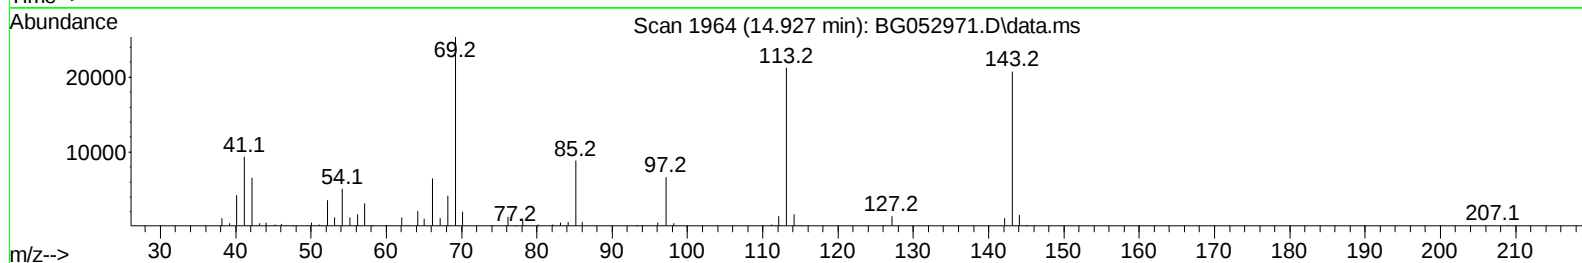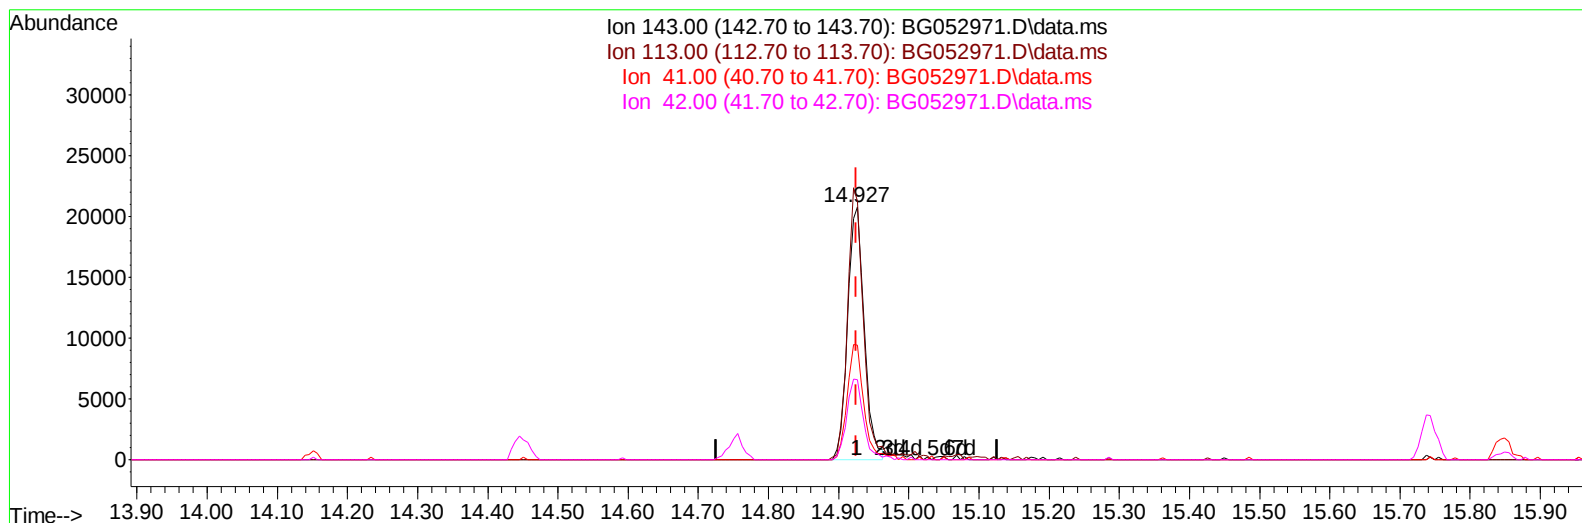

TIC: BG052971.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.927min (+ 0.001) 28.85 ng/u1

response 34287

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	102.39
41.00	47.20	45.25
42.00	29.40	31.51




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052971.D
Acq On : 31 Mar 2022 9:17
Operator : CG/JU
Sample : PB143753BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK753

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:16:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

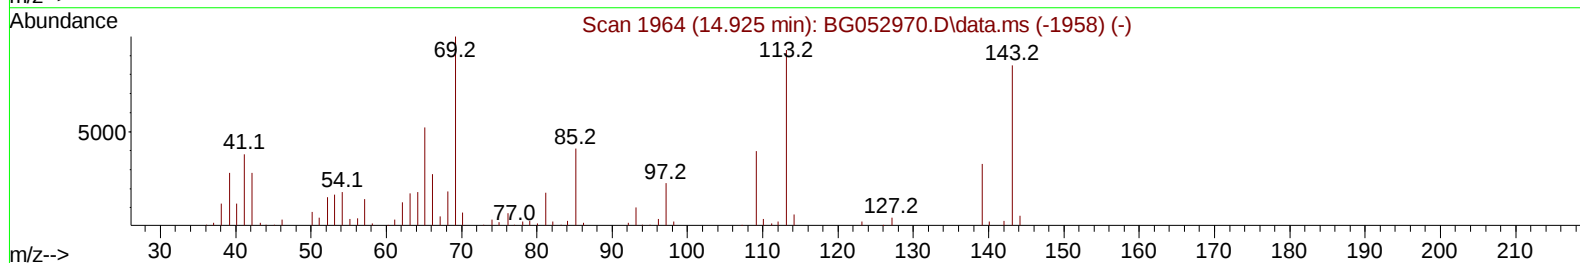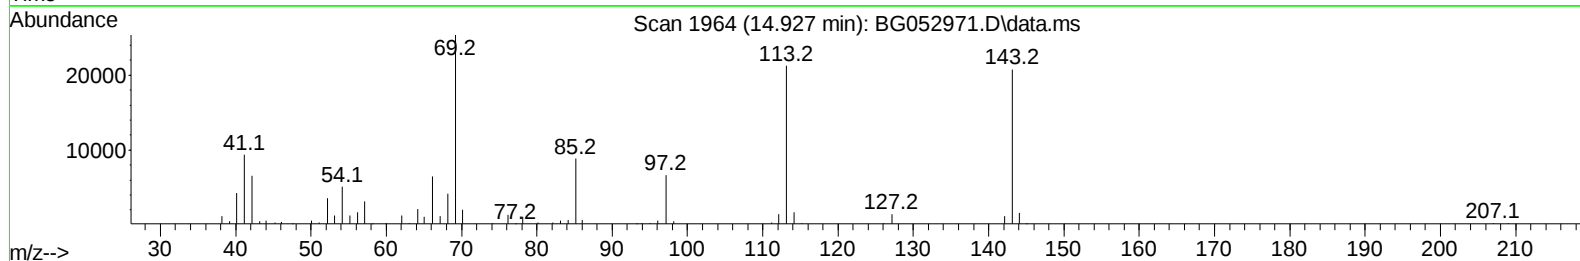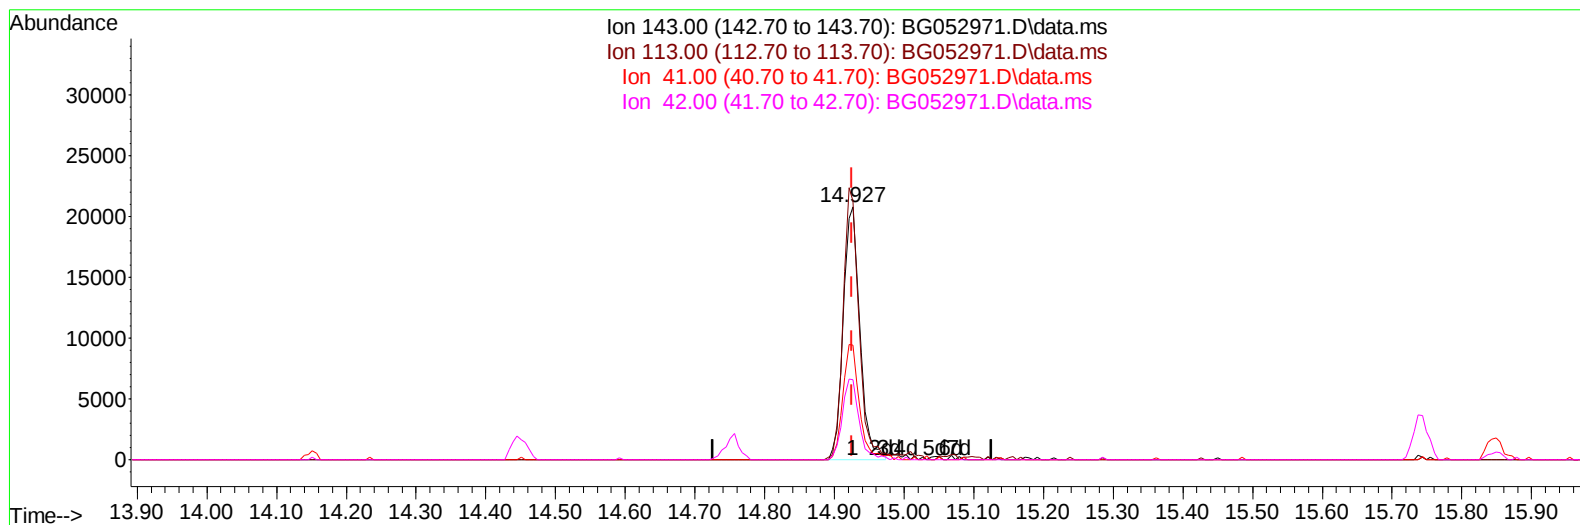

TIC: BG052971.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.927min (+ 0.001) 29.25 ng/ul m

response 34757

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	102.39
41.00	47.20	45.25
42.00	29.40	31.51

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052971.D
 Acq On : 31 Mar 2022 9:17
 Operator : CG/JU
 Sample : PB143753BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK753

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:16:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.130	152	24807	20.000	ng/ul	0.00
20) Naphthalene-d8	10.944	136	107739	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.756	164	92007	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.494	188	233348	20.000	ng/ul	0.00
79) Chrysene-d12	21.782	240	250636	20.000	ng/ul	0.00
88) Perylene-d12	25.084	264	242713	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.542	96	3636	5.177	ng/uL	0.00
4) Pyridine-d5	3.959	84	45728	26.081	ng/ul	0.00
7) Phenol-d5	7.278	99	63128	28.412	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.449	67	43474	32.037	ng/ul	0.00
11) 2-Chlorophenol-d4	7.660	132	44570	29.543	ng/ul	0.00
15) 4-Methylphenol-d8	8.823	113	49986	31.057	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	24686	31.830	ng/ul	0.00
24) 2-Nitrophenol-d4	10.016	143	26246	32.085	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.556	165	49061	27.569	ng/ul	0.00
31) 4-Chloroaniline-d4	11.067	131	71289	30.310	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	217762	30.808	ng/ul	0.00
49) Acenaphthylene-d8	14.445	160	230469	26.833	ng/ul	0.00
54) 4-Nitrophenol-d4	14.927	143	34757m	29.246	ng/ul	0.00
60) Fluorene-d10	15.743	176	186956	30.123	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.849	200	34523	29.072	ng/ul	0.00
73) Anthracene-d10	17.594	188	331103	30.471	ng/ul	0.00
81) Pyrene-d10	19.879	212	411475	29.347	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.866	264	384186	30.634	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052971.D
Acq On : 31 Mar 2022 9:17
Operator : CG/JU
Sample : PB143753BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK753

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:16:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

