




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052974.D
 Acq On : 31 Mar 2022 11:14
 Operator : CG/JU
 Sample : N2160-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ30

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:02:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

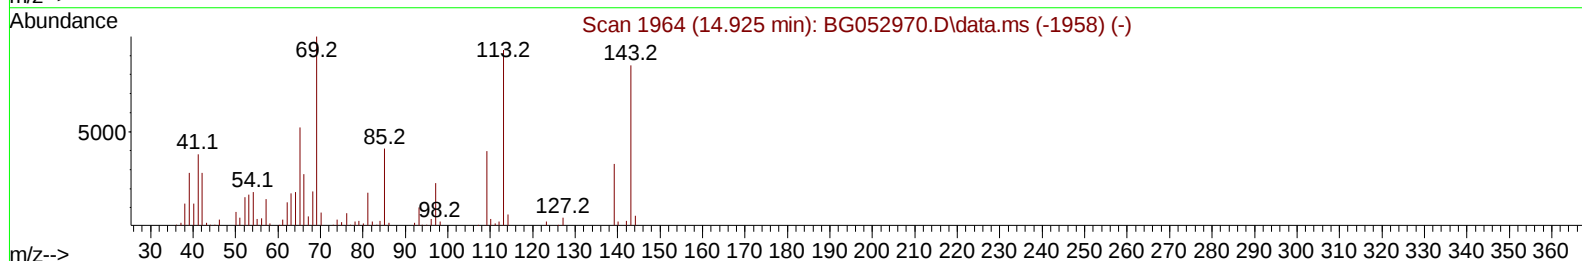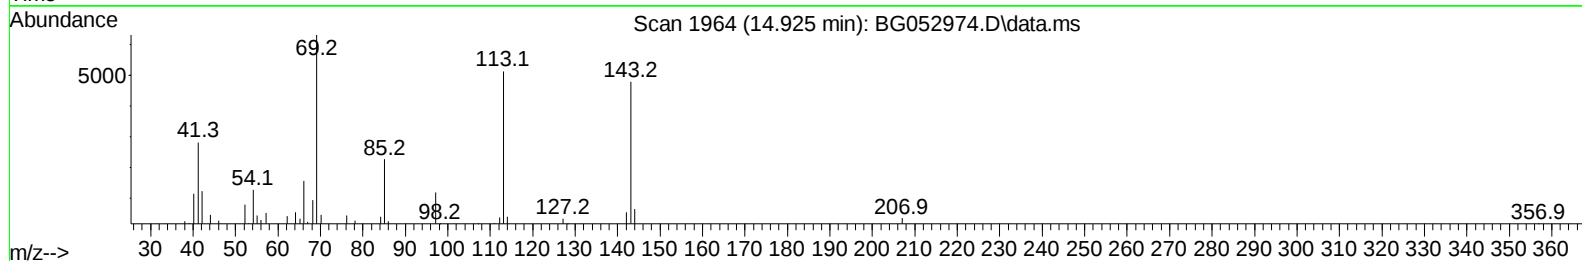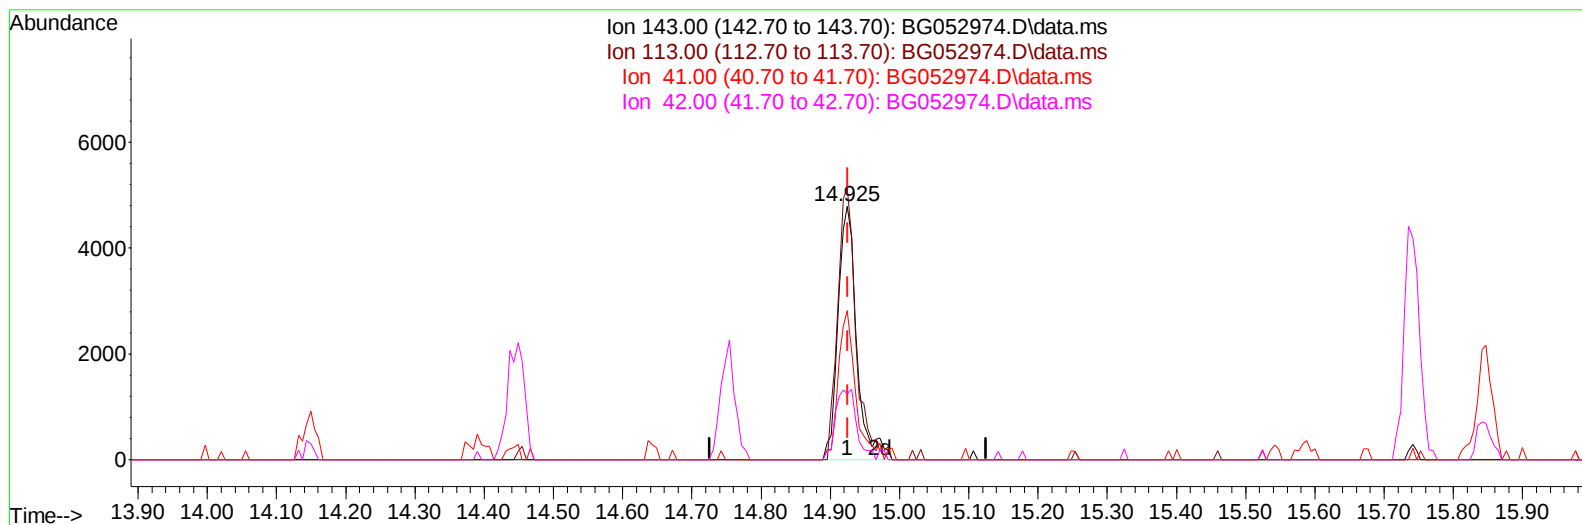

TIC: BG052974.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.001) 8.65 ng/ul m

response 8959

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	107.24
41.00	47.20	58.77#
42.00	29.40	25.83

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052974.D
 Acq On : 31 Mar 2022 11:14
 Operator : CG/JU
 Sample : N2160-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ30

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:02:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.134	152	22637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.942	136	101411	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.754	164	80147	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	196264	20.000	ng/ul	0.00
79) Chrysene-d12	21.774	240	209204	20.000	ng/ul	# 0.00
88) Perylene-d12	25.082	264	211933	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	3234	5.046	ng/uL	0.00
4) Pyridine-d5	3.969	84	15365	9.604	ng/ul	0.00
7) Phenol-d5	7.276	99	18194	8.974	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.447	67	49353	39.855	ng/ul	0.00
11) 2-Chlorophenol-d4	7.664	132	40695	29.560	ng/ul	0.00
15) 4-Methylphenol-d8	8.827	113	32817	22.344	ng/ul	0.00
21) Nitrobenzene-d5	9.291	128	30414	41.663	ng/ul	0.00
24) 2-Nitrophenol-d4	10.014	143	30980	40.236	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.554	165	53678	32.046	ng/ul	0.00
31) 4-Chloroaniline-d4	11.065	131	69660	31.465	ng/ul	0.00
46) Dimethylphthalate-d6	14.149	166	254037	41.258	ng/ul	0.00
49) Acenaphthylene-d8	14.449	160	268729	35.917	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	8959m	8.654	ng/ul	0.00
60) Fluorene-d10	15.741	176	222979	41.244	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.847	200	44888	44.943	ng/ul	0.00
73) Anthracene-d10	17.592	188	393281	43.032	ng/ul	0.00
81) Pyrene-d10	19.877	212	475357	40.617	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.858	264	476031	43.471	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052974.D
Acq On : 31 Mar 2022 11:14
Operator : CG/JU
Sample : N2160-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAZ30

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:02:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

