




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052980.D
Acq On : 31 Mar 2022 15:07
Operator : CG/JU
Sample : N2160-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:03:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

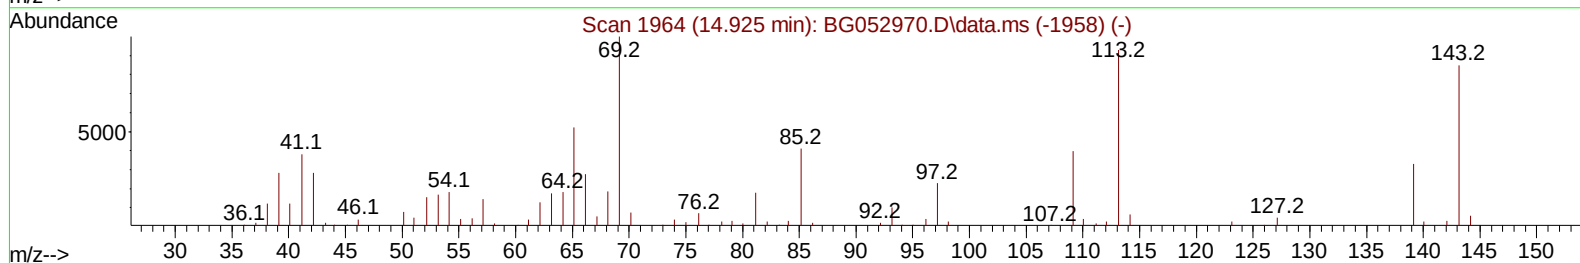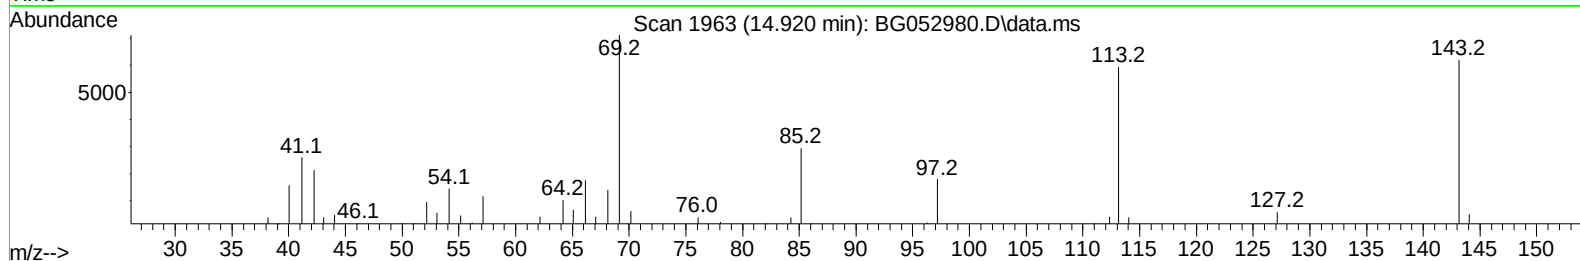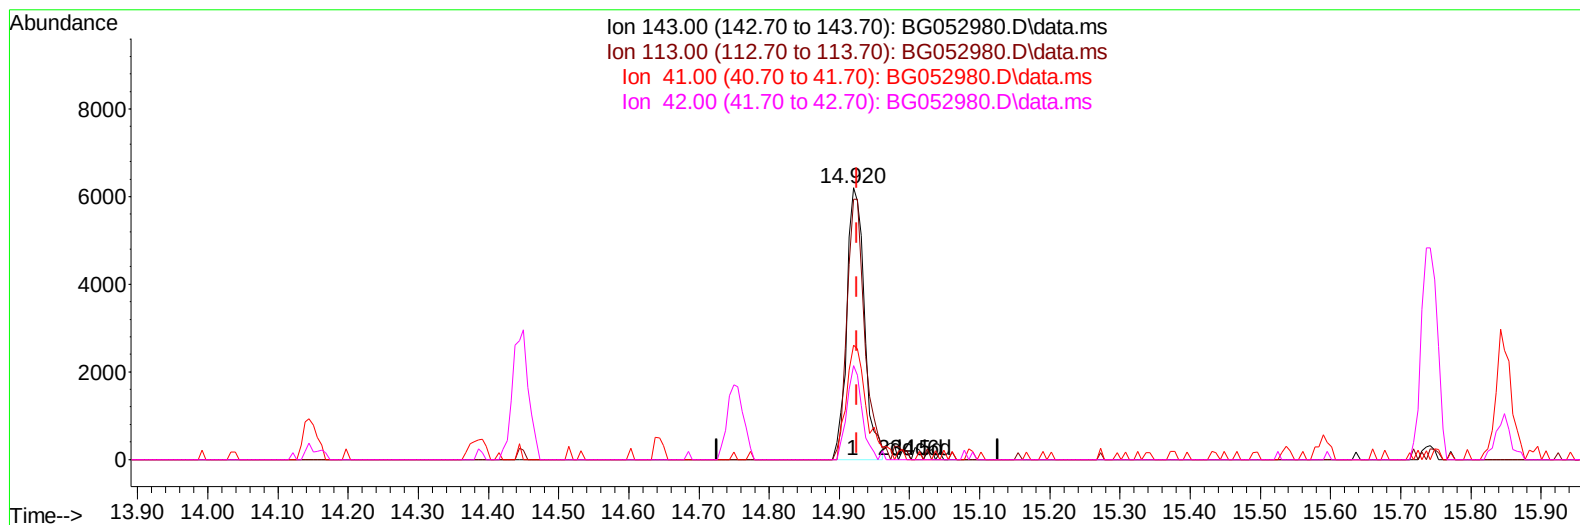

TIC: BG052980.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.920min (-0.006) 11.02 ng/ul

response 10858

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	95.93
41.00	47.20	42.01
42.00	29.40	34.54




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052980.D
 Acq On : 31 Mar 2022 15:07
 Operator : CG/JU
 Sample : N2160-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:03:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

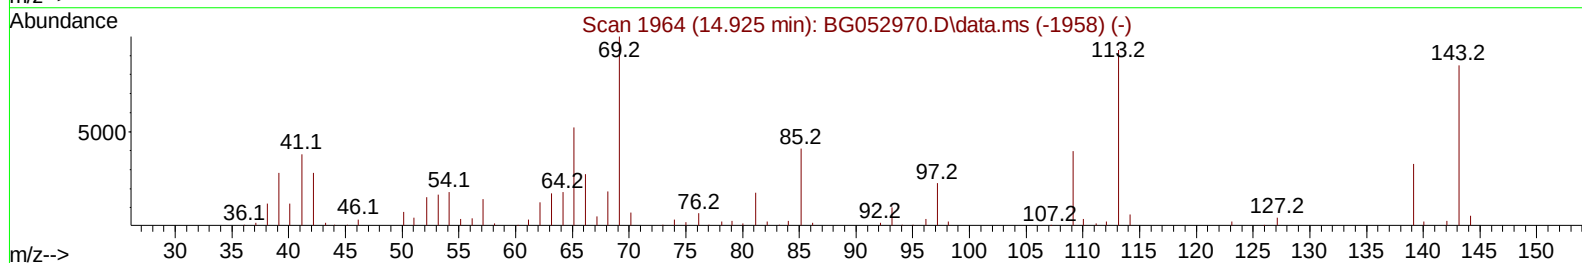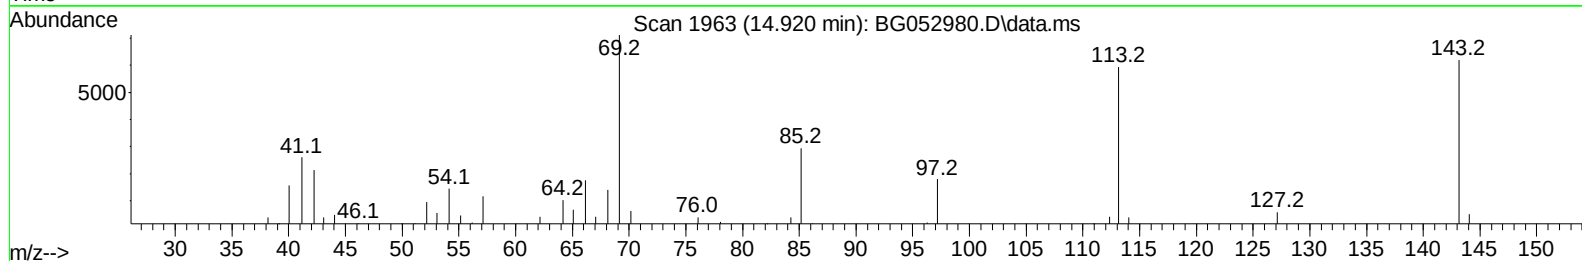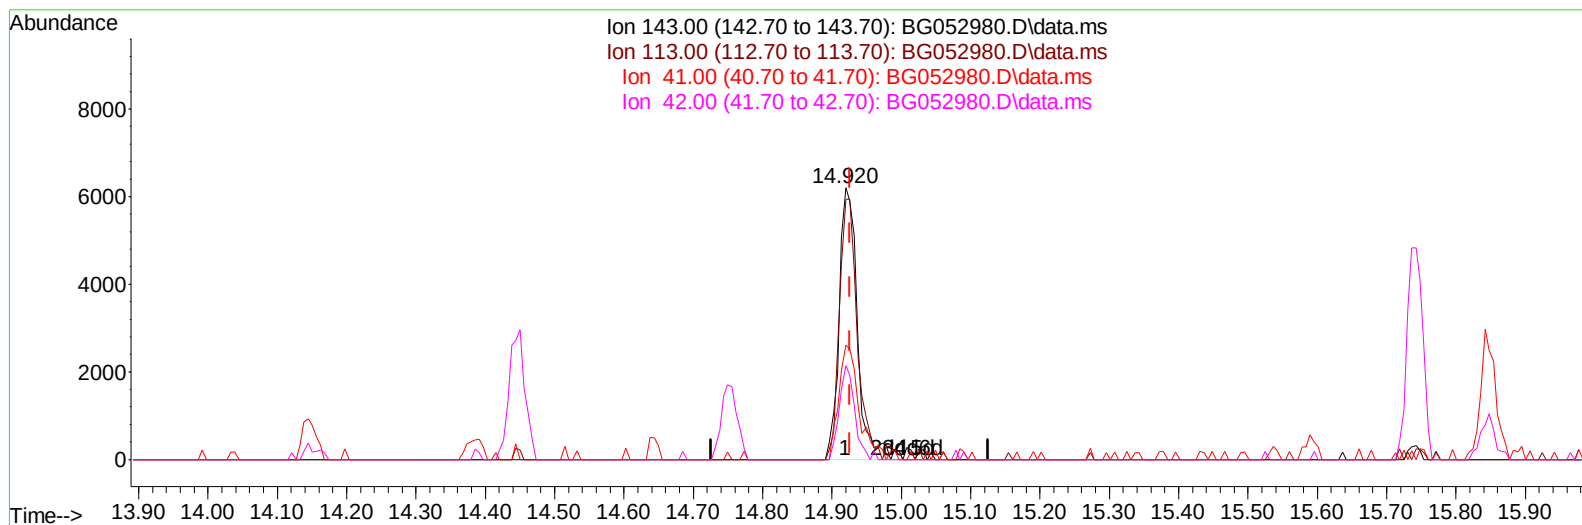

TIC: BG052980.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.920min (-0.006) 11.38 ng/ul m

response 11213

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	95.93
41.00	47.20	42.01
42.00	29.40	34.54

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052980.D
 Acq On : 31 Mar 2022 15:07
 Operator : CG/JU
 Sample : N2160-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:03:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	21289	20.000	ng/ul	0.00
20) Naphthalene-d8	10.949	136	95537	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.749	164	76285	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.493	188	185457	20.000	ng/ul	0.00
79) Chrysene-d12	21.775	240	200629	20.000	ng/ul	0.00
88) Perylene-d12	25.083	264	204104	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.553	96	3461	5.743	ng/uL	0.00
4) Pyridine-d5	3.964	84	19118	12.706	ng/ul	0.00
7) Phenol-d5	7.277	99	23601	12.378	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.448	67	61821	53.085	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	51260	39.592	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	43100	31.204	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	36138	52.548	ng/ul	0.00
24) 2-Nitrophenol-d4	10.021	143	38911	53.643	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	69340	43.941	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	81416	39.037	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	297305	50.730	ng/ul	0.00
49) Acenaphthylene-d8	14.450	160	331414	46.538	ng/ul	0.00
54) 4-Nitrophenol-d4	14.920	143	11213m	11.380	ng/ul	0.00
60) Fluorene-d10	15.742	176	266049	51.702	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	53482	56.667	ng/ul	0.00
73) Anthracene-d10	17.593	188	447625	51.832	ng/ul	0.00
81) Pyrene-d10	19.878	212	543837	48.455	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.859	264	549026	52.060	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052980.D
Acq On : 31 Mar 2022 15:07
Operator : CG/JU
Sample : N2160-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:03:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

