




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052990.D
 Acq On : 31 Mar 2022 21:53
 Operator : CG/JU
 Sample : N2160-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ6

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

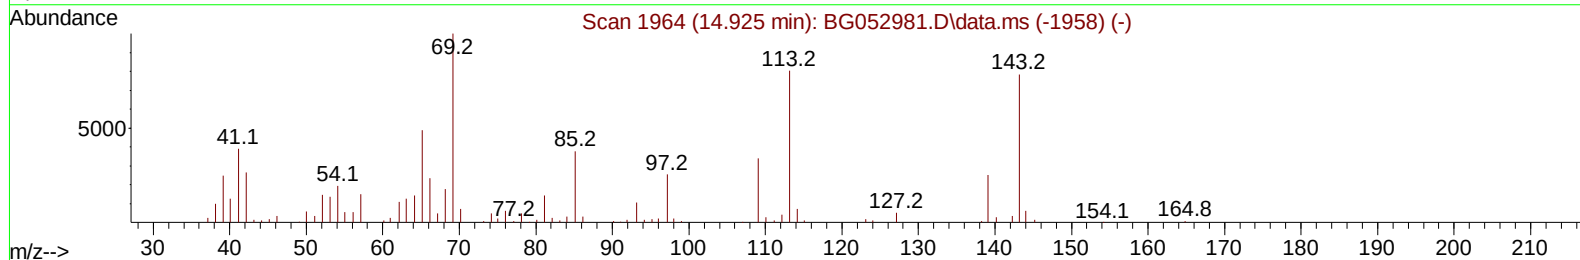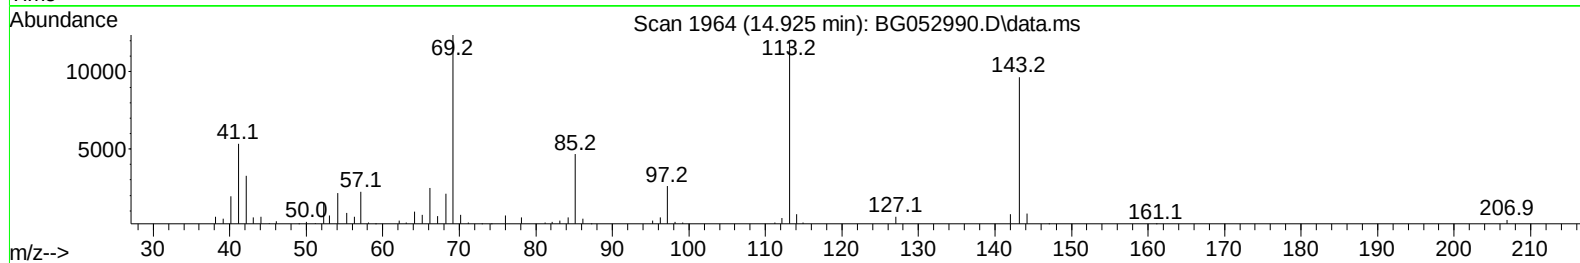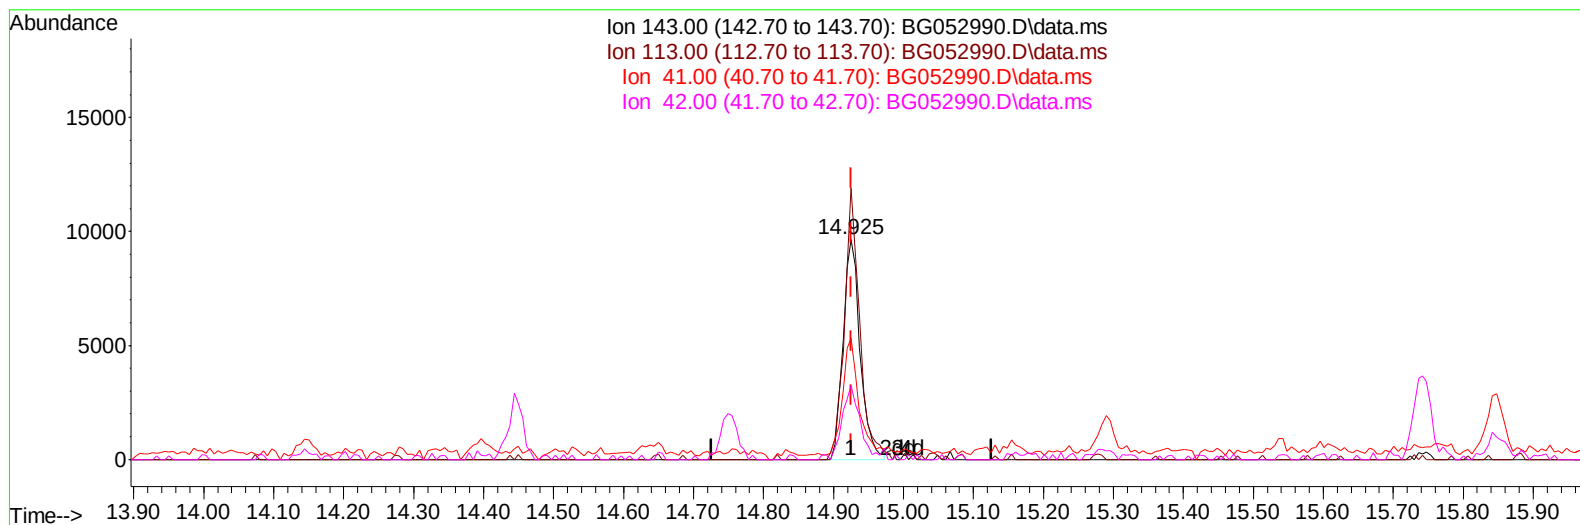

TIC: BG052990.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.000) 14.35 ng/ul

response 16278

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	123.30
41.00	47.20	55.17
42.00	29.40	33.64




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052990.D
 Acq On : 31 Mar 2022 21:53
 Operator : CG/JU
 Sample : N2160-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ6

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

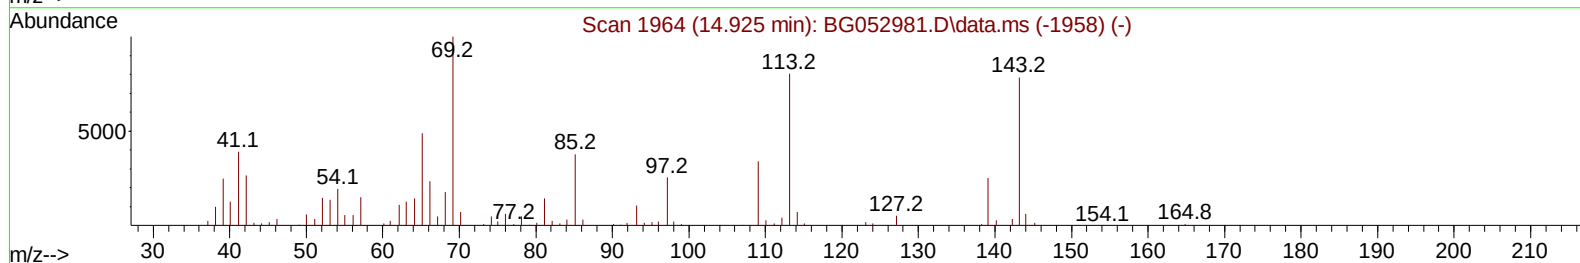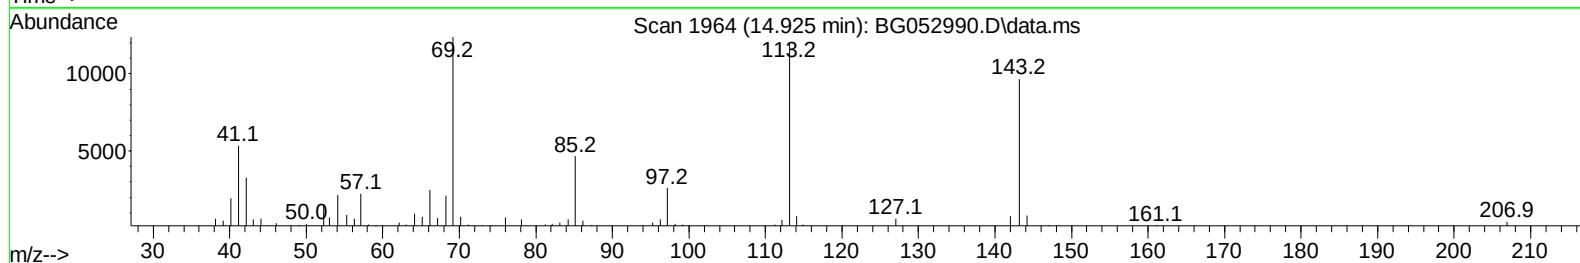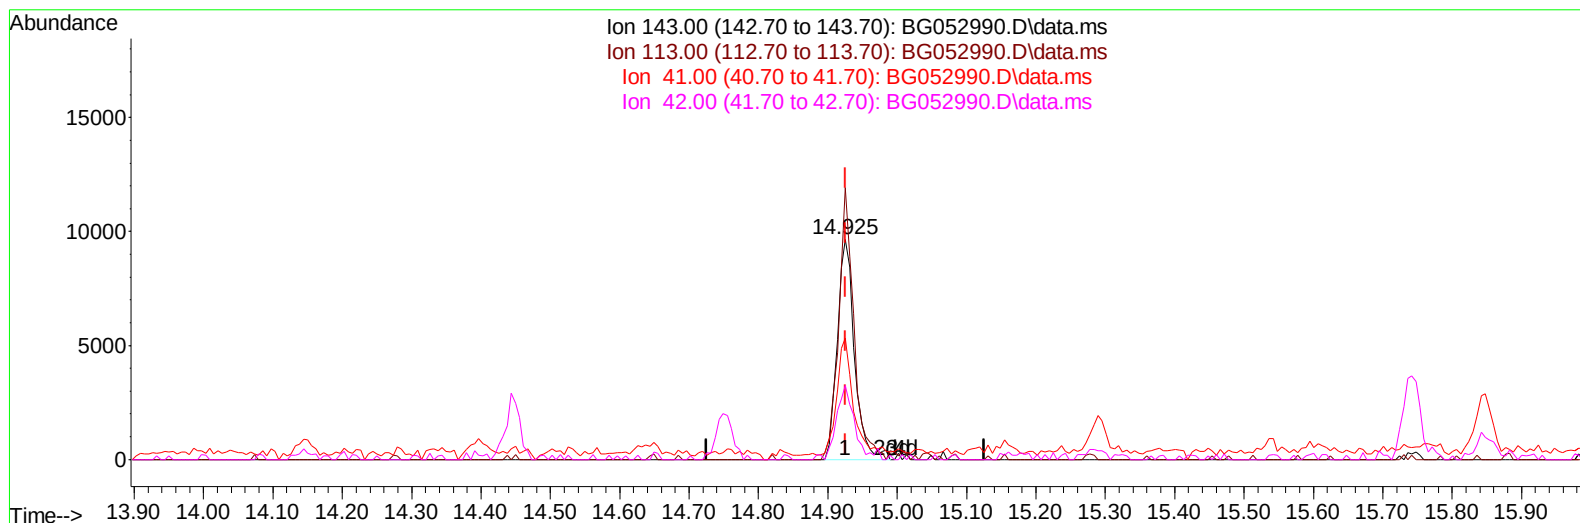

TIC: BG052990.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.000) 14.60 ng/ul m

response 16558

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	123.30
41.00	47.20	55.17
42.00	29.40	33.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052990.D
 Acq On : 31 Mar 2022 21:53
 Operator : CG/JU
 Sample : N2160-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ6

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:05:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	26693	20.000	ng/ul	0.00
20) Naphthalene-d8	10.948	136	115577	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.755	164	87815	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.492	188	204456	20.000	ng/ul	0.00
79) Chrysene-d12	21.781	240	221156	20.000	ng/ul	# 0.00
88) Perylene-d12	25.082	264	231640	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.553	96	3296	4.362	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.283	99	30350	12.695	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.453	67	52274	35.800	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	52661	32.440	ng/ul	0.00
15) 4-Methylphenol-d8	8.822	113	46742	26.990	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	30399	36.539	ng/ul	0.00
24) 2-Nitrophenol-d4	10.014	143	35836	40.838	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	66879	35.033	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	25460	10.091	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	254220	37.683	ng/ul	0.00
49) Acenaphthylene-d8	14.450	160	268557	32.760	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	16558m	14.598	ng/ul	0.00
60) Fluorene-d10	15.742	176	212854	35.933	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	47988	46.121	ng/ul	0.00
73) Anthracene-d10	17.592	188	362344	38.059	ng/ul	0.00
81) Pyrene-d10	19.877	212	452023	36.536	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.859	264	465665	38.906	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052990.D
Acq On : 31 Mar 2022 21:53
Operator : CG/JU
Sample : N2160-13
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYZ6

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:05:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

