




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052991.D
 Acq On : 31 Mar 2022 22:32
 Operator : CG/JU
 Sample : N2160-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ36

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

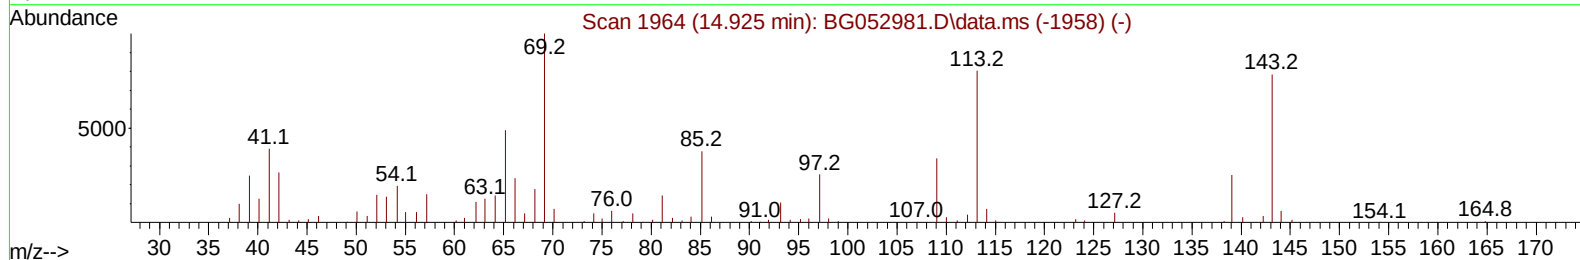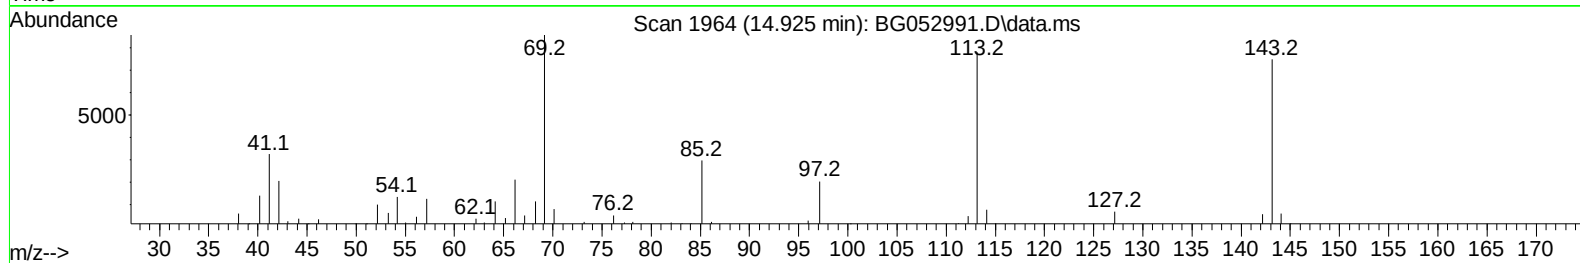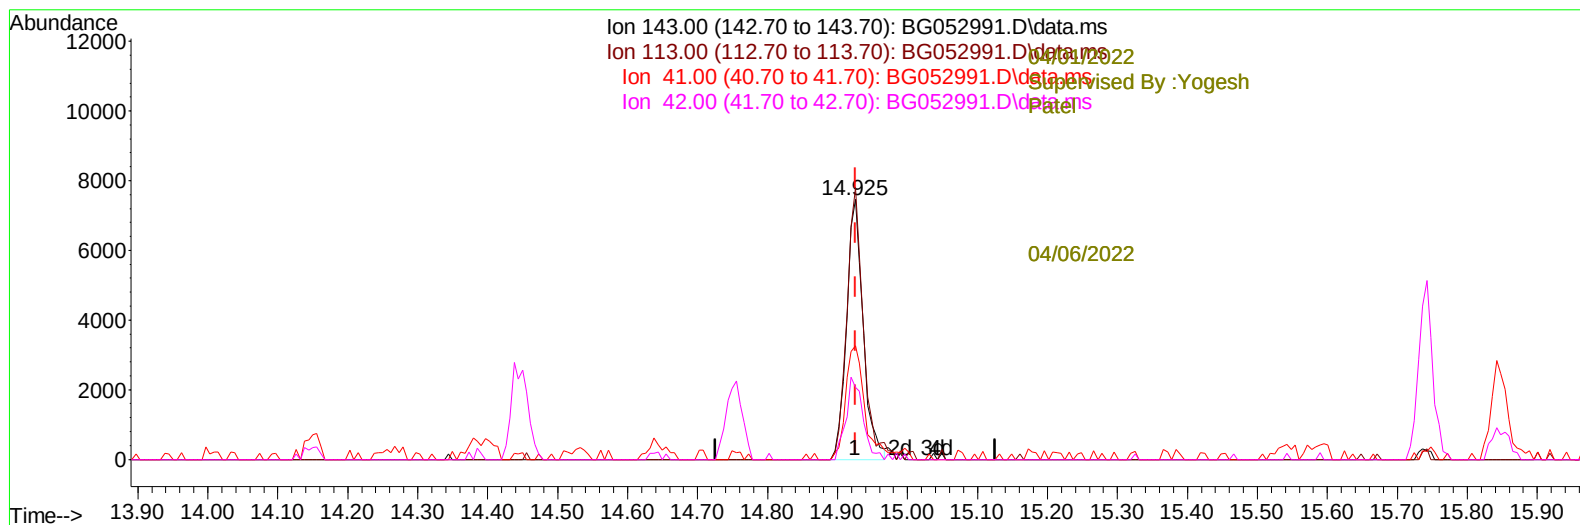

TIC: BG052991.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.000) 9.43 ng/u1

response 12285

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	104.35
41.00	47.20	43.66
42.00	29.40	27.78




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052991.D
 Acq On : 31 Mar 2022 22:32
 Operator : CG/JU
 Sample : N2160-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ36

Manual IntegrationsAPPROVED

Quant Time: Apr 01 01:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

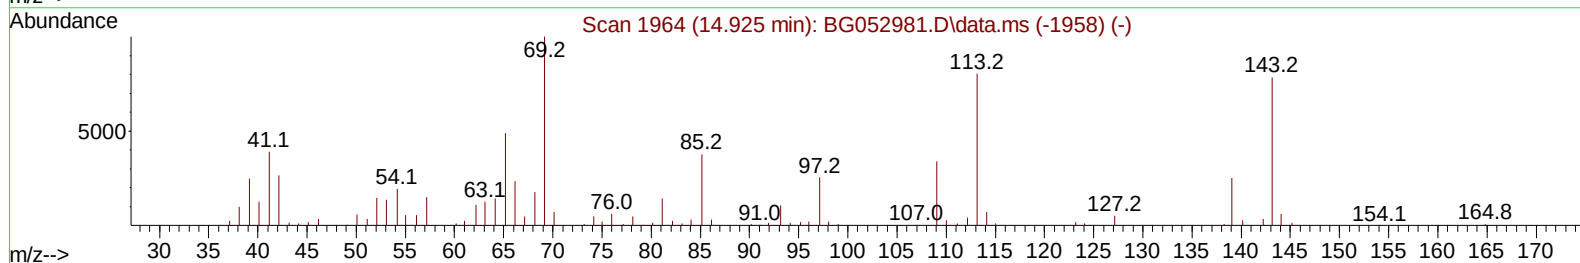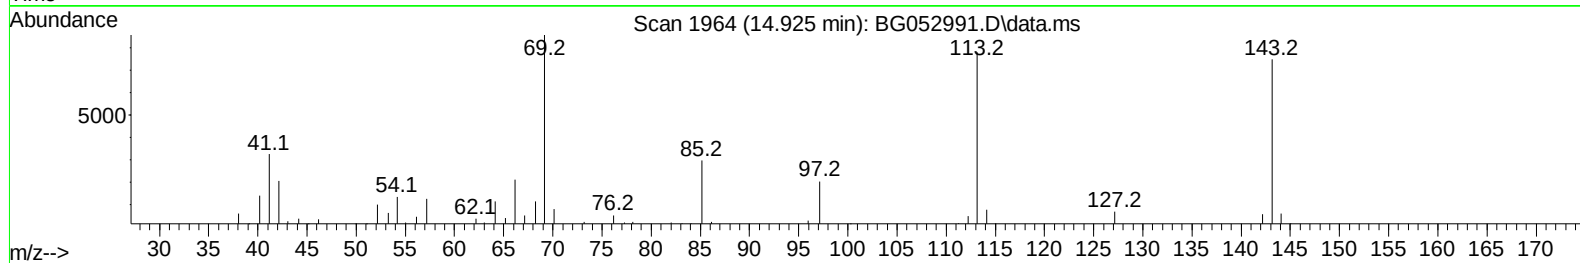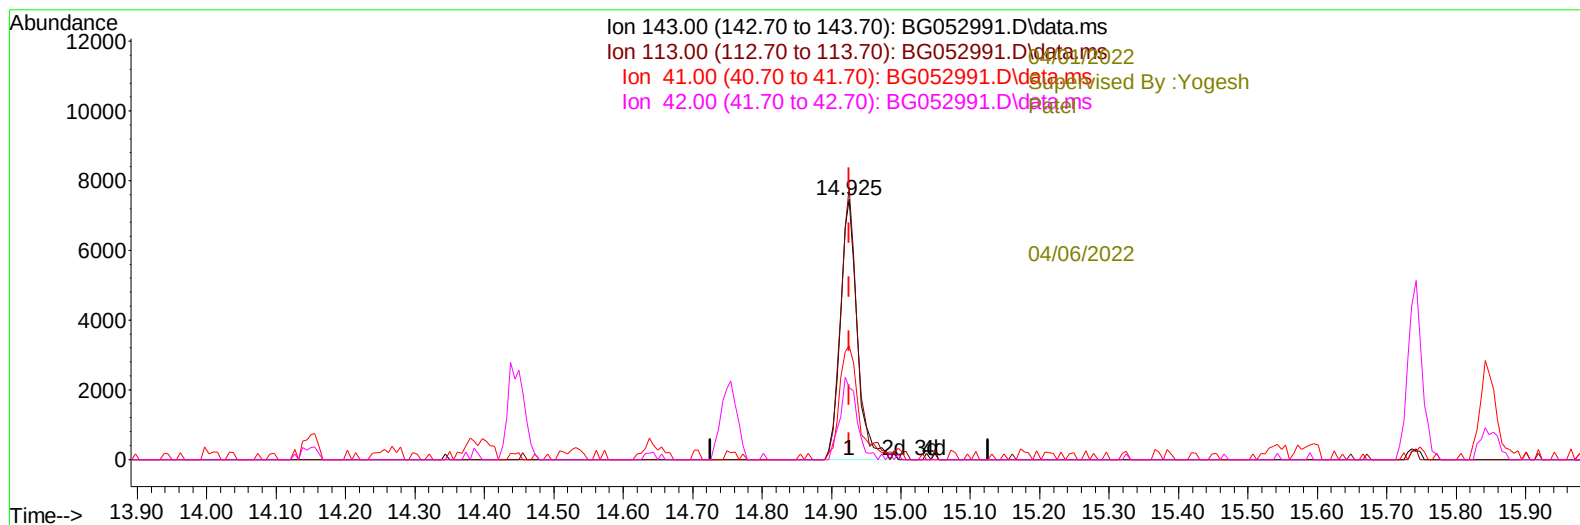

TIC: BG052991.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.925min (-0.000) 9.58 ng/ul m

response 12478

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	104.35
41.00	47.20	43.66
42.00	29.40	27.78

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052991.D
 Acq On : 31 Mar 2022 22:32
 Operator : CG/JU
 Sample : N2160-14
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ36

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:10:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----04/01/2022						
Supervised By :Yogesh Patel						
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	30098	20.000	ng/ul	0.00
20) Naphthalene-d8	10.943	136	130139	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.755	164	100846	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.493	188	234962	20.000	ng/ul	0.00
79) Chrysene-d12	21.775	240	253294	20.000	ng/ul	0.00
88) Perylene-d12	25.082	264	254219	20.000	ng/ul	0.00
-----04/06/2022						
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	3353	3.935	ng/uL	0.00
4) Pyridine-d5	3.976	84	14162	6.657	ng/ul	0.01
7) Phenol-d5	7.283	99	27076	10.044	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.453	67	62476	37.946	ng/ul	0.00
11) 2-Chlorophenol-d4	7.665	132	53890	29.441	ng/ul	0.00
15) 4-Methylphenol-d8	8.828	113	46022	23.568	ng/ul	0.00
21) Nitrobenzene-d5	9.292	128	36375	38.829	ng/ul	0.00
24) 2-Nitrophenol-d4	10.020	143	40425	40.913	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.561	165	69170	32.179	ng/ul	0.00
31) 4-Chloroaniline-d4	11.072	131	73357	25.821	ng/ul	0.00
46) Dimethylphthalate-d6	14.150	166	289658	37.388	ng/ul	0.00
49) Acenaphthylene-d8	14.450	160	317351	33.710	ng/ul	0.00
54) 4-Nitrophenol-d4	14.925	143	12478m	9.579	ng/ul	0.00
60) Fluorene-d10	15.742	176	249236	36.638	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	50056	41.863	ng/ul	0.00
73) Anthracene-d10	17.592	188	415342	37.961	ng/ul	0.00
81) Pyrene-d10	19.878	212	510068	35.997	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.859	264	507207	38.613	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

