




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052996.D
 Acq On : 1 Apr 2022 10:20
 Operator : CG/JU
 Sample : PB143768BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK768

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 04/04/2022
 Supervised By : Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:36:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

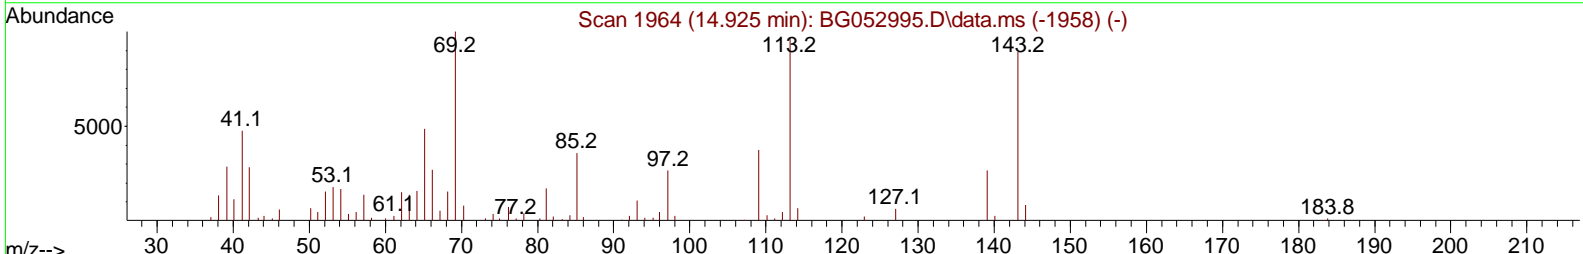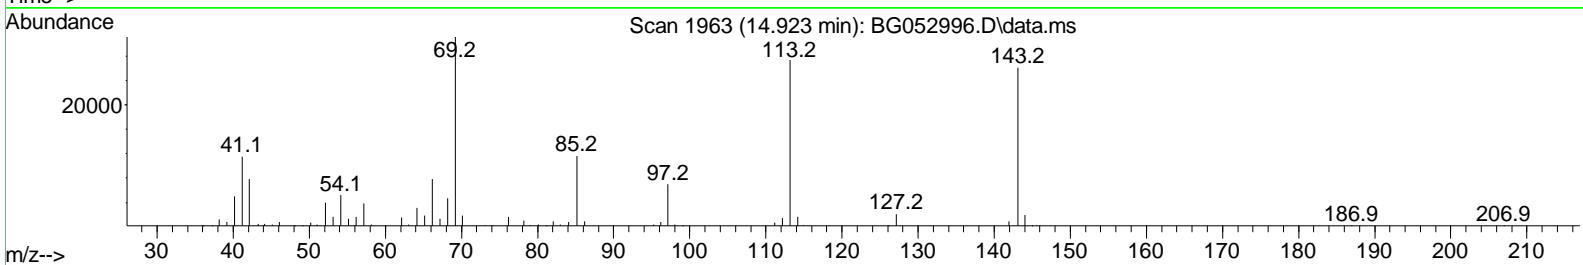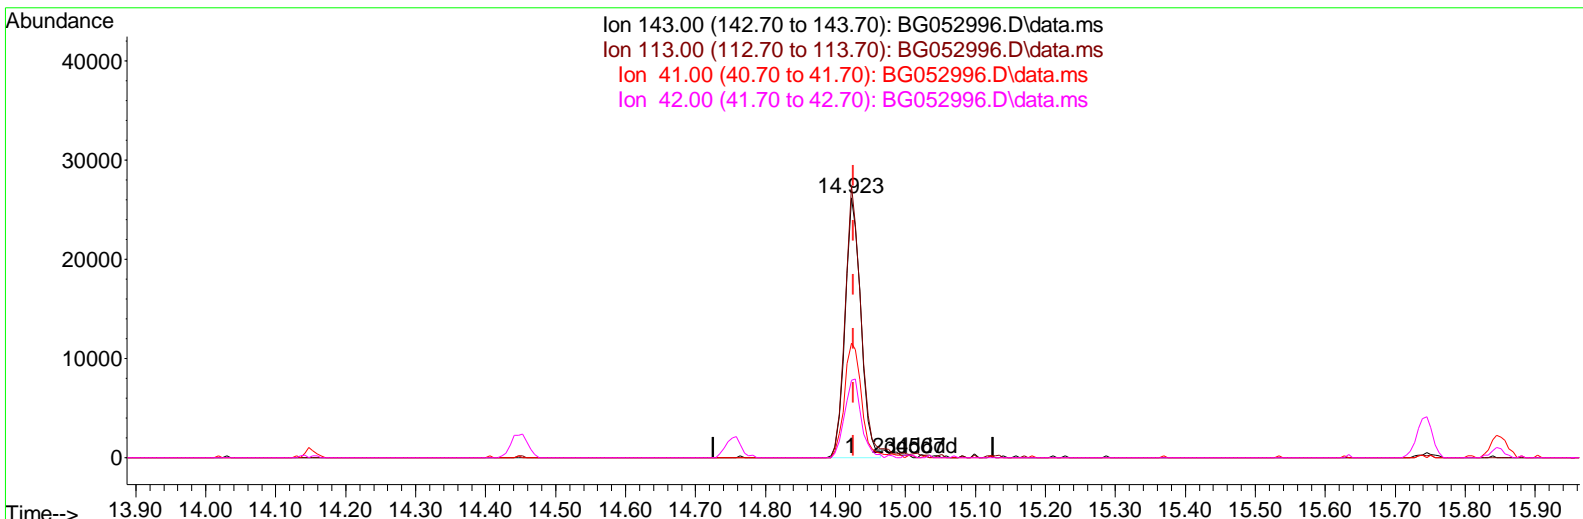

TIC: BG052996.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.923min (-0.003) 35.65 ng/ul

response	40816	
Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	104.71
41.00	47.20	44.02
42.00	29.40	29.87




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052996.D
 Acq On : 1 Apr 2022 10:20
 Operator : CG/JU
 Sample : PB143768BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 SBLK768

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 04/04/2022
 Supervised By : Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:36:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

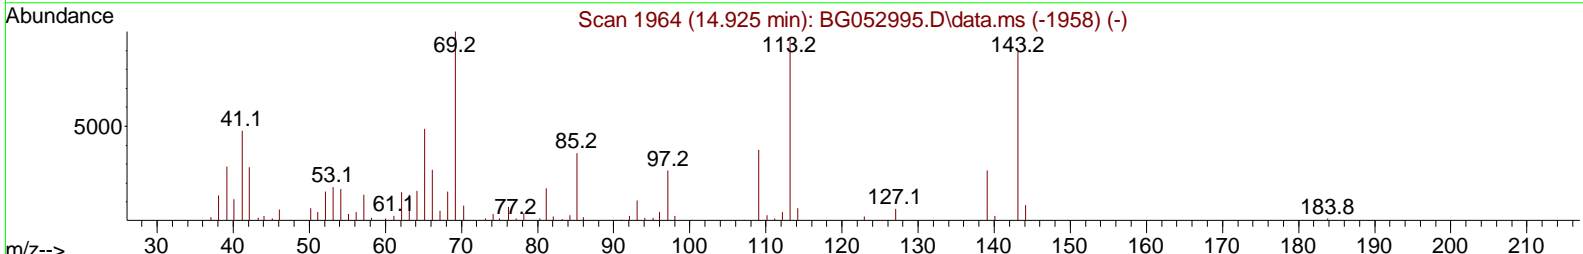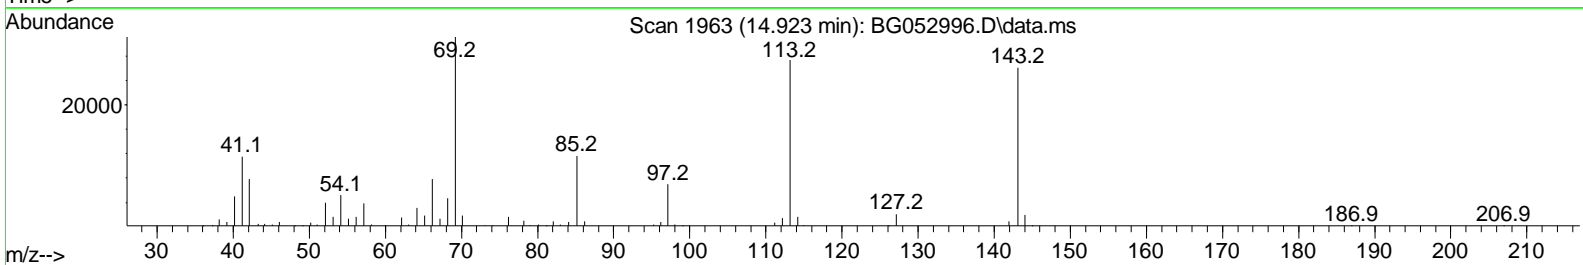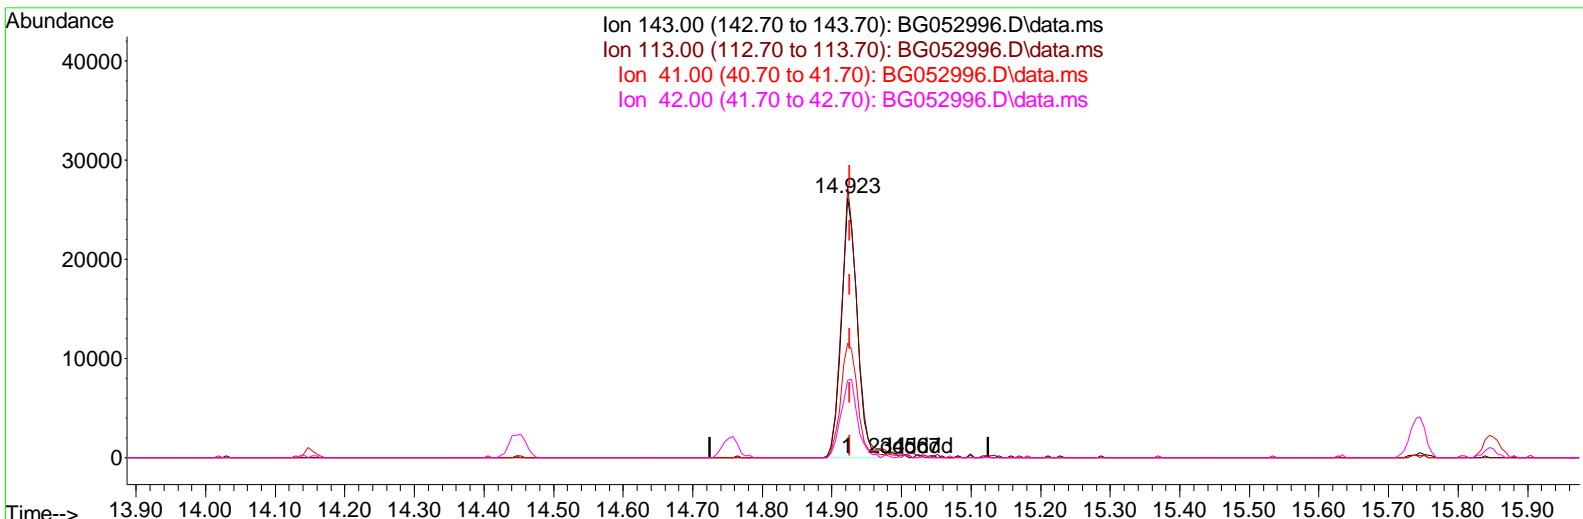

TIC: BG052996.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.923min (-0.003) 36.02 ng/ul m

response	41245	
Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	104.71
41.00	47.20	44.02
42.00	29.40	29.87

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052996.D
 Acq On : 1 Apr 2022 10:20
 Operator : CG/JU
 Sample : PB143768BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 SBLK768

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 04/04/2022
 Supervised By : Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:36:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.132	152	28203	20.000	ng/ul	0.00
20) Naphthalene-d8	10.946	136	111644	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.752	164	88650	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.496	188	212246	20.000	ng/ul	0.00
79) Chrysene-d12	21.778	240	224568	20.000	ng/ul	0.00
88) Perylene-d12	25.085	264	214772	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.550	96	5351	6.702	ng/uL	0.00
4) Pyridine-d5	3.967	84	71771	36.006	ng/ul	0.00
7) Phenol-d5	7.274	99	91814	36.347	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.450	67	61853	40.092	ng/ul	0.00
11) 2-Chlorophenol-d4	7.662	132	63337	36.927	ng/ul	0.00
15) 4-Methylphenol-d8	8.825	113	68981	37.698	ng/ul	0.00
21) Nitrobenzene-d5	9.295	128	35161	43.751	ng/ul	0.00
24) 2-Nitrophenol-d4	10.017	143	37837	44.637	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.558	165	68402	37.093	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131	94960	38.962	ng/ul	0.00
46) Dimethylphthalate-d6	14.153	166	264515	38.839	ng/ul	0.00
49) Acenaphthylene-d8	14.447	160	287884	34.787	ng/ul	0.00
54) 4-Nitrophenol-d4	14.923	143	41245m	36.020	ng/ul	0.00
60) Fluorene-d10	15.745	176	224197	37.492	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.851	200	41790	38.690	ng/ul	0.00
73) Anthracene-d10	17.595	188	379696	38.417	ng/ul	0.00
81) Pyrene-d10	19.875	212	461763	36.756	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.862	264	437904	39.460	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052996.D
 Acq On : 1 Apr 2022 10:20
 Operator : CG/JU
 Sample : PB143768BL
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :

BNA_G

Client Sample Id :

SBLK768

Manual Integrations APPROVED

Reviewed By : Jagrut Upadhyay 04/04/2022
 Supervised By : Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:36:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

