




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052997.D
Acq On : 1 Apr 2022 10:59
Operator : CG/JU
Sample : N2160-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 02 00:37:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/04/2022
Supervised By :Yogesh Patel 04/06/2022

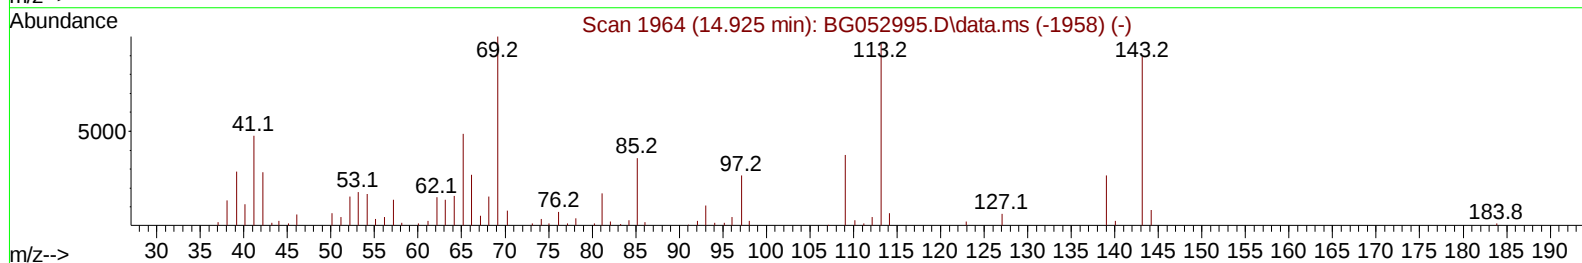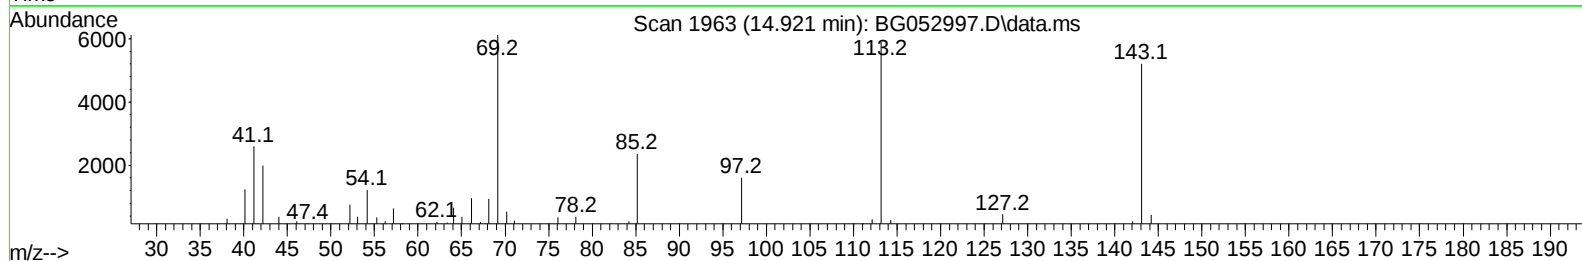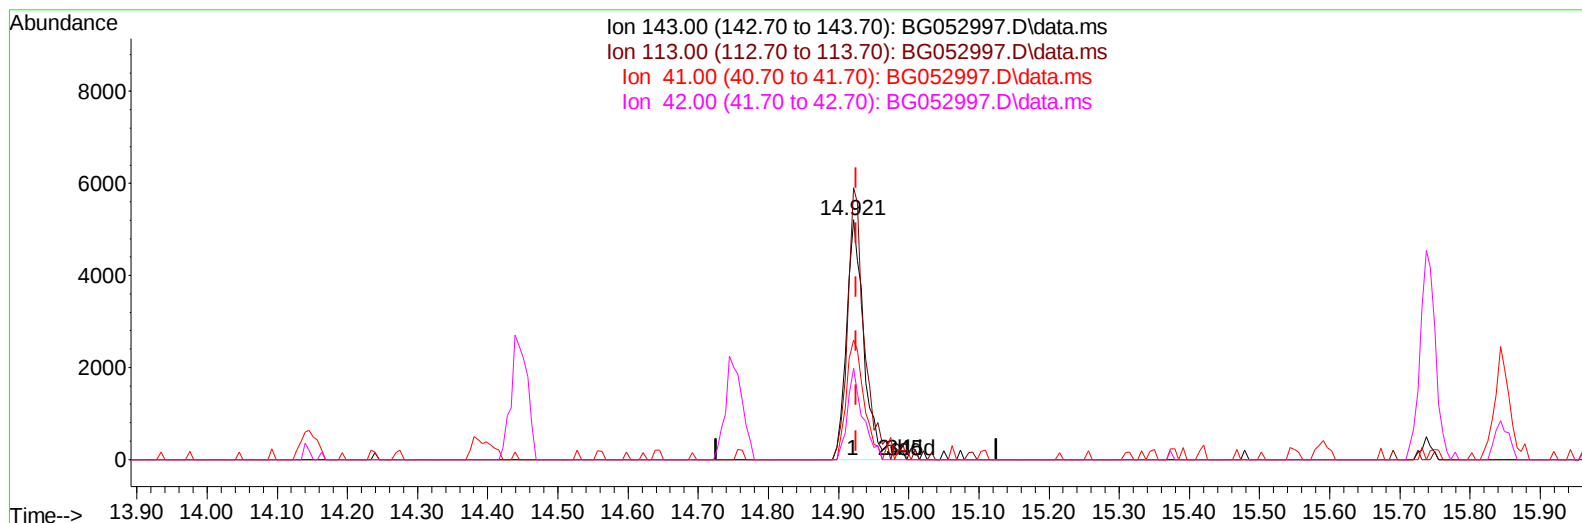

TIC: BG052997.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.921min (-0.005) 7.19 ng/u1

response 8778

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	113.26
41.00	47.20	49.79
42.00	29.40	38.16#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052997.D
 Acq On : 1 Apr 2022 10:59
 Operator : CG/JU
 Sample : N2160-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ2

Manual IntegrationsAPPROVED

Quant Time: Apr 02 00:37:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/04/2022
 Supervised By :Yogesh Patel 04/06/2022

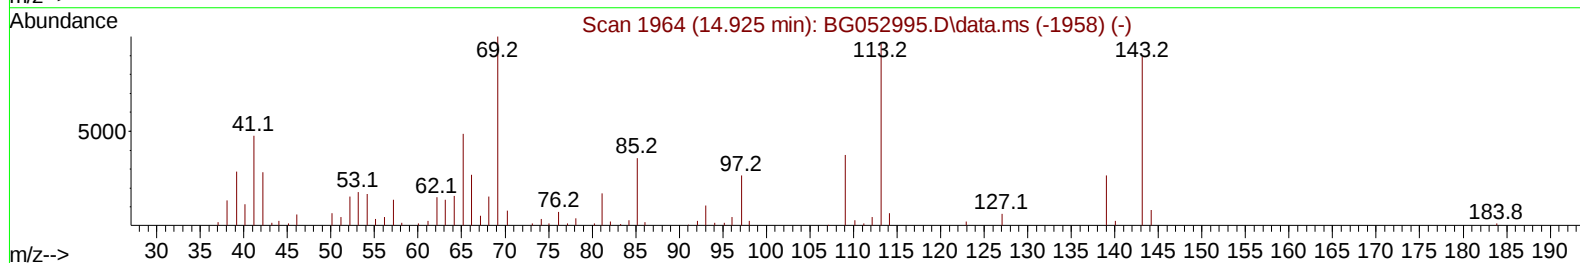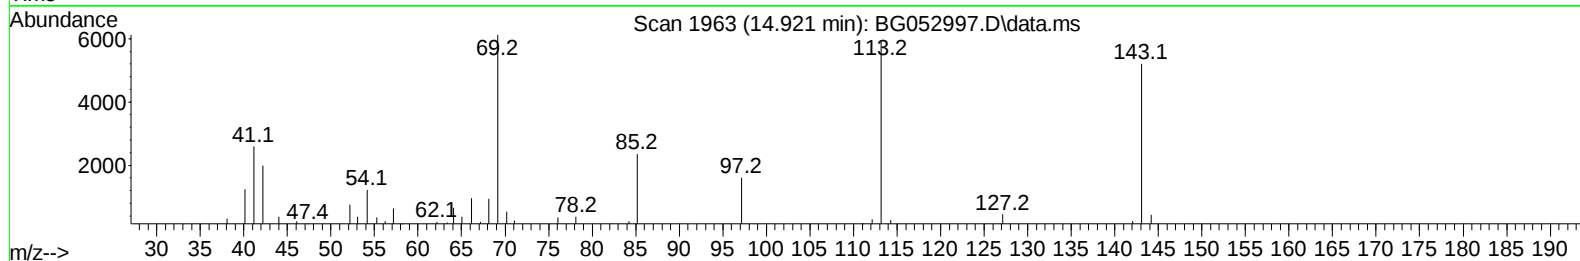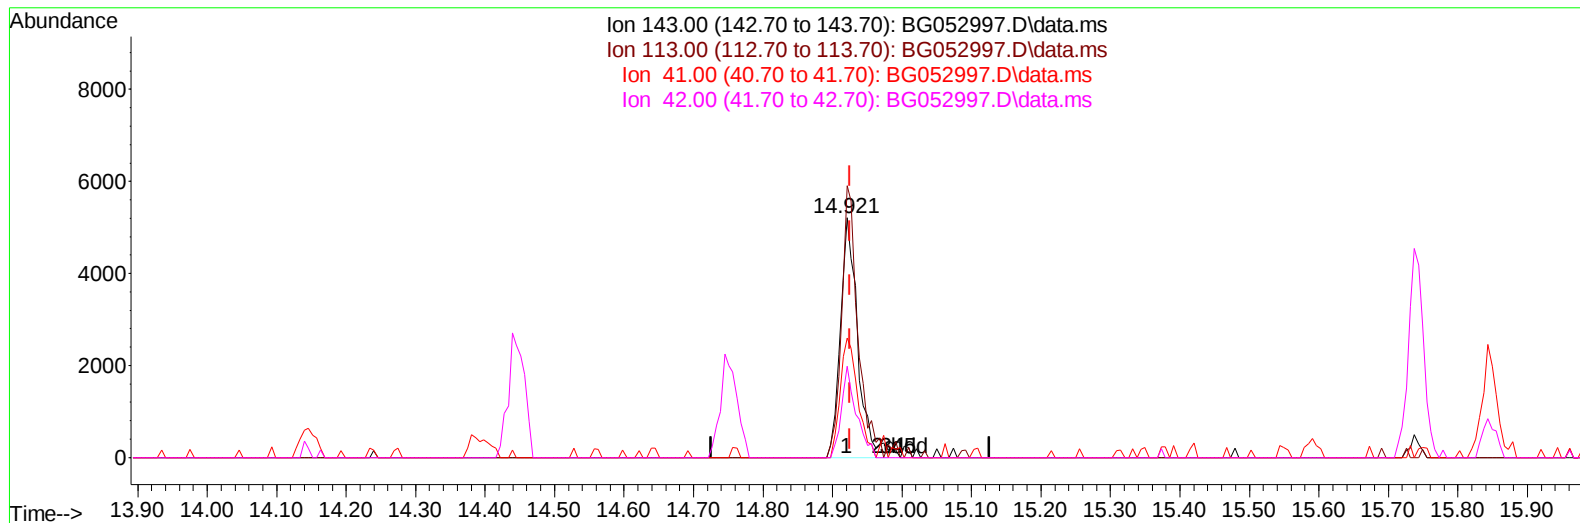

TIC: BG052997.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.921min (-0.005) 7.41 ng/ul m

response 9045

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.70	113.26
41.00	47.20	49.79
42.00	29.40	38.16#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052997.D
 Acq On : 1 Apr 2022 10:59
 Operator : CG/JU
 Sample : N2160-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAYZ2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/04/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:37:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.136	152	31579	20.000	ng/ul	0.00
20) Naphthalene-d8	10.944	136	127711	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.751	164	94557	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.494	188	226564	20.000	ng/ul	0.00
79) Chrysene-d12	21.776	240	244126	20.000	ng/ul	0.00
88) Perylene-d12	25.084	264	244250	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.554	96	4034	4.512	ng/uL	0.00
4) Pyridine-d5	3.971	84	18863	8.452	ng/ul	0.00
7) Phenol-d5	7.278	99	23263	8.225	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.449	67	63437	36.723	ng/ul	0.00
11) 2-Chlorophenol-d4	7.660	132	52708	27.445	ng/ul	0.00
15) 4-Methylphenol-d8	8.829	113	43611	21.286	ng/ul	0.00
21) Nitrobenzene-d5	9.293	128	36492	39.695	ng/ul	0.00
24) 2-Nitrophenol-d4	10.016	143	39805	41.051	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.556	165	65834	31.209	ng/ul	0.00
31) 4-Chloroaniline-d4	11.067	131	80250	28.784	ng/ul	0.00
46) Dimethylphthalate-d6	14.146	166	272809	37.555	ng/ul	0.00
49) Acenaphthylene-d8	14.445	160	304440	34.489	ng/ul	0.00
54) 4-Nitrophenol-d4	14.921	143	9045m	7.406	ng/ul	0.00
60) Fluorene-d10	15.743	176	239994	37.626	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.843	200	44239	38.369	ng/ul	0.00
73) Anthracene-d10	17.594	188	385646	36.553	ng/ul	0.00
81) Pyrene-d10	19.873	212	475977	34.852	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.860	264	478839	37.941	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052997.D
Acq On : 1 Apr 2022 10:59
Operator : CG/JU
Sample : N2160-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAYZ2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/04/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 02 00:37:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

