

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052985.D
 Acq On : 31 Mar 2022 18:38
 Operator : CG/JU
 Sample : N2160-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAZ28

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
 Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:04:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 31 00:50:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.135	152	23855	20.000	ng/u1	0.00
20) Naphthalene-d8	10.949	136	105503	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.755	164	83382	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.493	188	202140	20.000	ng/u1	0.00
79) Chrysene-d12	21.775	240	219074	20.000	ng/u1	0.00
88) Perylene-d12	25.083	264	218232	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.547	96	2619	3.878	ng/uL	0.00
4) Pyridine-d5	3.976	84	8646m	5.128	ng/u1	0.01
7) Phenol-d5	7.277	99	15324	7.172	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.448	67	50164	38.442	ng/u1	0.00
11) 2-Chlorophenol-d4	7.665	132	39918	27.515	ng/u1	0.00
15) 4-Methylphenol-d8	8.828	113	27744	17.926	ng/u1	0.00
21) Nitrobenzene-d5	9.292	128	28944	38.112	ng/u1	0.00
24) 2-Nitrophenol-d4	10.015	143	29678	37.050	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.555	165	53449	30.671	ng/u1	0.00
31) 4-Chloroaniline-d4	11.066	131	57911	25.144	ng/u1	0.00
46) Dimethylphthalate-d6	14.150	166	242590	37.871	ng/u1	0.00
49) Acenaphthylene-d8	14.444	160	261843	33.639	ng/u1	0.00
54) 4-Nitrophenol-d4	14.920	143	7958m	7.389	ng/u1	0.00
60) Fluorene-d10	15.742	176	207118	36.824	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	39485	38.384	ng/u1	0.00
73) Anthracene-d10	17.593	188	356666	37.891	ng/u1	0.00
81) Pyrene-d10	19.878	212	439398	35.853	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.859	264	437519	38.801	ng/u1	0.00
Target Compounds						
8) Phenol	7.307	94	2547	1.237	ng/u1#	58

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052985.D
Acq On : 31 Mar 2022 18:38
Operator : CG/JU
Sample : N2160-03
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
YAZ28

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

Quant Time: Apr 01 01:04:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 31 00:50:49 2022
Response via : Initial Calibration

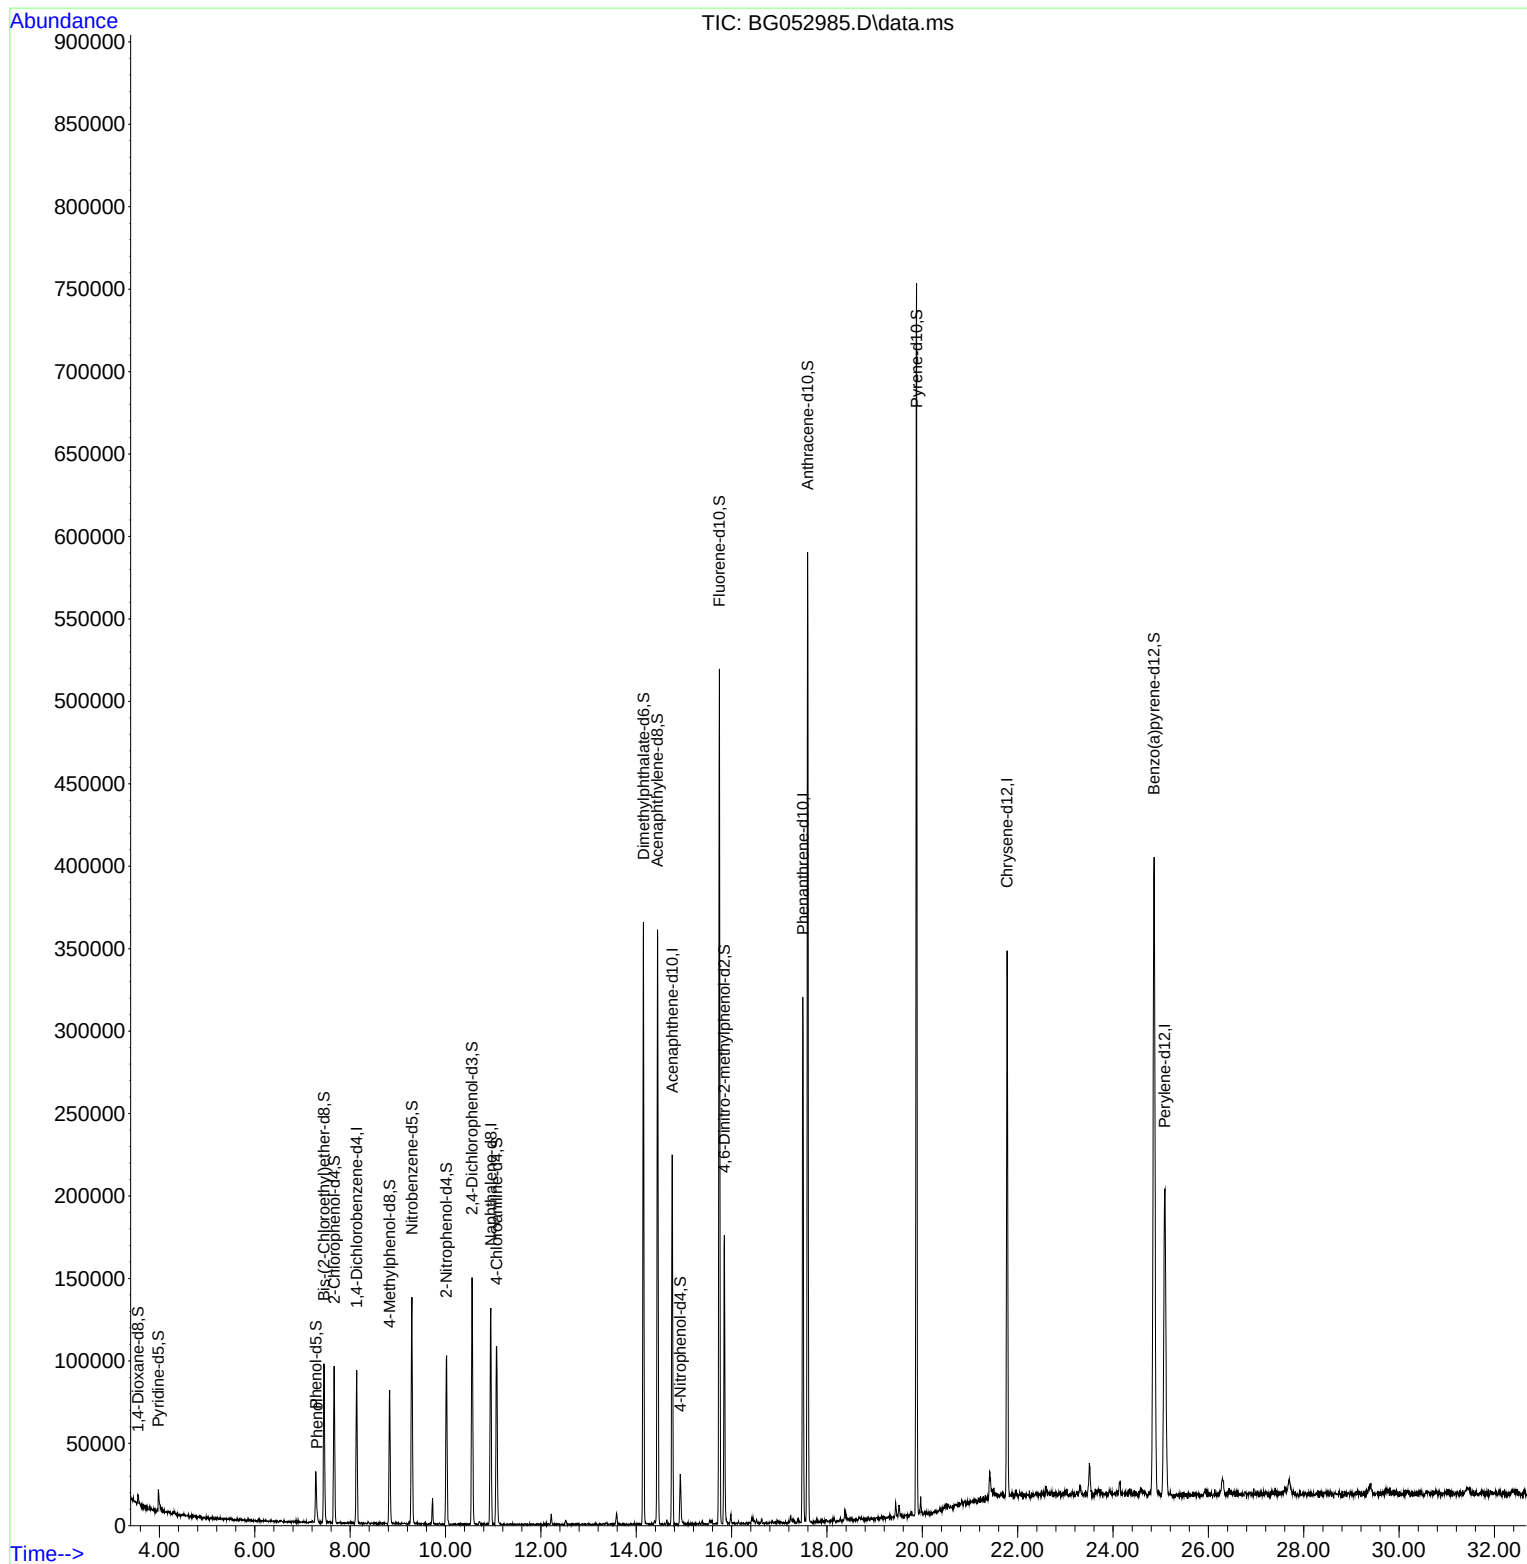

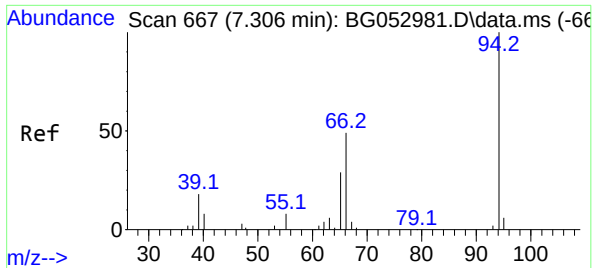

#8
Phenol
Concen: 1.237 ng/ul
RT: 7.307 min Scan# 667
Delta R.T. 0.000 min
Lab File: BG052985.D
Acq: 31 Mar 2022 18:38

Instrument :
BNA_G
ClientSampleId :
YAZ28

Tgt Ion: 94 Resp: 254
Ion Ratio Lower Upper
94 100
65 49.5 25.9 38.9
66 77.6 35.4 53.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/01/2022
Supervised By :Yogesh Patel 04/06/2022

