

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052946.D
 Acq On : 30 Mar 2022 12:39
 Operator : CG/JU
 Sample : PB143704BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.553	24	28	32	rVB5	8912	13676	1.33%	0.150%
2	3.658	42	46	47	rBV3	2645	3030	0.29%	0.033%
3	3.688	49	51	52	rVB	3352	1747	0.17%	0.019%
4	3.964	94	98	113	rBV	79065	145371	14.11%	1.593%
5	4.216	139	141	142	rBV3	1780	1587	0.15%	0.017%
6	4.305	154	156	162	rVB4	3762	5759	0.56%	0.063%
7	4.581	201	203	208	rVB5	1358	1851	0.18%	0.020%
8	4.622	208	210	212	rVV	1538	1485	0.14%	0.016%
9	4.657	215	216	219	rVB3	1793	1434	0.14%	0.016%
10	5.309	325	327	331	rVB4	2374	2916	0.28%	0.032%
11	5.738	398	400	402	rBV3	1618	1435	0.14%	0.016%
12	6.284	490	493	495	rVB3	1827	1824	0.18%	0.020%
13	6.319	495	499	501	rBV4	1645	2458	0.24%	0.027%
14	6.543	535	537	542	rVB4	1149	1549	0.15%	0.017%
15	7.277	655	662	673	rVB	115641	195241	18.95%	2.139%
16	7.447	683	691	699	rVV	82906	144274	14.00%	1.581%
17	7.659	721	727	736	rBV	104259	184208	17.88%	2.018%
18	8.135	800	808	817	rVB2	82473	147194	14.29%	1.613%
19	8.828	919	926	933	rBV2	135190	237483	23.05%	2.602%
20	9.292	996	1005	1015	rBV	111060	199351	19.35%	2.184%
21	9.357	1015	1016	1021	rVV	982	1440	0.14%	0.016%
22	9.439	1024	1030	1032	rVB2	822	1439	0.14%	0.016%
23	9.562	1050	1051	1056	rBV3	897	1486	0.14%	0.016%
24	9.791	1084	1090	1093	rBV3	692	1415	0.14%	0.016%
25	10.014	1121	1128	1137	rVB	88656	161865	15.71%	1.773%
26	10.343	1180	1184	1186	rBV2	856	1451	0.14%	0.016%
27	10.555	1213	1220	1229	rBV2	132994	239410	23.23%	2.623%
28	10.943	1277	1286	1293	rBV	109968	210301	20.41%	2.304%
29	11.066	1301	1307	1316	rBV	138617	253219	24.57%	2.774%
30	12.523	1550	1555	1560	rBV2	2537	4011	0.39%	0.044%
31	14.150	1825	1832	1839	rVB	301379	448579	43.53%	4.915%
32	14.444	1875	1882	1891	rBV	292092	478012	46.39%	5.237%
33	14.749	1928	1934	1942	rVB2	198421	326405	31.68%	3.576%
34	14.920	1956	1963	1974	rVV	146354	242771	23.56%	2.660%
35	15.014	1977	1979	1982	rVV3	1821	2302	0.22%	0.025%
36	15.742	2096	2103	2112	rVB	415985	642539	62.36%	7.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052946.D
 Acq On : 30 Mar 2022 12:39
 Operator : CG/JU
 Sample : PB143704BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.848	2115	2121	2128	rBV	139208	211928	20.57%	2.322%
38	15.977	2140	2143	2148	rVV3	3298	4854	0.47%	0.053%
39	16.529	2233	2237	2239	rVV3	1107	1622	0.16%	0.018%
40	17.281	2362	2365	2369	rVB2	1981	2462	0.24%	0.027%

41	17.493	2395	2401	2409	rVB	295544	462246	44.86%	5.065%
42	17.592	2411	2418	2427	rVB2	524136	794043	77.06%	8.700%
43	17.763	2441	2447	2449	rBV2	1102	1556	0.15%	0.017%
44	17.933	2473	2476	2479	rBV2	1329	1617	0.16%	0.018%
45	18.068	2497	2499	2502	rBV3	1394	1575	0.15%	0.017%

46	18.362	2544	2549	2552	rBV4	1823	3265	0.32%	0.036%
47	18.462	2562	2566	2568	rVB3	2001	2013	0.20%	0.022%
48	18.491	2568	2571	2572	rBV2	1726	1646	0.16%	0.018%
49	18.556	2579	2582	2584	rVB3	1563	2009	0.19%	0.022%
50	18.579	2584	2586	2588	rBV2	1515	1558	0.15%	0.017%

51	18.662	2598	2600	2604	rVV2	1853	1453	0.14%	0.016%
52	19.055	2664	2667	2668	rVV2	1613	1507	0.15%	0.017%
53	19.214	2692	2694	2697	rVB3	1810	2177	0.21%	0.024%
54	19.384	2720	2723	2726	rBV4	1195	1595	0.15%	0.017%
55	19.443	2729	2733	2739	rVB6	8099	12171	1.18%	0.133%

56	19.507	2742	2744	2750	rVB3	8167	11154	1.08%	0.122%
57	19.596	2757	2759	2761	rBV	3584	3407	0.33%	0.037%
58	19.684	2772	2774	2775	rBV	2061	1405	0.14%	0.015%
59	19.831	2798	2799	2800	rBV	2602	1447	0.14%	0.016%
60	19.878	2800	2807	2815	rVV	699799	1030396	100.00%	11.289%

61	19.977	2821	2824	2826	rBV4	2210	2255	0.22%	0.025%
62	20.101	2841	2845	2848	rVV4	3765	5125	0.50%	0.056%
63	20.136	2850	2851	2853	rBV2	2474	1582	0.15%	0.017%
64	20.224	2864	2866	2868	rVV3	2048	2108	0.20%	0.023%
65	20.265	2871	2873	2874	rVV2	2543	2090	0.20%	0.023%

66	20.295	2877	2878	2881	rVB3	3061	1743	0.17%	0.019%
67	20.400	2893	2896	2898	rBV3	2964	3765	0.37%	0.041%
68	20.518	2912	2916	2917	rBV4	4496	4764	0.46%	0.052%
69	20.535	2917	2919	2920	rBV2	3017	2159	0.21%	0.024%
70	20.776	2958	2960	2963	rBV4	3059	3969	0.39%	0.043%

71	21.123	3017	3019	3021	rVB2	3084	2272	0.22%	0.025%
72	21.775	3124	3130	3138	rVB	337266	578138	56.11%	6.334%
73	21.869	3144	3146	3148	rVB3	3243	2188	0.21%	0.024%
74	22.292	3216	3218	3219	rBV2	3233	1892	0.18%	0.021%
75	23.449	3414	3415	3416	rBV	4427	1985	0.19%	0.022%

76	24.859	3644	3655	3668	rBV2	354318	1010321	98.05%	11.070%
----	--------	------	------	------	------	--------	---------	--------	---------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052946.D
 Acq On : 30 Mar 2022 12:39
 Operator : CG/JU
 Sample : PB143704BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK704

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	25.082	3683	3693	3710	rVB2	188012	572753	55.59%	6.275%
78	25.370	3740	3742	3745	rVB4	3675	2964	0.29%	0.032%
79	25.693	3795	3797	3798	rVB2	3388	1836	0.18%	0.020%
80	25.781	3810	3812	3815	rBV3	2899	3095	0.30%	0.034%
81	26.087	3862	3864	3865	rBV2	3152	1713	0.17%	0.019%
82	26.439	3922	3924	3926	rBV3	4533	2842	0.28%	0.031%
83	26.551	3941	3943	3944	rBV2	5184	2566	0.25%	0.028%
84	28.031	4193	4195	4196	rBV2	4271	1885	0.18%	0.021%
85	28.213	4225	4226	4228	rBV2	3497	2002	0.19%	0.022%
86	28.801	4324	4326	4328	rBV3	3119	2441	0.24%	0.027%
87	28.930	4344	4348	4349	rBV4	4244	4339	0.42%	0.048%
88	29.206	4394	4395	4397	rBV2	4039	2477	0.24%	0.027%
89	29.347	4417	4419	4420	rBV2	3329	2067	0.20%	0.023%
90	29.829	4499	4501	4502	rBV	3305	1495	0.15%	0.016%
91	29.893	4511	4512	4513	rBV	4461	2036	0.20%	0.022%
92	31.092	4715	4716	4720	rBV4	3372	4700	0.46%	0.051%
93	31.368	4761	4763	4764	rBV2	3070	2833	0.27%	0.031%
94	31.720	4821	4823	4825	rBV2	2968	2560	0.25%	0.028%
95	31.996	4868	4870	4871	rVB2	4471	2526	0.25%	0.028%
96	32.014	4871	4873	4875	rBV2	2529	1983	0.19%	0.022%
97	32.226	4907	4909	4911	rBV3	3082	3513	0.34%	0.038%
98	32.284	4917	4919	4921	rBV3	3777	2462	0.24%	0.027%
99	32.384	4934	4936	4937	rBV2	3082	2282	0.22%	0.025%
100	32.443	4944	4946	4948	rBV3	3921	1711	0.17%	0.019%




Sum of corrected areas: 9127061

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052946.D
Acq On : 30 Mar 2022 12:39
Operator : CG/JU
Sample : PB143704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

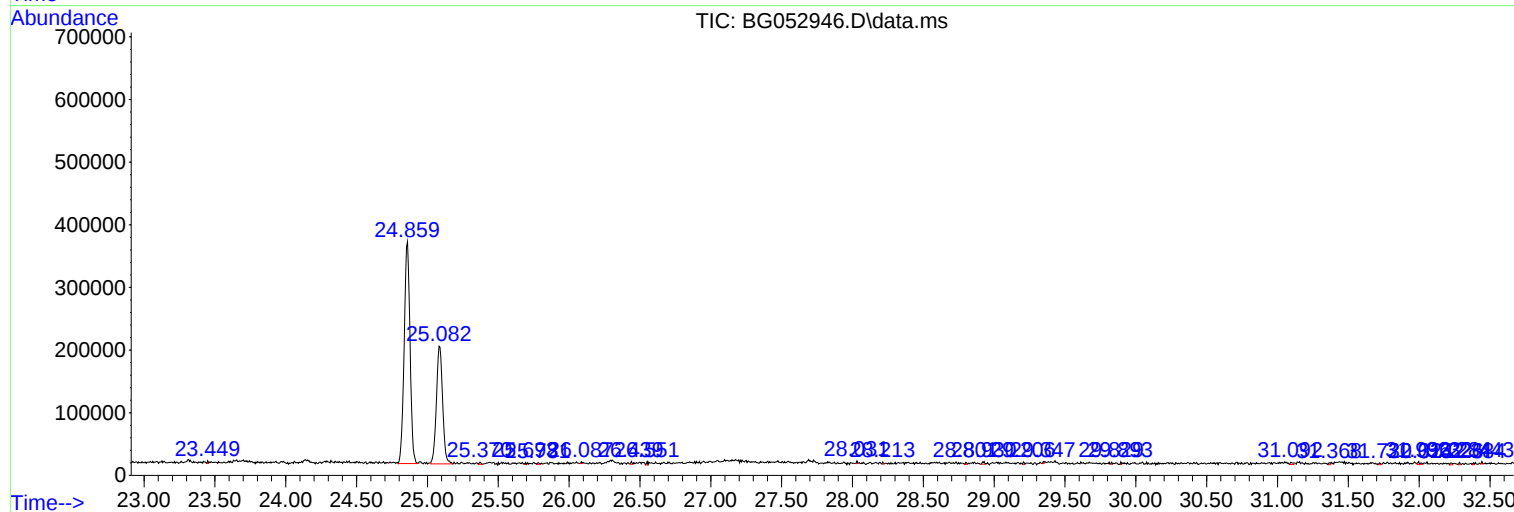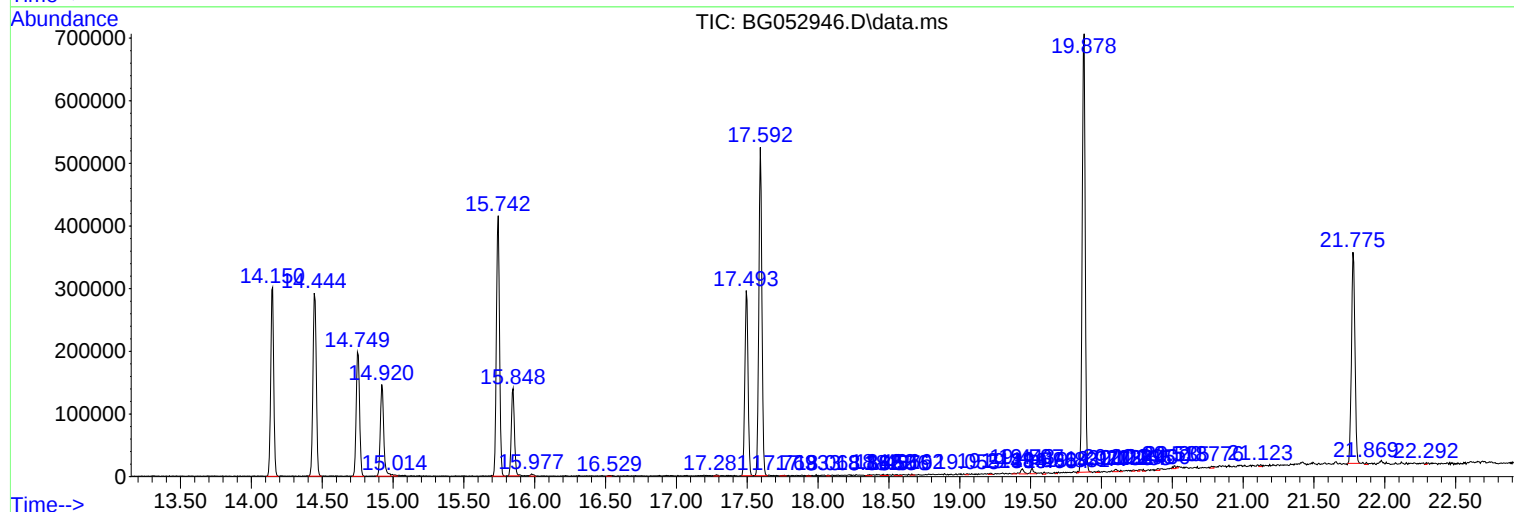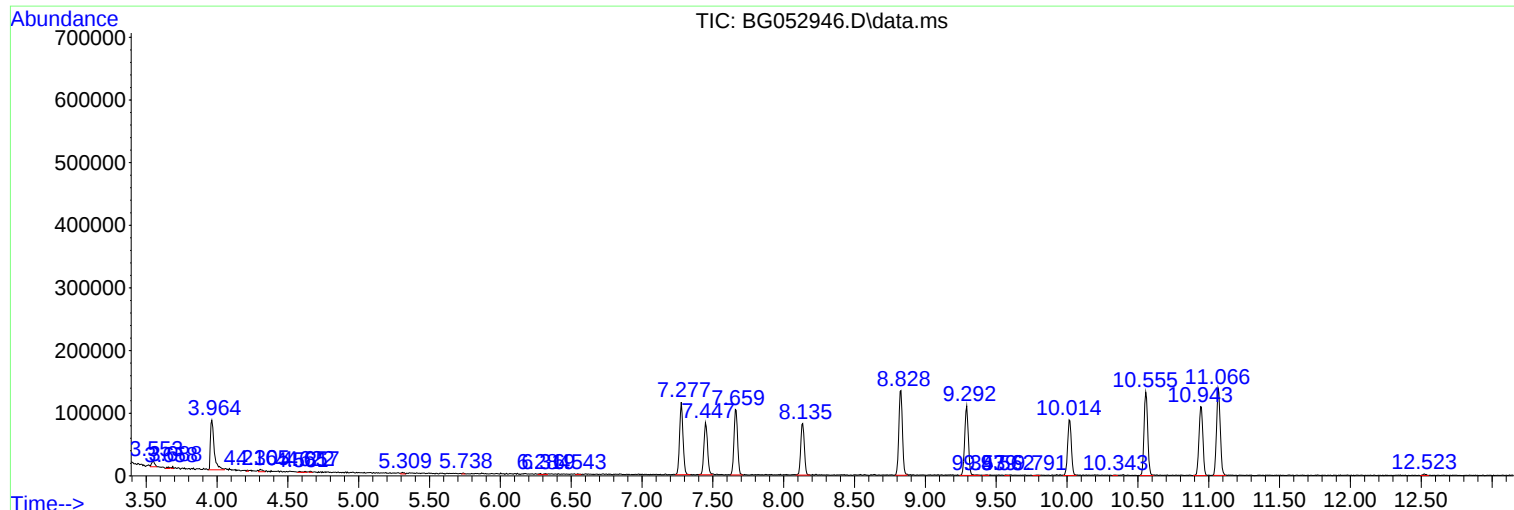

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052946.D
Acq On : 30 Mar 2022 12:39
Operator : CG/JU
Sample : PB143704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052946.D
Acq On : 30 Mar 2022 12:39
Operator : CG/JU
Sample : PB143704BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK704

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc