

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052948.D
 Acq On : 30 Mar 2022 13:56
 Operator : CG/JU
 Sample : N2130-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.876	82	83	84	rBV	3356	1417	0.22%	0.054%
2	4.405	171	173	176	rBV2	1691	2232	0.35%	0.086%
3	5.433	346	348	351	rBV2	1093	1012	0.16%	0.039%
4	5.656	384	386	389	rVB3	1571	1457	0.23%	0.056%
5	5.685	389	391	393	rBV2	1243	1134	0.18%	0.044%
6	5.991	442	443	445	rBV2	1002	833	0.13%	0.032%
7	6.849	585	589	590	rBV2	780	845	0.13%	0.032%
8	7.078	626	628	631	rBV3	666	999	0.16%	0.038%
9	7.448	688	691	694	rBV	1281	1851	0.29%	0.071%
10	7.495	696	699	703	rVB2	1222	1853	0.29%	0.071%
11	7.577	711	713	714	rBV2	1035	802	0.12%	0.031%
12	7.812	750	753	758	rBV3	691	794	0.12%	0.030%
13	7.912	767	770	772	rBV2	795	1021	0.16%	0.039%
14	7.941	773	775	776	rVB	1326	804	0.13%	0.031%
15	7.976	779	781	783	rBV	812	862	0.13%	0.033%
16	8.006	784	786	789	rBV2	1042	1029	0.16%	0.039%
17	8.135	801	808	821	rVB	88784	157524	24.53%	6.045%
18	8.270	829	831	833	rBV	1082	933	0.15%	0.036%
19	8.305	836	837	841	rVB2	1152	1046	0.16%	0.040%
20	8.347	841	844	845	rBV2	1286	1135	0.18%	0.044%
21	8.758	913	914	918	rVB2	870	789	0.12%	0.030%
22	8.858	928	931	932	rBV2	1002	824	0.13%	0.032%
23	8.969	948	950	953	rVB2	857	776	0.12%	0.030%
24	8.993	953	954	958	rBV	986	1102	0.17%	0.042%
25	9.263	997	1000	1002	rVB2	1563	1214	0.19%	0.047%
26	9.281	1002	1003	1006	rBV	1127	1095	0.17%	0.042%
27	9.310	1006	1008	1011	rVV	821	826	0.13%	0.032%
28	9.686	1071	1072	1076	rBV	808	857	0.13%	0.033%
29	9.721	1076	1078	1083	rVB2	677	788	0.12%	0.030%
30	9.903	1106	1109	1110	rBV	837	820	0.13%	0.031%
31	10.156	1148	1152	1153	rBV2	878	864	0.13%	0.033%
32	10.943	1279	1286	1294	rBV	129046	227117	35.36%	8.715%
33	11.207	1327	1331	1332	rBV2	950	966	0.15%	0.037%
34	11.895	1446	1448	1451	rVB	1097	1056	0.16%	0.041%
35	11.995	1464	1465	1467	rBV	1019	933	0.15%	0.036%
36	12.288	1512	1515	1517	rBV	700	839	0.13%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052948.D
 Acq On : 30 Mar 2022 13:56
 Operator : CG/JU
 Sample : N2130-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	12.658	1576	1578	1579	rBV	1088	786	0.12%	0.030%
38	12.764	1592	1596	1599	rBV2	928	1207	0.19%	0.046%
39	12.858	1609	1612	1615	rBV2	1218	889	0.14%	0.034%
40	13.122	1653	1657	1659	rBV2	764	1186	0.18%	0.046%
41	14.127	1826	1828	1831	rVB2	820	833	0.13%	0.032%
42	14.168	1831	1835	1837	rBV2	742	857	0.13%	0.033%
43	14.750	1928	1934	1946	rVB	216022	351877	54.78%	13.502%
44	14.873	1954	1955	1958	rVB	1114	897	0.14%	0.034%
45	15.090	1990	1992	1996	rVB	655	849	0.13%	0.033%
46	15.161	2000	2004	2005	rBV	709	848	0.13%	0.033%
47	15.596	2077	2078	2081	rBV2	874	934	0.15%	0.036%
48	15.854	2119	2122	2126	rBV2	1203	2073	0.32%	0.080%
49	16.054	2154	2156	2159	rVB2	1024	1160	0.18%	0.045%
50	16.083	2159	2161	2164	rBV2	1046	1359	0.21%	0.052%
51	16.465	2224	2226	2231	rVB3	1047	1031	0.16%	0.040%
52	16.571	2241	2244	2247	rVB2	720	848	0.13%	0.033%
53	16.706	2263	2267	2268	rVB2	870	821	0.13%	0.032%
54	17.276	2362	2364	2366	rBV2	839	781	0.12%	0.030%
55	17.381	2380	2382	2387	rVB2	777	941	0.15%	0.036%
56	17.493	2394	2401	2408	rBV	340280	512371	79.77%	19.661%
57	17.693	2433	2435	2439	rBV2	763	777	0.12%	0.030%
58	18.098	2501	2504	2506	rBV2	1050	951	0.15%	0.036%
59	18.180	2515	2518	2521	rBV2	1123	1314	0.20%	0.050%
60	18.257	2528	2531	2534	rBV2	1340	1546	0.24%	0.059%
61	18.462	2563	2566	2572	rVB3	1264	1932	0.30%	0.074%
62	18.509	2572	2574	2576	rBV	785	815	0.13%	0.031%
63	18.556	2581	2582	2587	rBV3	1175	1338	0.21%	0.051%
64	18.797	2622	2623	2624	rBV	1863	812	0.13%	0.031%
65	18.821	2624	2627	2630	rVV2	1248	1648	0.26%	0.063%
66	18.856	2630	2633	2634	rVV2	1259	967	0.15%	0.037%
67	18.891	2637	2639	2640	rVB	1580	1057	0.16%	0.041%
68	18.909	2640	2642	2644	rBV2	1303	1323	0.21%	0.051%
69	19.079	2669	2671	2673	rBV2	1198	1207	0.19%	0.046%
70	19.126	2677	2679	2682	rBV4	1219	970	0.15%	0.037%
71	19.320	2710	2712	2714	rVB2	1431	820	0.13%	0.031%
72	19.843	2799	2801	2803	rBV2	1763	1347	0.21%	0.052%
73	19.907	2810	2812	2815	rVB3	2594	2015	0.31%	0.077%
74	19.990	2824	2826	2829	rBV2	2431	1578	0.25%	0.061%
75	20.072	2838	2840	2841	rBV2	2009	1195	0.19%	0.046%
76	20.131	2848	2850	2851	rVB2	2430	1196	0.19%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052948.D
Acq On : 30 Mar 2022 13:56
Operator : CG/JU
Sample : N2130-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Title : SVOA CALIBRATION

77	20.407	2896	2897	2898	rBV	3075	1500	0.23%	0.058%
78	21.775	3124	3130	3137	rVB	387057	642298	100.00%	24.647%
79	25.083	3683	3693	3704	rVB3	211390	634429	98.77%	24.345%




Sum of corrected areas: 2606032

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052948.D
Acq On : 30 Mar 2022 13:56
Operator : CG/JU
Sample : N2130-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

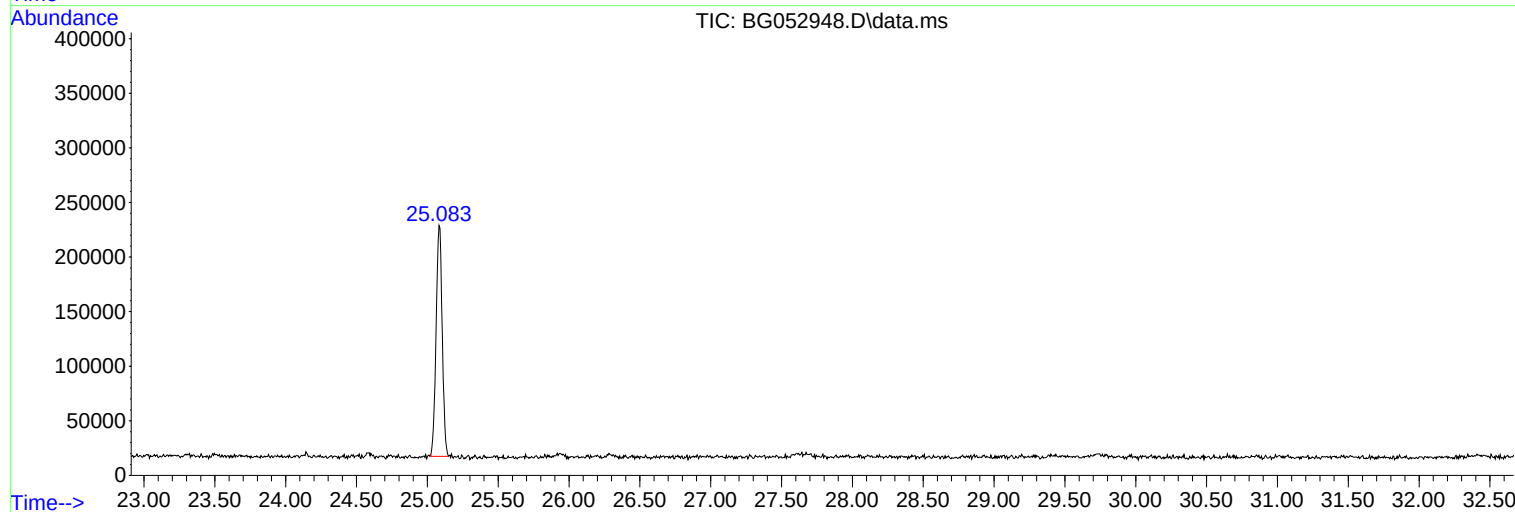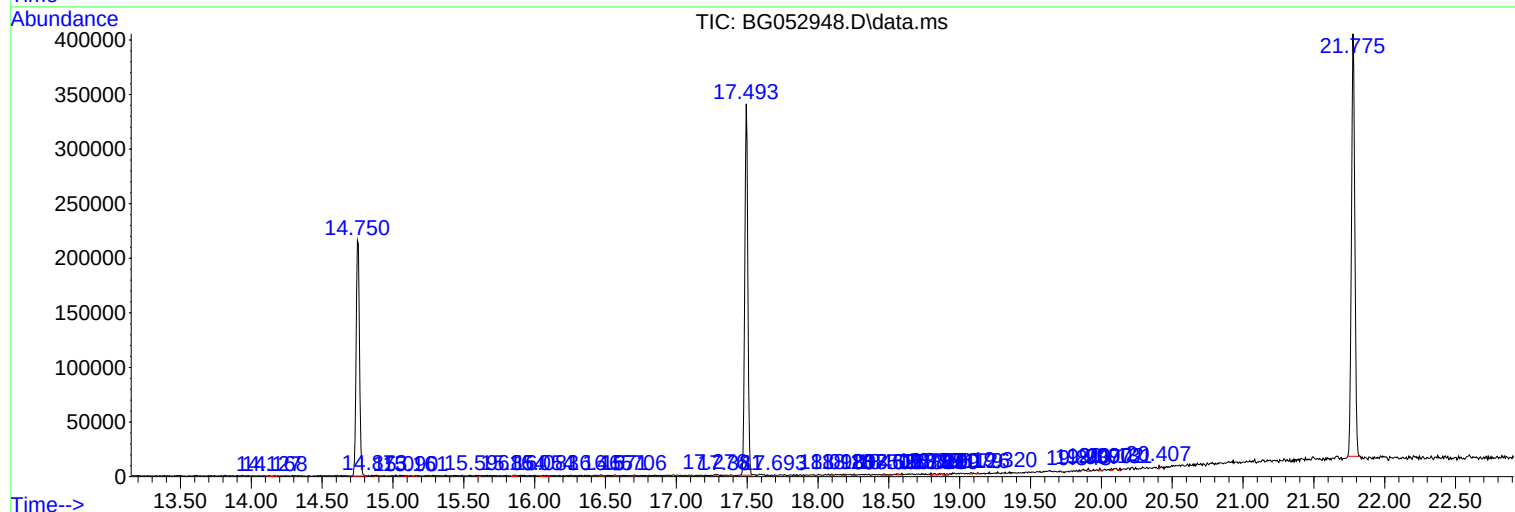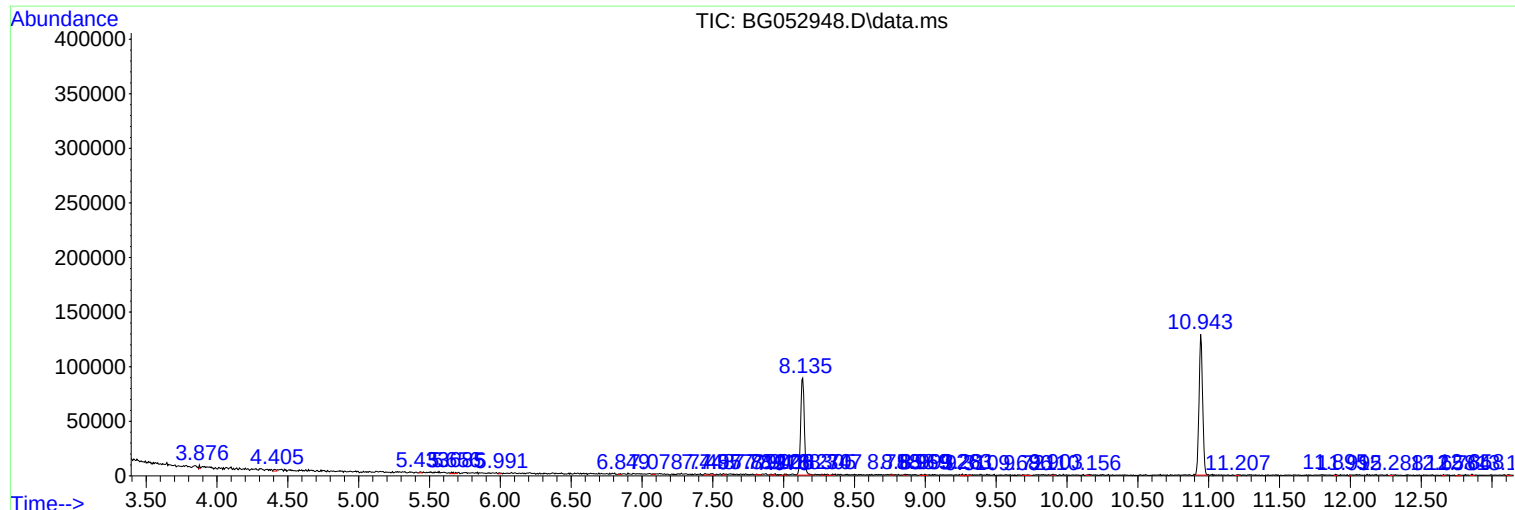

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052948.D
Acq On : 30 Mar 2022 13:56
Operator : CG/JU
Sample : N2130-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052948.D
Acq On : 30 Mar 2022 13:56
Operator : CG/JU
Sample : N2130-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc