

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052961.D
 Acq On : 30 Mar 2022 23:13
 Operator : CG/JU
 Sample : PB143726BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	24	27	36	rVB7	10171	16620	1.50%	0.163%
2	3.963	95	98	116	rVB	102920	175132	15.86%	1.716%
3	4.128	122	126	131	rVB5	2033	3207	0.29%	0.031%
4	4.856	246	250	252	rVB3	1582	2273	0.21%	0.022%
5	4.909	255	259	261	rBV3	1224	1556	0.14%	0.015%
6	5.015	276	277	280	rBV4	2347	2130	0.19%	0.021%
7	5.185	305	306	310	rVB4	2312	1746	0.16%	0.017%
8	5.267	318	320	322	rVB2	1955	1530	0.14%	0.015%
9	5.285	322	323	327	rVB3	1563	1676	0.15%	0.016%
10	5.355	332	335	337	rVV3	1292	1523	0.14%	0.015%
11	5.514	360	362	365	rBV2	1804	1986	0.18%	0.019%
12	6.284	491	493	498	rBV3	876	1424	0.13%	0.014%
13	6.472	521	525	529	rBV4	1049	1547	0.14%	0.015%
14	6.683	558	561	565	rBV2	875	1458	0.13%	0.014%
15	6.848	585	589	590	rBV2	1347	1652	0.15%	0.016%
16	7.276	654	662	672	rBV2	132263	231164	20.93%	2.265%
17	7.453	684	692	699	rVV	96897	167981	15.21%	1.646%
18	7.506	699	701	706	rVV4	1674	2372	0.21%	0.023%
19	7.664	721	728	736	rVV	124689	214502	19.42%	2.101%
20	8.134	801	808	817	rVB	87158	149933	13.57%	1.469%
21	8.827	919	926	933	rBV	160938	282466	25.57%	2.767%
22	9.291	997	1005	1012	rBV	132462	238533	21.60%	2.337%
23	10.020	1120	1129	1138	rBV	110816	199952	18.10%	1.959%
24	10.554	1213	1220	1228	rBV	162284	289769	26.23%	2.839%
25	10.807	1260	1263	1268	rBV2	1201	1769	0.16%	0.017%
26	10.948	1280	1287	1294	rBV	120317	222532	20.15%	2.180%
27	11.071	1300	1308	1321	rBV	162402	307635	27.85%	3.014%
28	12.117	1482	1486	1490	rVB2	742	1456	0.13%	0.014%
29	12.528	1549	1556	1561	rVB2	2541	4611	0.42%	0.045%
30	14.149	1825	1832	1838	rBV	372363	543737	49.23%	5.327%
31	14.449	1876	1883	1891	rVB	366012	585056	52.97%	5.731%
32	14.749	1928	1934	1943	rVB	226556	359977	32.59%	3.526%
33	14.925	1957	1964	1973	rBV	174750	285791	25.87%	2.800%
34	15.741	2096	2103	2111	rVB	515645	781101	70.72%	7.652%
35	15.847	2115	2121	2130	rBV	156471	241543	21.87%	2.366%
36	15.982	2136	2144	2149	rBV3	5457	7369	0.67%	0.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052961.D
 Acq On : 30 Mar 2022 23:13
 Operator : CG/JU
 Sample : PB143726BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	16.529	2231	2237	2238	rBV2	1745	1894	0.17%	0.019%
38	17.492	2395	2401	2410	rVV	313258	490034	44.36%	4.800%
39	17.592	2412	2418	2428	rVV2	570870	911936	82.56%	8.934%
40	17.997	2482	2487	2491	rVV4	1613	1953	0.18%	0.019%
41	18.032	2491	2493	2497	rVB2	1197	1696	0.15%	0.017%
42	18.743	2611	2614	2619	rBV2	2009	2994	0.27%	0.029%
43	18.914	2642	2643	2647	rBV3	1475	1415	0.13%	0.014%
44	18.978	2651	2654	2657	rBV3	1313	1686	0.15%	0.017%
45	19.125	2676	2679	2681	rBV2	1418	1614	0.15%	0.016%
46	19.313	2710	2711	2715	rVB2	1127	1470	0.13%	0.014%
47	19.442	2729	2733	2737	rBV4	9038	12818	1.16%	0.126%
48	19.507	2740	2744	2749	rBV2	9586	14124	1.28%	0.138%
49	19.707	2772	2778	2782	rVV5	1549	3513	0.32%	0.034%
50	19.754	2785	2786	2789	rVV3	2194	1464	0.13%	0.014%
51	19.812	2793	2796	2797	rBV3	2043	2220	0.20%	0.022%
52	19.877	2800	2807	2817	rVB	773662	1104551	100.00%	10.820%
53	20.124	2847	2849	2851	rVB3	1968	1452	0.13%	0.014%
54	20.341	2884	2886	2888	rBV3	2353	1896	0.17%	0.019%
55	20.605	2929	2931	2933	rBV3	2803	2645	0.24%	0.026%
56	21.246	3038	3040	3041	rBV	4204	2194	0.20%	0.021%
57	21.774	3124	3130	3138	rBV	323738	552930	50.06%	5.417%
58	22.033	3172	3174	3176	rVB3	3285	2375	0.22%	0.023%
59	22.051	3176	3177	3179	rBV2	2931	2102	0.19%	0.021%
60	22.098	3184	3185	3190	rVB5	3314	3310	0.30%	0.032%
61	22.468	3246	3248	3249	rBV2	3265	3050	0.28%	0.030%
62	22.573	3265	3266	3267	rBV	3323	1586	0.14%	0.016%
63	23.308	3387	3391	3395	rBV7	6825	11122	1.01%	0.109%
64	23.801	3473	3475	3476	rBV2	4408	3320	0.30%	0.033%
65	23.954	3499	3501	3504	rBV3	3419	2797	0.25%	0.027%
66	24.130	3529	3531	3533	rBV3	4315	4893	0.44%	0.048%
67	24.189	3539	3541	3544	rBV2	4303	5112	0.46%	0.050%
68	24.318	3559	3563	3565	rBV5	3835	6268	0.57%	0.061%
69	24.530	3597	3599	3600	rVB	4426	2718	0.25%	0.027%
70	24.553	3600	3603	3604	rBV3	3054	2715	0.25%	0.027%
71	24.735	3633	3634	3636	rBV2	3685	2088	0.19%	0.020%
72	24.858	3644	3655	3669	rBV2	369964	1062589	96.20%	10.409%
73	24.999	3677	3679	3680	rBV	2644	2338	0.21%	0.023%
74	25.088	3682	3694	3706	rVV2	188793	562069	50.89%	5.506%
75	25.399	3745	3747	3749	rBV3	3364	3173	0.29%	0.031%
76	25.528	3767	3769	3770	rBV2	2624	1561	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052961.D
 Acq On : 30 Mar 2022 23:13
 Operator : CG/JU
 Sample : PB143726BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	25.657	3790	3791	3795	rBV4	2716	1956	0.18%	0.019%
78	26.092	3863	3865	3866	rVB	3442	1883	0.17%	0.018%
79	26.239	3888	3890	3892	rBV3	3116	1706	0.15%	0.017%
80	26.262	3892	3894	3895	rBV2	4522	4128	0.37%	0.040%
81	26.280	3895	3897	3900	rBV4	4933	5793	0.52%	0.057%
82	26.462	3927	3928	3931	rBV2	4594	4192	0.38%	0.041%
83	26.691	3965	3967	3968	rBV2	2578	1735	0.16%	0.017%
84	26.915	4003	4005	4007	rBV3	2907	2825	0.26%	0.028%
85	27.020	4021	4023	4024	rVB2	3315	1527	0.14%	0.015%
86	27.126	4039	4041	4043	rBV3	4073	3938	0.36%	0.039%
87	27.149	4043	4045	4048	rVV3	4307	3902	0.35%	0.038%
88	27.478	4099	4101	4104	rVB4	3688	2710	0.25%	0.027%
89	27.625	4123	4126	4127	rBV3	3340	3650	0.33%	0.036%
90	28.019	4189	4193	4194	rBV3	3141	3240	0.29%	0.032%
91	28.095	4204	4206	4207	rBV2	3588	1673	0.15%	0.016%
92	28.183	4219	4221	4222	rBV2	3011	2285	0.21%	0.022%
93	28.912	4343	4345	4347	rBV3	2905	2766	0.25%	0.027%
94	29.176	4388	4390	4392	rBV3	3519	2551	0.23%	0.025%
95	30.351	4588	4590	4593	rBV3	3981	3319	0.30%	0.033%
96	30.480	4610	4612	4616	rBV5	3450	5487	0.50%	0.054%
97	31.238	4739	4741	4744	rBV2	3607	4921	0.45%	0.048%
98	31.585	4798	4800	4801	rBV2	3036	2110	0.19%	0.021%
99	32.495	4953	4955	4956	rBV2	3450	1752	0.16%	0.017%
100	32.548	4962	4964	4965	rVB2	3457	1552	0.14%	0.015%




Sum of corrected areas: 10207995

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052961.D
Acq On : 30 Mar 2022 23:13
Operator : CG/JU
Sample : PB143726BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

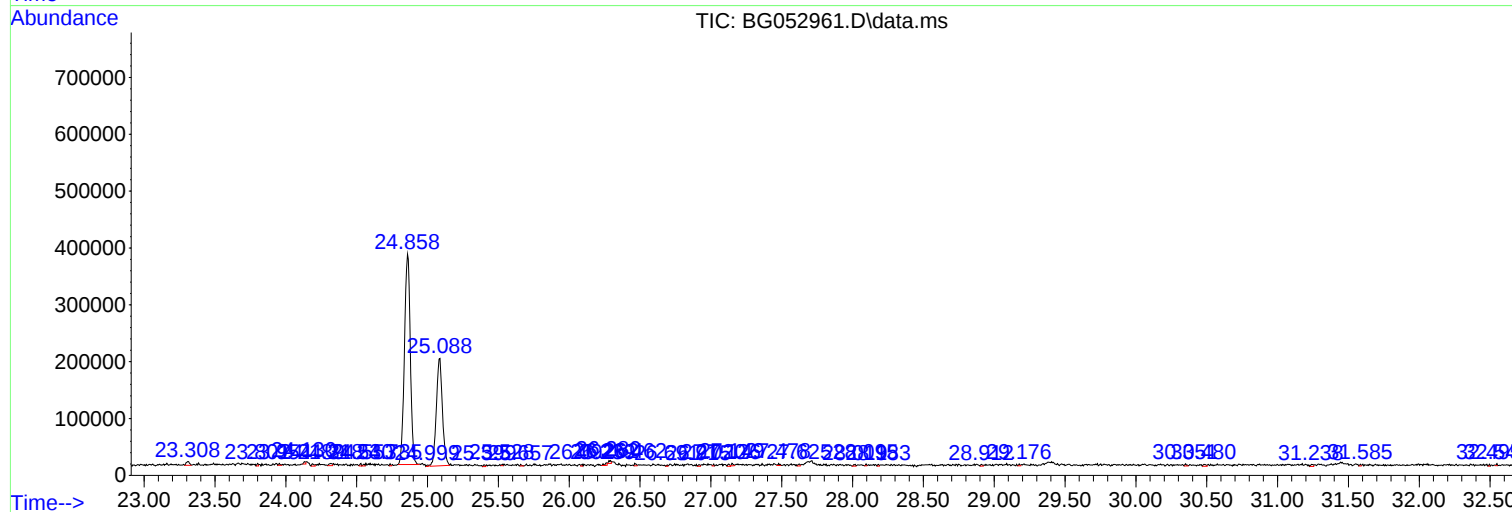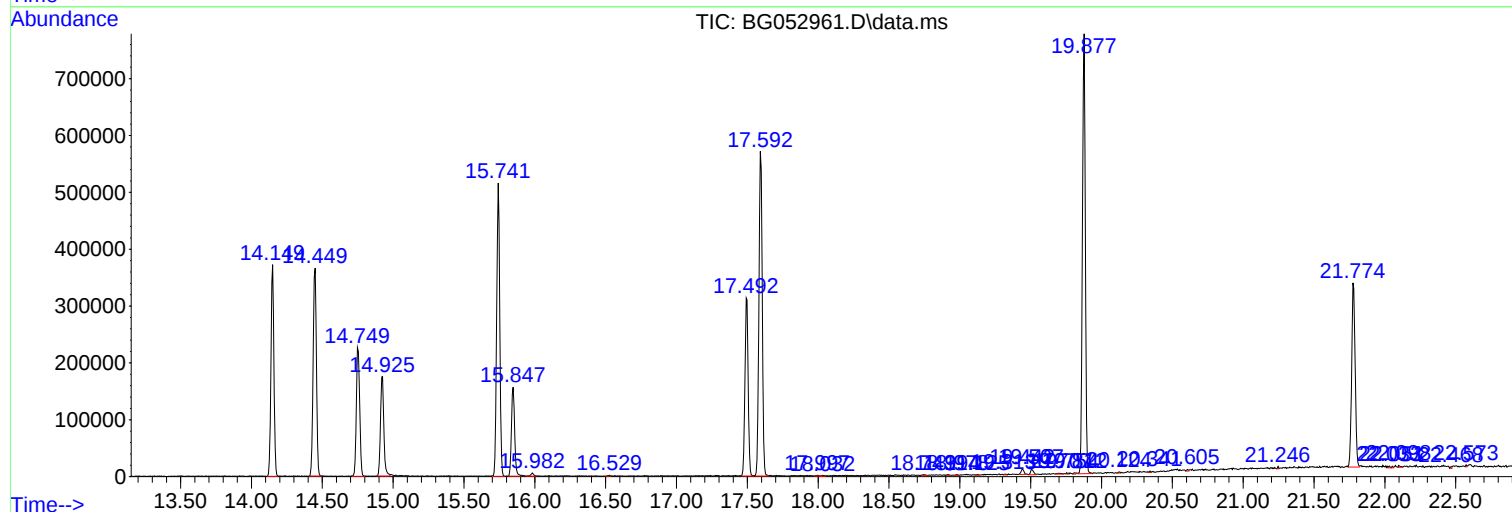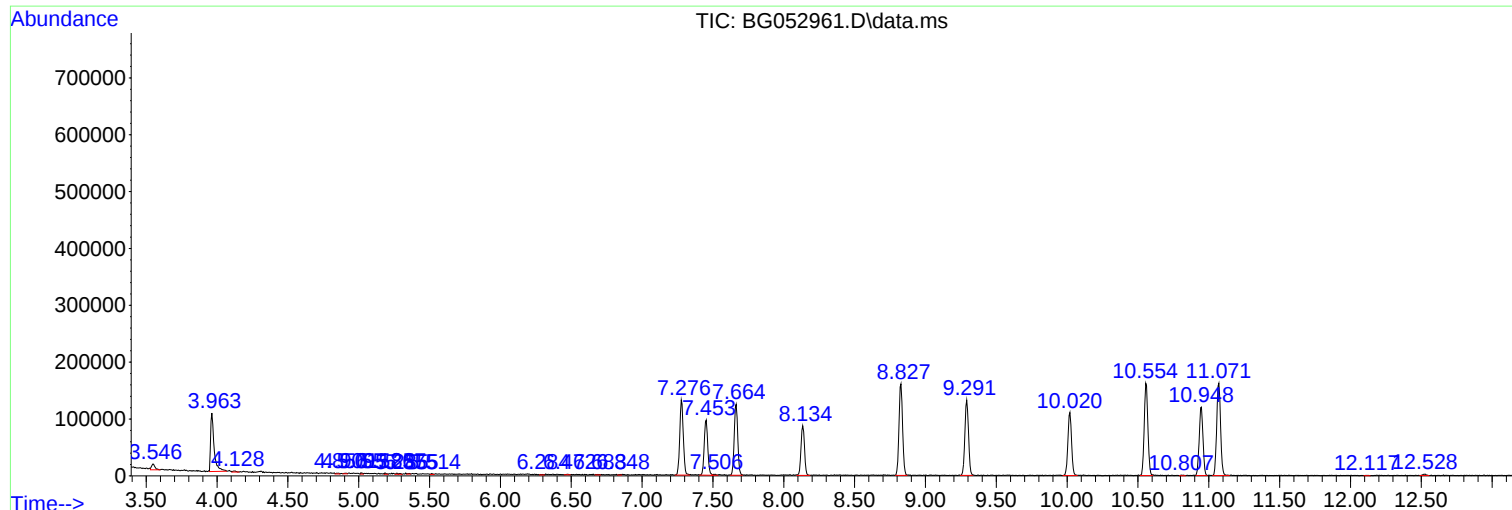

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052961.D
Acq On : 30 Mar 2022 23:13
Operator : CG/JU
Sample : PB143726BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052961.D
Acq On : 30 Mar 2022 23:13
Operator : CG/JU
Sample : PB143726BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK726

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------