

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052971.D
 Acq On : 31 Mar 2022 9:17
 Operator : CG/JU
 Sample : PB143753BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.542	23	26	30	rVV2	6413	7874	0.77%	0.081%
2	3.601	34	36	37	rBV2	2273	2148	0.21%	0.022%
3	3.959	94	97	109	rBV	80784	139163	13.53%	1.433%
4	4.165	130	132	135	rBV3	1288	1456	0.14%	0.015%
5	4.265	146	149	152	rBV3	1838	2297	0.22%	0.024%
6	4.294	152	154	156	rBV3	2379	2151	0.21%	0.022%
7	4.353	161	164	168	rBV4	1020	1398	0.14%	0.014%
8	4.441	178	179	183	rBV3	1143	1371	0.13%	0.014%
9	4.658	213	216	219	rBV5	2075	2267	0.22%	0.023%
10	4.999	271	274	275	rBV2	1920	1481	0.14%	0.015%
11	5.293	322	324	326	rBV3	1819	1457	0.14%	0.015%
12	5.833	413	416	417	rBV3	1904	1852	0.18%	0.019%
13	5.974	438	440	446	rBV3	842	1509	0.15%	0.016%
14	6.139	464	468	470	rBV3	1498	1720	0.17%	0.018%
15	6.620	546	550	552	rBV3	1106	1502	0.15%	0.015%
16	6.961	604	608	609	rBV2	1294	1682	0.16%	0.017%
17	7.061	623	625	627	rBV2	1224	1362	0.13%	0.014%
18	7.278	655	662	675	rVB	111150	195395	18.99%	2.012%
19	7.449	683	691	699	rBV	82698	140955	13.70%	1.451%
20	7.660	720	727	740	rVB	103363	181393	17.63%	1.868%
21	8.136	801	808	815	rVB	90991	155527	15.12%	1.601%
22	8.823	919	925	932	rBV	139619	236484	22.99%	2.435%
23	9.152	977	981	983	rBV2	963	1369	0.13%	0.014%
24	9.293	996	1005	1014	rBV	110811	203137	19.75%	2.092%
25	9.428	1024	1028	1030	rBV2	859	1397	0.14%	0.014%
26	10.016	1120	1128	1140	rBV2	91510	166114	16.15%	1.710%
27	10.556	1214	1220	1228	rVB2	137989	247248	24.04%	2.546%
28	10.944	1279	1286	1295	rVB	132587	243268	23.65%	2.505%
29	11.073	1301	1308	1319	rBV	140515	264217	25.69%	2.721%
30	12.518	1548	1554	1559	rVB3	2601	4718	0.46%	0.049%
31	14.151	1825	1832	1842	rVV	327080	486251	47.27%	5.007%
32	14.445	1876	1882	1892	rVB	318096	513377	49.91%	5.286%
33	14.756	1926	1935	1941	rBV	252764	400846	38.97%	4.127%
34	14.927	1957	1964	1974	rBV	157932	260378	25.31%	2.681%
35	15.003	1976	1977	1980	rVB2	2581	1463	0.14%	0.015%
36	15.743	2097	2103	2110	rVB	460393	700396	68.09%	7.212%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052971.D
 Acq On : 31 Mar 2022 9:17
 Operator : CG/JU
 Sample : PB143753BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.849	2115	2121	2127	rBV2	141867	216904	21.09%	2.233%
38	15.978	2140	2143	2149	rVB3	4394	6677	0.65%	0.069%
39	16.525	2234	2236	2239	rVV2	1253	1626	0.16%	0.017%
40	17.271	2360	2363	2364	rVV3	1593	1380	0.13%	0.014%
41	17.288	2364	2366	2369	rVB2	1972	1840	0.18%	0.019%
42	17.494	2395	2401	2408	rVB	360542	564287	54.86%	5.810%
43	17.594	2412	2418	2428	rVV2	547715	843150	81.96%	8.682%
44	17.758	2443	2446	2451	rBV	934	1533	0.15%	0.016%
45	18.422	2557	2559	2564	rBV4	1347	2242	0.22%	0.023%
46	18.545	2577	2580	2582	rVB3	1495	1670	0.16%	0.017%
47	18.804	2622	2624	2628	rVV3	1552	2016	0.20%	0.021%
48	18.851	2631	2632	2637	rVB	1583	2392	0.23%	0.025%
49	18.939	2644	2647	2649	rVV3	1439	1420	0.14%	0.015%
50	18.998	2655	2657	2663	rVB4	1521	2279	0.22%	0.023%
51	19.062	2667	2668	2674	rVV5	1093	1849	0.18%	0.019%
52	19.133	2678	2680	2681	rVV2	2215	1381	0.13%	0.014%
53	19.203	2689	2692	2696	rVV4	1723	3036	0.30%	0.031%
54	19.315	2708	2711	2713	rVB3	1470	1736	0.17%	0.018%
55	19.409	2724	2727	2728	rBV2	1356	1666	0.16%	0.017%
56	19.444	2728	2733	2737	rVV4	8595	12341	1.20%	0.127%
57	19.473	2737	2738	2741	rVV2	1328	1416	0.14%	0.015%
58	19.515	2741	2745	2749	rVB	6773	9927	0.97%	0.102%
59	19.585	2753	2757	2758	rBV4	1693	2176	0.21%	0.022%
60	19.638	2761	2766	2767	rBV5	1538	2483	0.24%	0.026%
61	19.685	2772	2774	2777	rVV4	1373	1971	0.19%	0.020%
62	19.708	2777	2778	2781	rVB3	1497	1429	0.14%	0.015%
63	19.797	2791	2793	2794	rBV2	1803	1374	0.13%	0.014%
64	19.879	2800	2807	2816	rVV	708040	1028679	100.00%	10.592%
65	20.501	2910	2913	2915	rBV3	4077	5449	0.53%	0.056%
66	20.601	2928	2930	2932	rVB3	2598	2323	0.23%	0.024%
67	20.701	2945	2947	2949	rVB2	2468	1488	0.14%	0.015%
68	20.883	2976	2978	2979	rBV2	2930	1980	0.19%	0.020%
69	21.083	3010	3012	3016	rBV5	4148	4327	0.42%	0.045%
70	21.412	3066	3068	3073	rVB4	3633	4438	0.43%	0.046%
71	21.782	3124	3131	3139	rVB	384855	638798	62.10%	6.578%
72	22.023	3170	3172	3175	rBV4	3222	4698	0.46%	0.048%
73	22.252	3210	3211	3212	rBV	3313	1650	0.16%	0.017%
74	22.446	3243	3244	3246	rBV2	3181	2453	0.24%	0.025%
75	22.963	3330	3332	3333	rBV2	3206	2366	0.23%	0.024%
76	23.204	3371	3373	3376	rBV4	3569	3462	0.34%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052971.D
 Acq On : 31 Mar 2022 9:17
 Operator : CG/JU
 Sample : PB143753BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK753

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	23.309	3388	3391	3395	rVB5	7645	10864	1.06%	0.112%
78	23.392	3403	3405	3407	rBV3	3905	3573	0.35%	0.037%
79	23.486	3419	3421	3425	rBV5	5842	10141	0.99%	0.104%
80	23.627	3442	3445	3448	rBV5	3876	7186	0.70%	0.074%
81	24.138	3529	3532	3538	rVB8	7192	13691	1.33%	0.141%
82	24.314	3560	3562	3563	rBV2	3133	2010	0.20%	0.021%
83	24.860	3645	3655	3670	rVB	331196	973771	94.66%	10.027%
84	25.089	3682	3694	3706	rBV2	210419	643011	62.51%	6.621%
85	25.589	3777	3779	3781	rVB2	3768	1998	0.19%	0.021%
86	25.653	3787	3790	3791	rBV3	3916	4284	0.42%	0.044%
87	26.141	3871	3873	3876	rBV4	2791	2977	0.29%	0.031%
88	26.300	3894	3900	3910	rVB4	8360	24563	2.39%	0.253%
89	26.417	3918	3920	3921	rBV2	3412	1855	0.18%	0.019%
90	27.686	4134	4136	4138	rBV3	5725	5366	0.52%	0.055%
91	28.256	4231	4233	4236	rBV4	3596	3633	0.35%	0.037%
92	28.555	4282	4284	4285	rVB2	3984	2057	0.20%	0.021%
93	28.790	4322	4324	4326	rBV3	3846	3458	0.34%	0.036%
94	30.453	4605	4607	4610	rBV2	3687	3633	0.35%	0.037%
95	30.711	4650	4651	4655	rBV4	5044	6032	0.59%	0.062%
96	31.393	4765	4767	4769	rBV3	2838	1778	0.17%	0.018%
97	31.416	4769	4771	4772	rBV2	3951	2713	0.26%	0.028%
98	31.745	4825	4827	4828	rBV2	3669	2298	0.22%	0.024%
99	32.209	4903	4906	4909	rBV5	4871	7881	0.77%	0.081%
100	32.615	4973	4975	4978	rBV4	3025	1965	0.19%	0.020%




Sum of corrected areas: 9711673

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052971.D
Acq On : 31 Mar 2022 9:17
Operator : CG/JU
Sample : PB143753BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

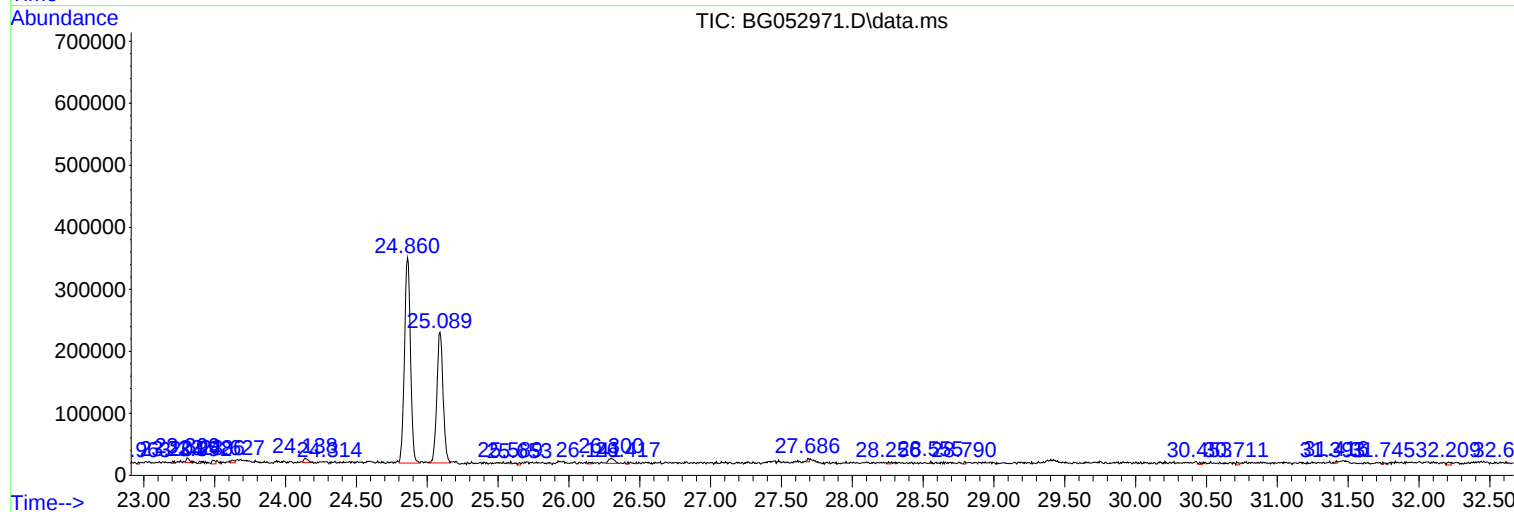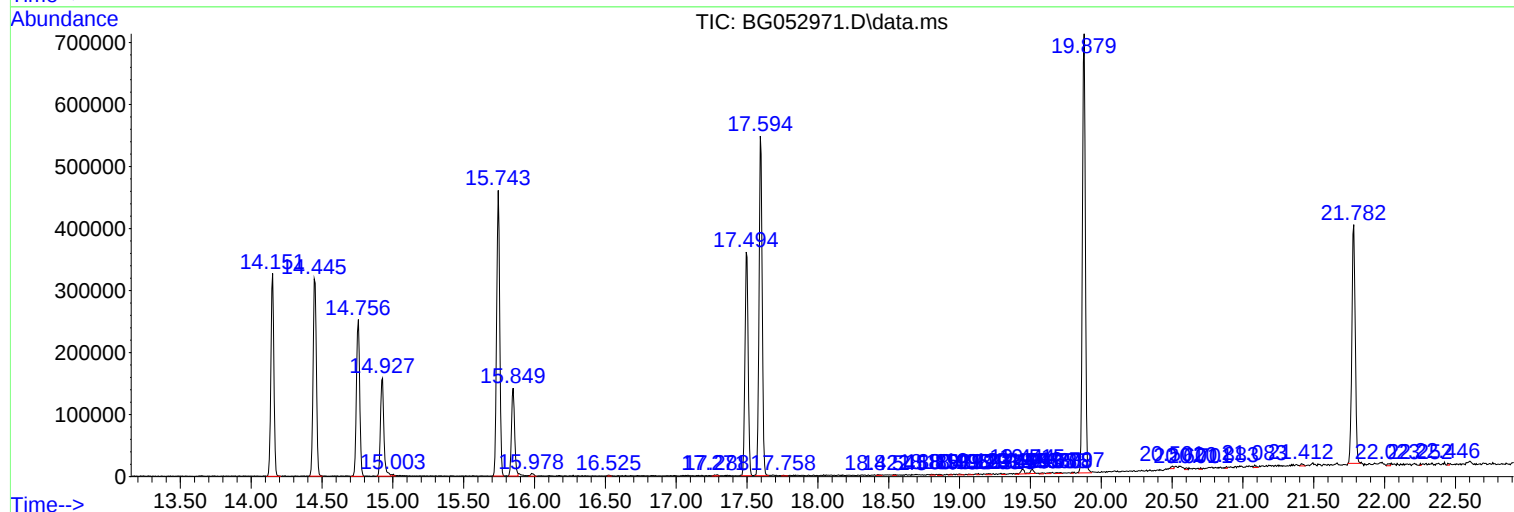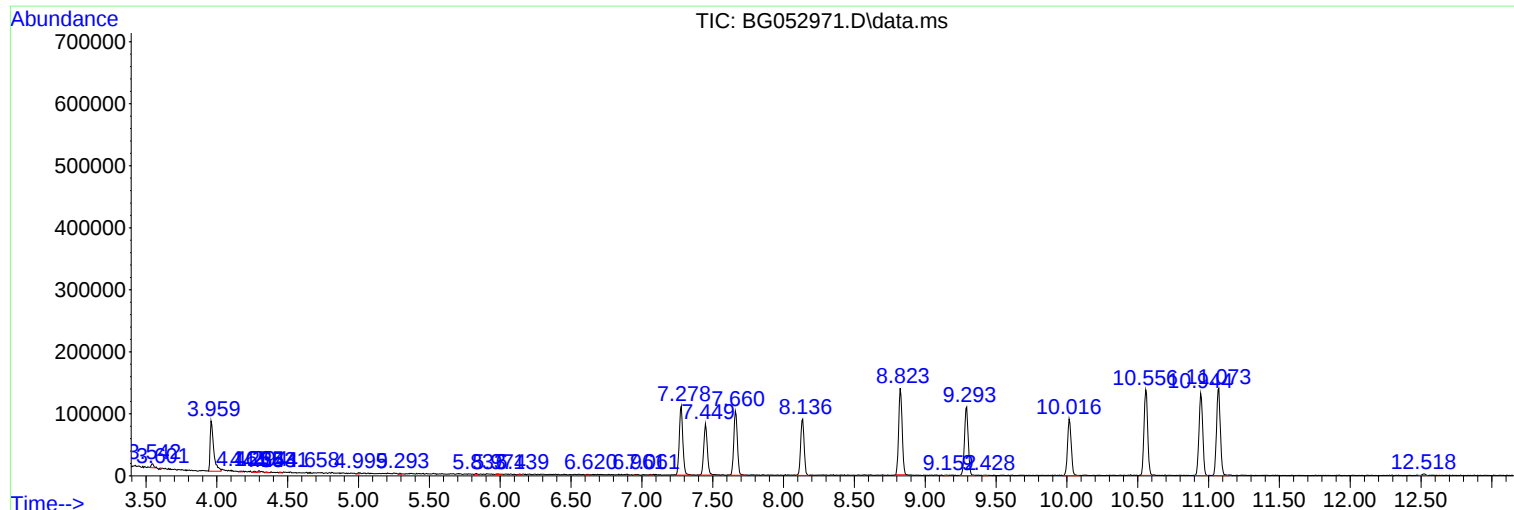

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052971.D
Acq On : 31 Mar 2022 9:17
Operator : CG/JU
Sample : PB143753BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052971.D
Acq On : 31 Mar 2022 9:17
Operator : CG/JU
Sample : PB143753BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK753

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc