

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052982.D
 Acq On : 31 Mar 2022 16:30
 Operator : CG/JU
 Sample : PB143754BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.545	24	27	33	rVB5	8615	14615	1.35%	0.145%
2	3.851	77	79	83	rVB3	3088	3396	0.31%	0.034%
3	3.962	95	98	111	rBV	86459	153551	14.20%	1.527%
4	4.098	120	121	124	rVB3	2834	1630	0.15%	0.016%
5	4.274	148	151	152	rBV2	2164	2133	0.20%	0.021%
6	4.385	168	170	172	rBV3	1972	1698	0.16%	0.017%
7	4.432	176	178	181	rVB4	2188	2056	0.19%	0.020%
8	5.214	310	311	314	rBV2	2085	1483	0.14%	0.015%
9	5.924	430	432	435	rVV4	1877	1512	0.14%	0.015%
10	6.518	529	533	535	rBV3	1251	1636	0.15%	0.016%
11	6.594	543	546	549	rBV3	1143	1550	0.14%	0.015%
12	6.618	549	550	554	rVB3	1409	1685	0.16%	0.017%
13	7.281	656	663	674	rVB	120085	208529	19.28%	2.073%
14	7.452	686	692	701	rBV	86474	150651	13.93%	1.498%
15	7.663	720	728	736	rVB2	117311	198236	18.33%	1.971%
16	7.740	739	741	746	rVB3	1126	1415	0.13%	0.014%
17	8.080	796	799	802	rBV3	1170	1578	0.15%	0.016%
18	8.133	802	808	816	rVB	95697	162722	15.05%	1.618%
19	8.251	824	828	831	rVB4	939	1433	0.13%	0.014%
20	8.826	918	926	937	rBV	146859	262305	24.25%	2.608%
21	9.290	997	1005	1015	rVV	122290	221565	20.49%	2.203%
22	10.019	1122	1129	1137	rBV2	101311	181717	16.80%	1.807%
23	10.113	1141	1145	1148	rBV3	942	1671	0.15%	0.017%
24	10.559	1213	1221	1232	rVV	152160	270456	25.01%	2.689%
25	10.947	1278	1287	1295	rVB	138978	250192	23.13%	2.487%
26	11.070	1301	1308	1316	rBV	148650	269028	24.88%	2.675%
27	11.141	1319	1320	1323	rVB3	1720	1448	0.13%	0.014%
28	11.781	1426	1429	1433	rBV3	1078	1600	0.15%	0.016%
29	11.999	1461	1466	1467	rBV	1187	1437	0.13%	0.014%
30	12.527	1548	1556	1558	rBV3	2514	4848	0.45%	0.048%
31	14.149	1826	1832	1838	rVB	348621	508144	46.99%	5.052%
32	14.448	1876	1883	1890	rVV	341168	532909	49.28%	5.298%
33	14.754	1928	1935	1942	rBV	248904	396946	36.70%	3.946%
34	14.924	1957	1964	1972	rBV	165896	266403	24.63%	2.649%
35	15.000	1975	1977	1981	rVB4	1706	1889	0.17%	0.019%
36	15.741	2096	2103	2110	rBV	457350	717701	66.36%	7.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052982.D
 Acq On : 31 Mar 2022 16:30
 Operator : CG/JU
 Sample : PB143754BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.846	2116	2121	2134	rVV2	155139	238134	22.02%	2.368%
38	15.981	2140	2144	2152	rVB3	4671	7695	0.71%	0.077%
39	16.269	2188	2193	2196	rVB3	1266	2227	0.21%	0.022%
40	16.522	2235	2236	2243	rVB4	1516	2293	0.21%	0.023%
41	17.227	2353	2356	2361	rBV2	1300	1574	0.15%	0.016%
42	17.286	2361	2366	2370	rBV2	1444	2685	0.25%	0.027%
43	17.497	2394	2402	2408	rBV	351969	548600	50.73%	5.454%
44	17.597	2412	2419	2427	rVV2	554762	860628	79.58%	8.556%
45	17.861	2461	2464	2468	rVB3	1009	1611	0.15%	0.016%
46	18.014	2488	2490	2493	rBV2	1608	1737	0.16%	0.017%
47	18.607	2588	2591	2595	rVB4	1139	1968	0.18%	0.020%
48	18.948	2647	2649	2652	rVB3	1550	1649	0.15%	0.016%
49	19.160	2681	2685	2686	rBV4	1844	1693	0.16%	0.017%
50	19.259	2699	2702	2703	rBV2	1859	1887	0.17%	0.019%
51	19.342	2715	2716	2721	rBV4	1768	2052	0.19%	0.020%
52	19.441	2729	2733	2738	rBV2	8619	12021	1.11%	0.120%
53	19.518	2741	2746	2749	rBV2	7824	11501	1.06%	0.114%
54	19.559	2751	2753	2756	rVB4	2438	2653	0.25%	0.026%
55	19.600	2756	2760	2763	rBV4	2107	3012	0.28%	0.030%
56	19.694	2774	2776	2779	rVB3	2229	2050	0.19%	0.020%
57	19.735	2779	2783	2785	rBV3	1637	2840	0.26%	0.028%
58	19.876	2800	2807	2815	rBV	781006	1081476	100.00%	10.752%
59	20.052	2835	2837	2839	rVB3	1443	1464	0.14%	0.015%
60	20.158	2853	2855	2859	rBV4	2295	2464	0.23%	0.024%
61	20.217	2863	2865	2867	rBV3	3101	3296	0.30%	0.033%
62	20.246	2869	2870	2872	rBV2	2529	2164	0.20%	0.022%
63	20.317	2880	2882	2884	rBV3	1990	1695	0.16%	0.017%
64	20.387	2891	2894	2896	rBV3	1501	1889	0.17%	0.019%
65	20.464	2905	2907	2909	rBV3	3367	3324	0.31%	0.033%
66	20.511	2910	2915	2917	rVV5	4670	8459	0.78%	0.084%
67	20.722	2948	2951	2953	rBV4	2829	3170	0.29%	0.032%
68	21.263	3042	3043	3046	rBV3	2615	2881	0.27%	0.029%
69	21.368	3058	3061	3062	rBV2	3068	3041	0.28%	0.030%
70	21.562	3092	3094	3098	rVB4	4434	4825	0.45%	0.048%
71	21.779	3124	3131	3139	rBV	369900	627557	58.03%	6.239%
72	21.932	3155	3157	3159	rBV3	2979	2158	0.20%	0.021%
73	22.884	3317	3319	3320	rVB2	3810	1959	0.18%	0.019%
74	22.902	3320	3322	3324	rBV2	3327	4011	0.37%	0.040%
75	23.800	3473	3475	3476	rBV2	3073	1928	0.18%	0.019%
76	24.141	3528	3533	3540	rBV10	7425	16381	1.51%	0.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG052982.D
 Acq On : 31 Mar 2022 16:30
 Operator : CG/JU
 Sample : PB143754BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK754

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

77	24.206	3542	3544	3546	rVB3	4180	3112	0.29%	0.031%
78	24.705	3627	3629	3633	rBV4	3523	4950	0.46%	0.049%
79	24.858	3644	3655	3670	rVB2	364898	1077027	99.59%	10.708%
80	25.087	3683	3694	3711	rVB2	211168	633390	58.57%	6.297%
81	25.310	3728	3732	3733	rBV3	4210	4738	0.44%	0.047%
82	25.375	3741	3743	3745	rBV3	3118	1980	0.18%	0.020%
83	26.279	3895	3897	3898	rBV2	5502	3963	0.37%	0.039%
84	26.679	3963	3965	3967	rBV2	3419	3743	0.35%	0.037%
85	26.961	4011	4013	4015	rBV3	3147	2663	0.25%	0.026%
86	27.172	4046	4049	4050	rBV3	4653	4334	0.40%	0.043%
87	27.378	4082	4084	4085	rBV2	4330	3635	0.34%	0.036%
88	27.807	4155	4157	4158	rBV2	3618	1742	0.16%	0.017%
89	27.936	4177	4179	4180	rVB2	3590	1415	0.13%	0.014%
90	27.971	4183	4185	4186	rBV2	3063	2179	0.20%	0.022%
91	28.359	4249	4251	4253	rBV3	3344	2242	0.21%	0.022%
92	29.169	4387	4389	4390	rBV2	3182	1626	0.15%	0.016%
93	29.293	4408	4410	4411	rBV	3194	1868	0.17%	0.019%
94	29.869	4506	4508	4511	rBV4	2893	2582	0.24%	0.026%
95	30.368	4590	4593	4594	rBV3	3461	3098	0.29%	0.031%
96	30.573	4627	4628	4630	rBV2	3131	1430	0.13%	0.014%
97	30.597	4630	4632	4633	rBV2	3357	1829	0.17%	0.018%
98	31.590	4799	4801	4804	rBV4	2645	2734	0.25%	0.027%
99	32.524	4959	4960	4962	rVB2	4300	1945	0.18%	0.019%
100	32.547	4962	4964	4967	rBV3	3065	3800	0.35%	0.038%


Sum of corrected areas: 10058445

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052982.D
Acq On : 31 Mar 2022 16:30
Operator : CG/JU
Sample : PB143754BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

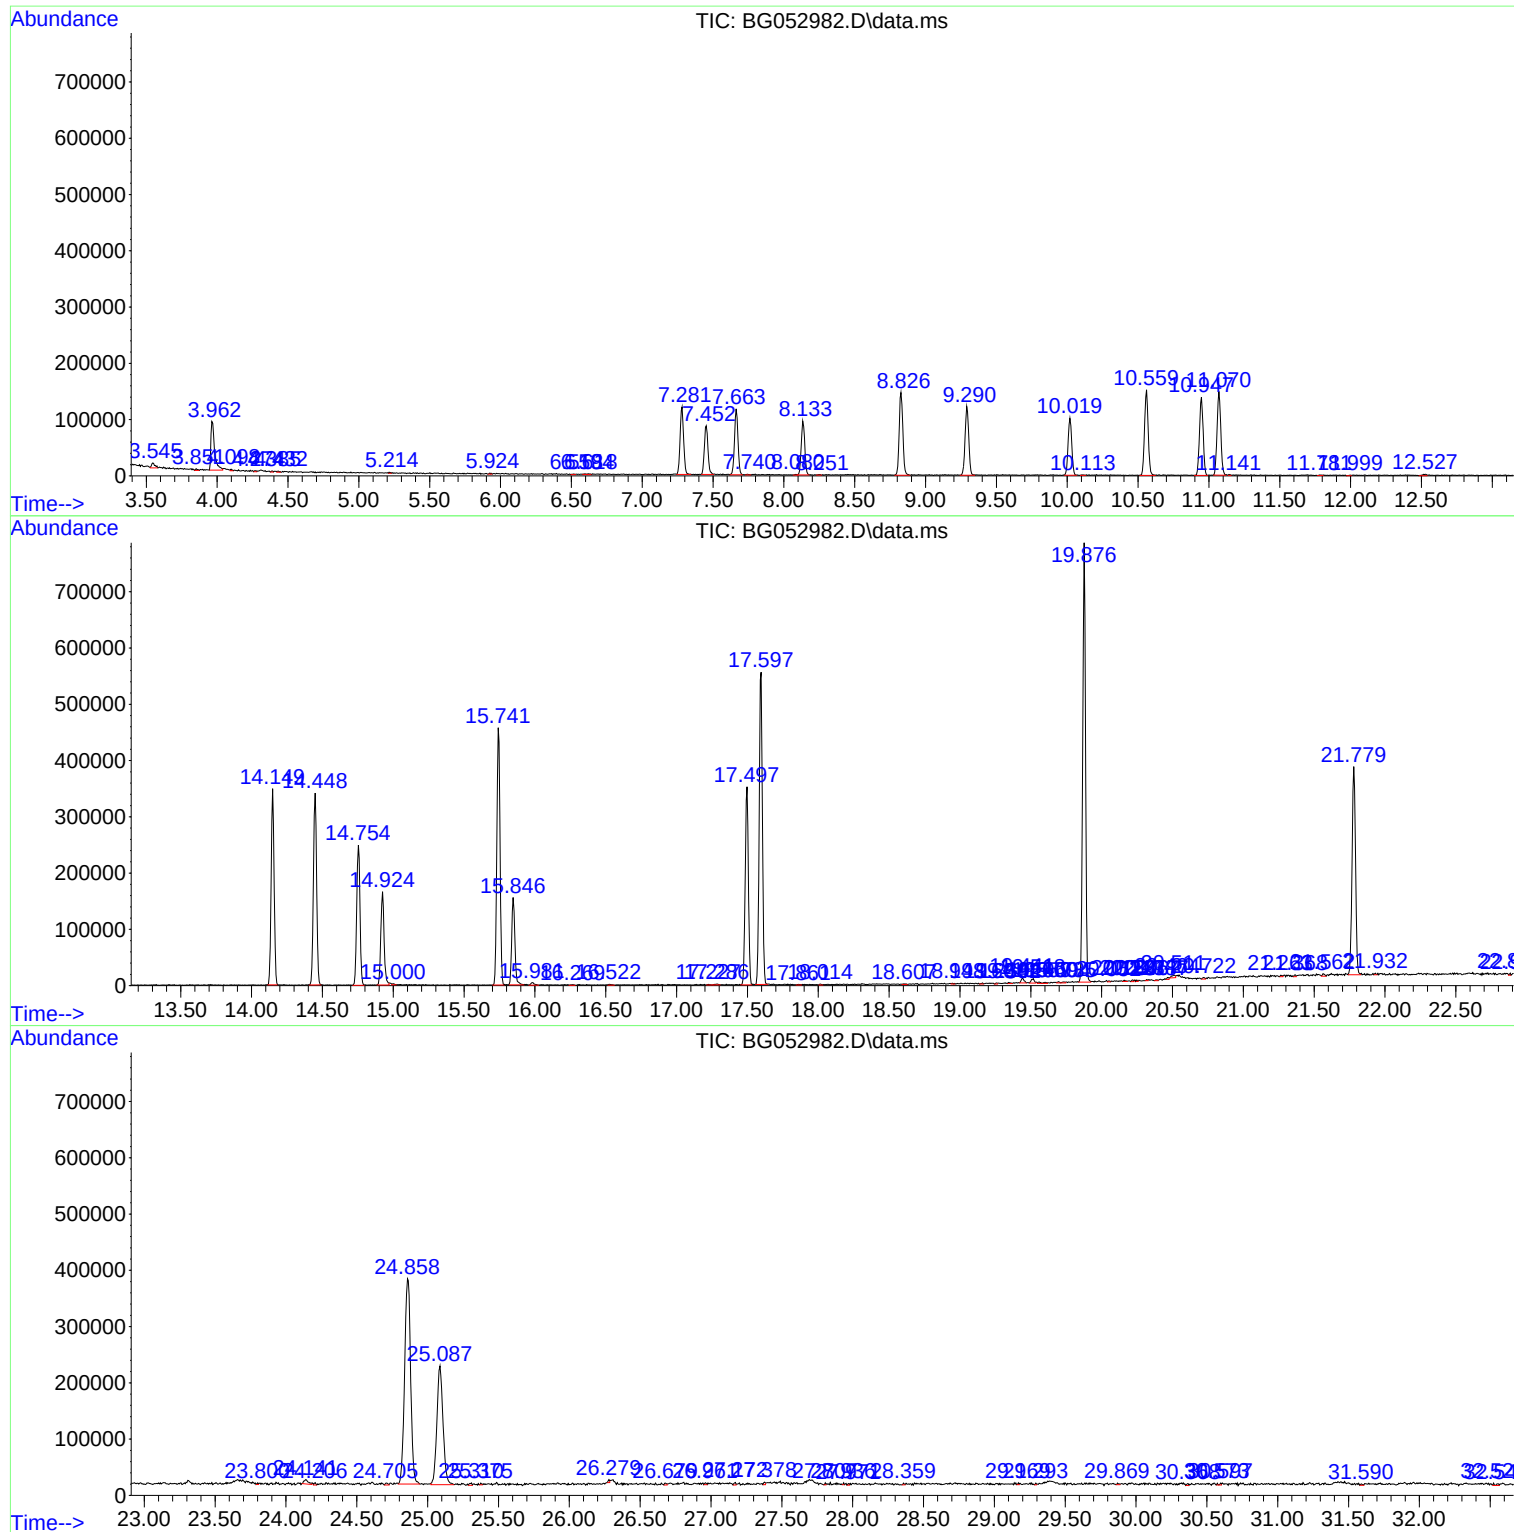

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052982.D
Acq On : 31 Mar 2022 16:30
Operator : CG/JU
Sample : PB143754BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG052982.D
Acq On : 31 Mar 2022 16:30
Operator : CG/JU
Sample : PB143754BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK754

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc