

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG053003.D
 Acq On : 1 Apr 2022 18:51
 Operator : CG/JU
 Sample : N2166-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0R41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

Signal : TIC: BG053003.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	25	28	30	rBV4	5087	5247	0.47%	0.053%
2	3.986	100	102	105	rBV2	9231	11474	1.02%	0.116%
3	4.304	154	156	161	rVB4	3152	2799	0.25%	0.028%
4	5.954	432	437	439	rVB4	1251	2203	0.20%	0.022%
5	5.990	439	443	446	rBV4	1025	1917	0.17%	0.019%
6	6.313	495	498	501	rBV4	1544	2020	0.18%	0.020%
7	7.282	655	663	671	rBV	36163	68048	6.07%	0.689%
8	7.447	686	691	701	rVB	96128	166406	14.84%	1.684%
9	7.664	720	728	735	rBV	101764	181830	16.22%	1.840%
10	8.134	801	808	817	rVB	109746	191562	17.09%	1.939%
11	8.363	842	847	851	rVB4	1359	2506	0.22%	0.025%
12	8.580	880	884	887	rVB2	962	1455	0.13%	0.015%
13	8.827	917	926	934	rBV	92095	164748	14.70%	1.668%
14	9.291	996	1005	1015	rBV2	136968	247911	22.11%	2.509%
15	9.456	1030	1033	1035	rVB3	1376	1530	0.14%	0.015%
16	9.726	1073	1079	1083	rBV3	3931	6915	0.62%	0.070%
17	10.014	1121	1128	1136	rBV2	109007	202913	18.10%	2.054%
18	10.278	1168	1173	1176	rBV2	904	1636	0.15%	0.017%
19	10.560	1212	1221	1229	rBV	153714	281637	25.12%	2.851%
20	10.713	1241	1247	1256	rBV3	3287	7717	0.69%	0.078%
21	10.942	1279	1286	1296	rBV	159081	286282	25.54%	2.898%
22	11.071	1300	1308	1317	rBV2	108527	199469	17.79%	2.019%
23	12.211	1496	1502	1507	rBV3	5571	9165	0.82%	0.093%
24	12.516	1550	1554	1562	rVB3	2856	5778	0.52%	0.058%
25	13.356	1693	1697	1700	rBV2	1141	1450	0.13%	0.015%
26	13.579	1732	1735	1738	rVB2	1299	1809	0.16%	0.018%
27	14.149	1825	1832	1841	rBV	362539	533025	47.54%	5.395%
28	14.378	1867	1871	1874	rBV5	3121	4709	0.42%	0.048%
29	14.449	1874	1883	1890	rVB	355595	584647	52.15%	5.918%
30	14.643	1913	1916	1918	rBV2	1946	1581	0.14%	0.016%
31	14.754	1928	1935	1943	rBV	264200	430805	38.43%	4.360%
32	14.925	1954	1964	1974	rBV2	38669	70950	6.33%	0.718%
33	15.377	2037	2041	2047	rVB3	1758	1867	0.17%	0.019%
34	15.541	2065	2069	2070	rBV2	1959	2174	0.19%	0.022%
35	15.588	2074	2077	2082	rVB4	1840	2636	0.24%	0.027%
36	15.741	2096	2103	2112	rBV2	514750	788902	70.37%	7.985%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
 Data File : BG053003.D
 Acq On : 1 Apr 2022 18:51
 Operator : CG/JU
 Sample : N2166-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0R41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
 Title : SVOA CALIBRATION

37	15.847	2115	2121	2127	rBV	180326	275832	24.60%	2.792%
38	15.976	2140	2143	2148	rVB4	5363	7469	0.67%	0.076%
39	16.082	2158	2161	2164	rBV3	1098	1516	0.14%	0.015%
40	16.376	2206	2211	2214	rBV2	1606	3410	0.30%	0.035%
41	16.423	2216	2219	2221	rVV3	4664	4992	0.45%	0.051%
42	16.446	2221	2223	2227	rVV4	2849	4087	0.36%	0.041%
43	16.475	2227	2228	2232	rVV3	1879	2001	0.18%	0.020%
44	16.528	2232	2237	2239	rVV4	2172	3133	0.28%	0.032%
45	16.622	2248	2253	2258	rBV4	2503	4369	0.39%	0.044%
46	16.957	2309	2310	2313	rVB4	1871	1597	0.14%	0.016%
47	17.239	2354	2358	2361	rVB4	3222	3987	0.36%	0.040%
48	17.286	2361	2366	2369	rBV5	2377	3327	0.30%	0.034%
49	17.398	2383	2385	2389	rVB2	2378	2783	0.25%	0.028%
50	17.498	2395	2402	2408	rBV	349031	558763	49.84%	5.656%
51	17.592	2412	2418	2425	rBV	616837	955102	85.19%	9.667%
52	17.774	2445	2449	2450	rBV	2350	1822	0.16%	0.018%
53	17.856	2459	2463	2464	rBV3	1951	1846	0.16%	0.019%
54	17.985	2482	2485	2486	rVB2	1897	1737	0.15%	0.018%
55	18.156	2507	2514	2517	rBV4	2939	6419	0.57%	0.065%
56	18.385	2548	2553	2556	rBV5	8615	15785	1.41%	0.160%
57	18.620	2592	2593	2596	rBV2	1694	1467	0.13%	0.015%
58	18.672	2601	2602	2606	rVB2	2277	2426	0.22%	0.025%
59	18.796	2619	2623	2628	rBV4	14287	19705	1.76%	0.199%
60	19.142	2681	2682	2685	rBV3	3031	2200	0.20%	0.022%
61	19.242	2696	2699	2701	rBV3	2207	2518	0.22%	0.025%
62	19.436	2729	2732	2737	rVB4	10856	13049	1.16%	0.132%
63	19.513	2741	2745	2748	rBV2	9219	11271	1.01%	0.114%
64	19.877	2800	2807	2813	rBV	754158	1121098	100.00%	11.347%
65	21.774	3124	3130	3139	rVB	362745	626945	55.92%	6.346%
66	24.858	3645	3655	3666	rVB2	397157	1118300	99.75%	11.319%
67	25.081	3684	3693	3707	rVB2	215248	623173	55.59%	6.308%




Sum of corrected areas: 9879852

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG053003.D
Acq On : 1 Apr 2022 18:51
Operator : CG/JU
Sample : N2166-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0R41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

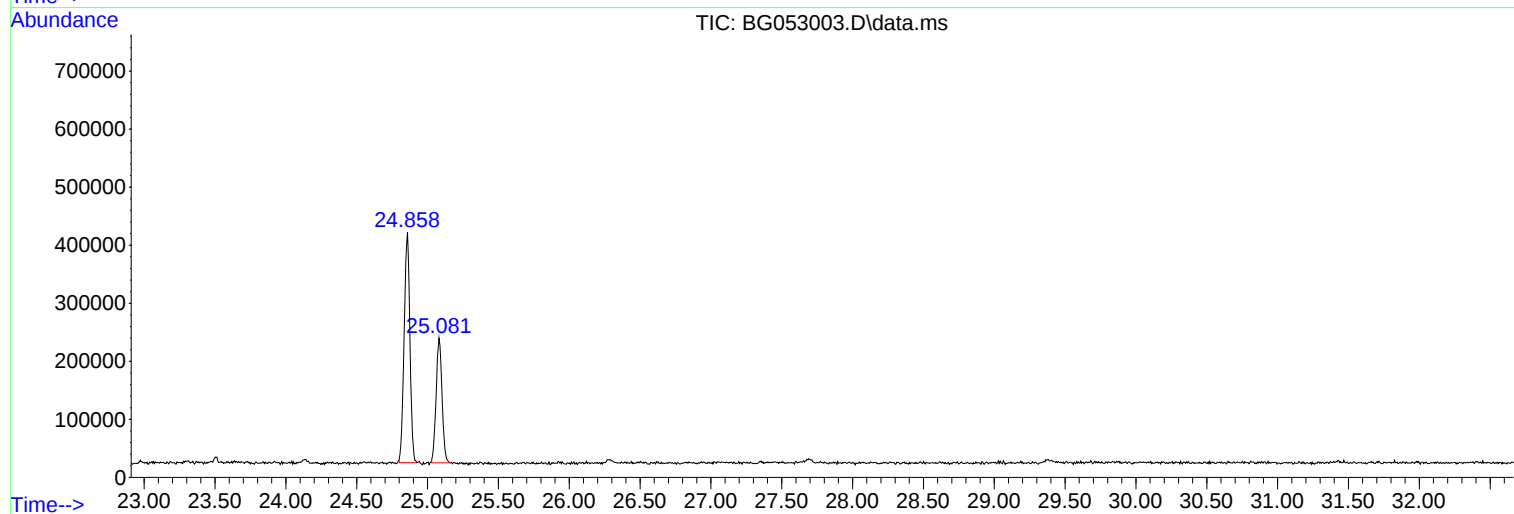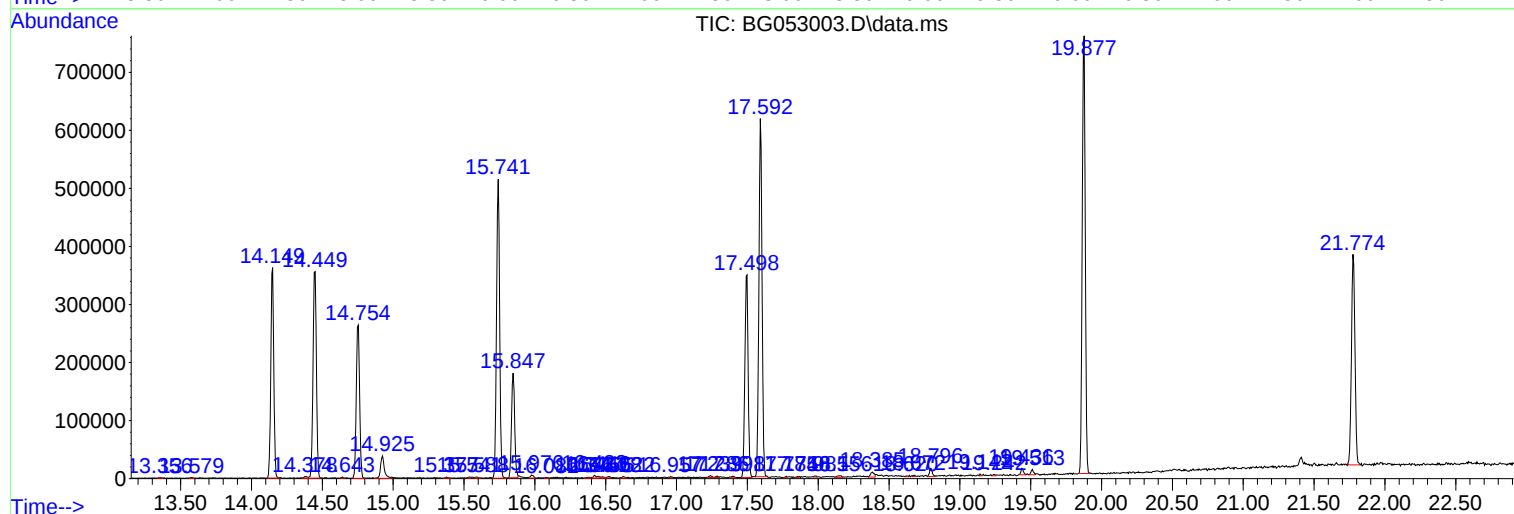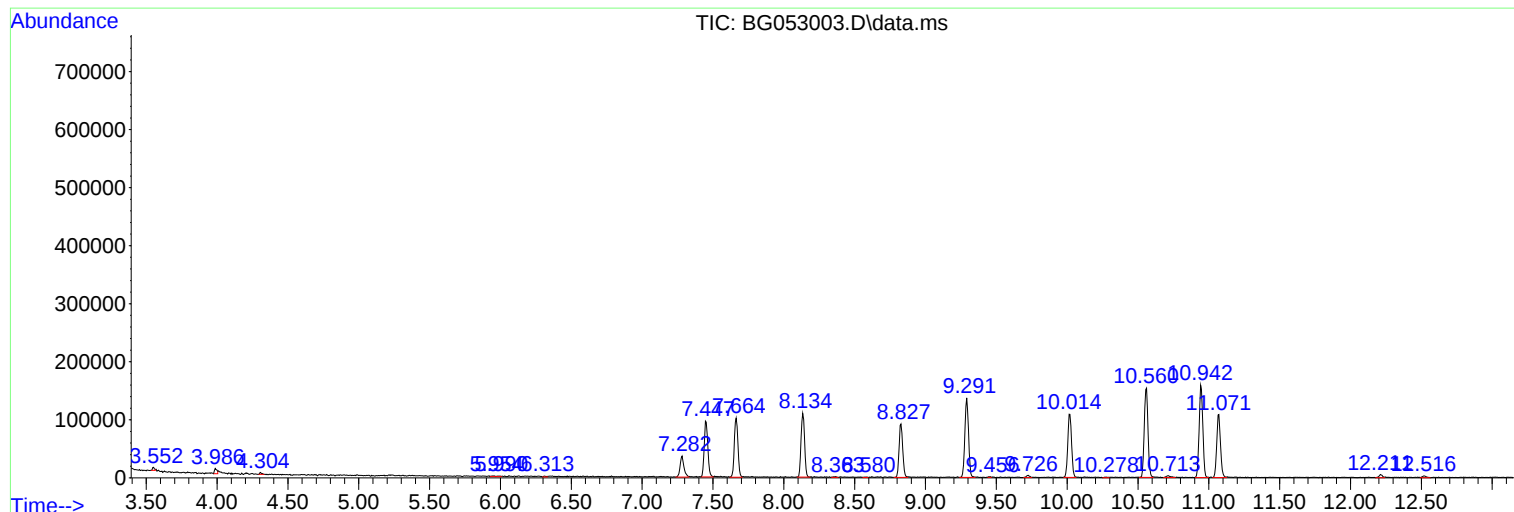

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG053003.D
Acq On : 1 Apr 2022 18:51
Operator : CG/JU
Sample : N2166-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0R41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033022\
Data File : BG053003.D
Acq On : 1 Apr 2022 18:51
Operator : CG/JU
Sample : N2166-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0R41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG031822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------