
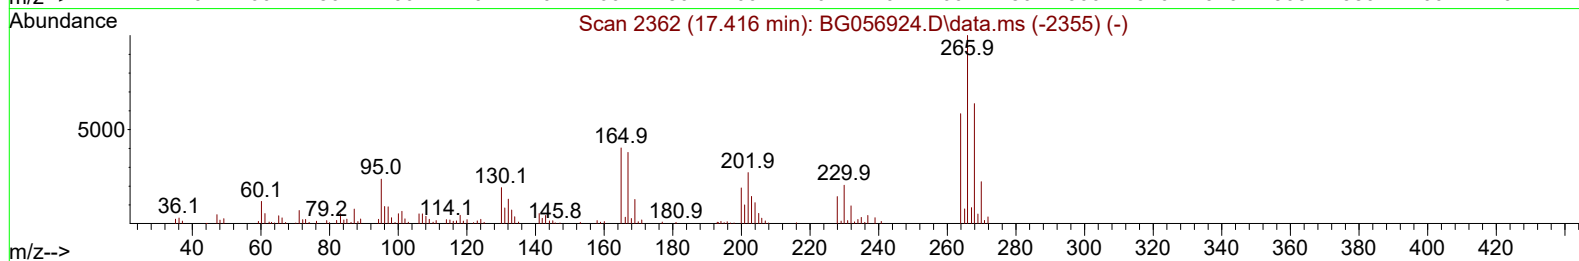
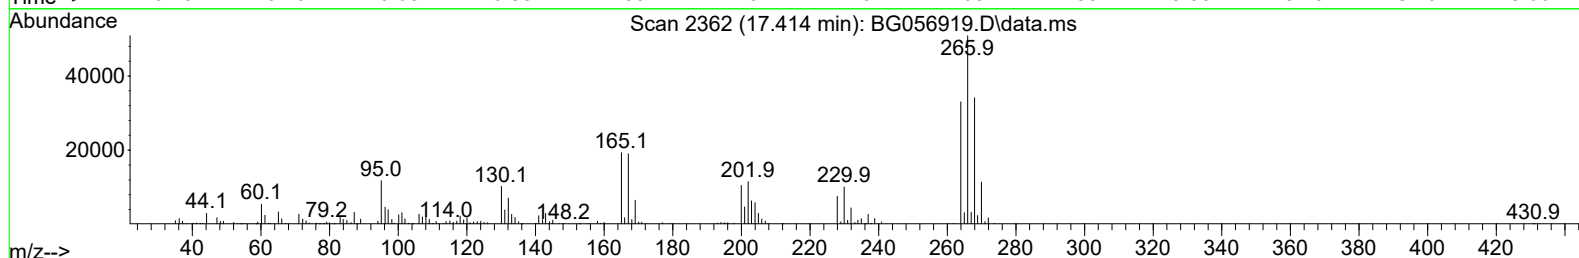


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033023\
Data File : BG056919.D
Acq On : 30 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:59:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

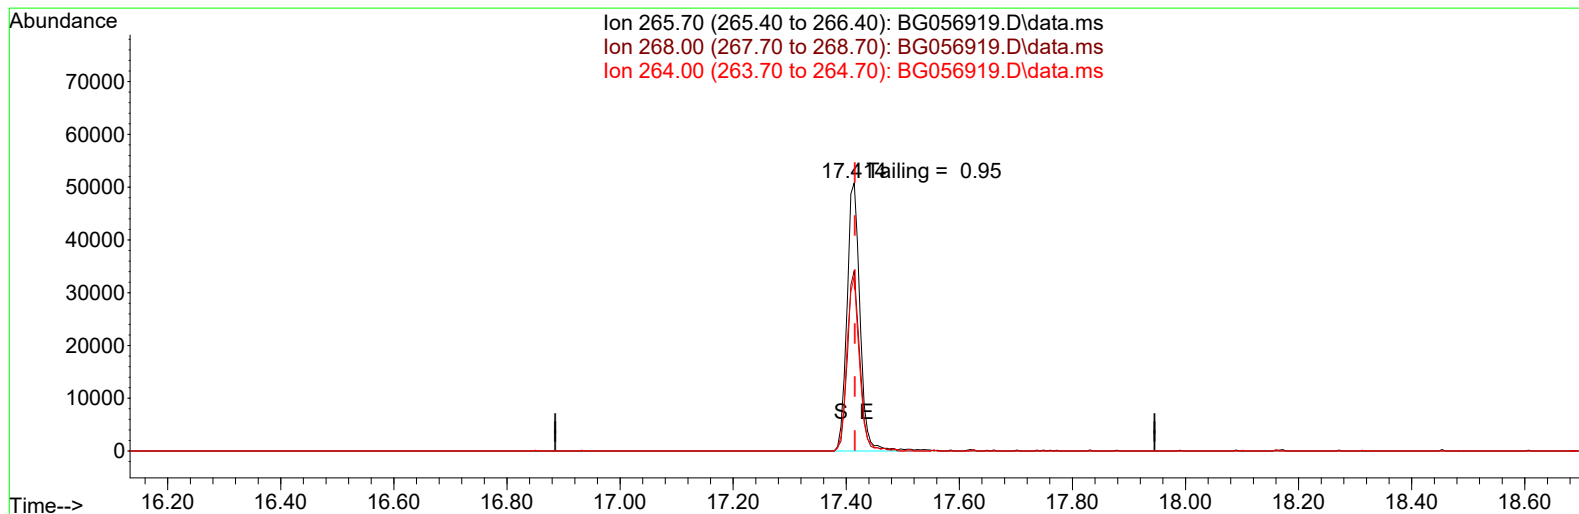

TIC: BG056919.D\data.ms

(70) Pentachlorophenol (C)




17.414min (-0.002) 19773.86 ng

response 80694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	67.12
264.00	58.50	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033023\
Data File : BG056919.D
Acq On : 30 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 04:59:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

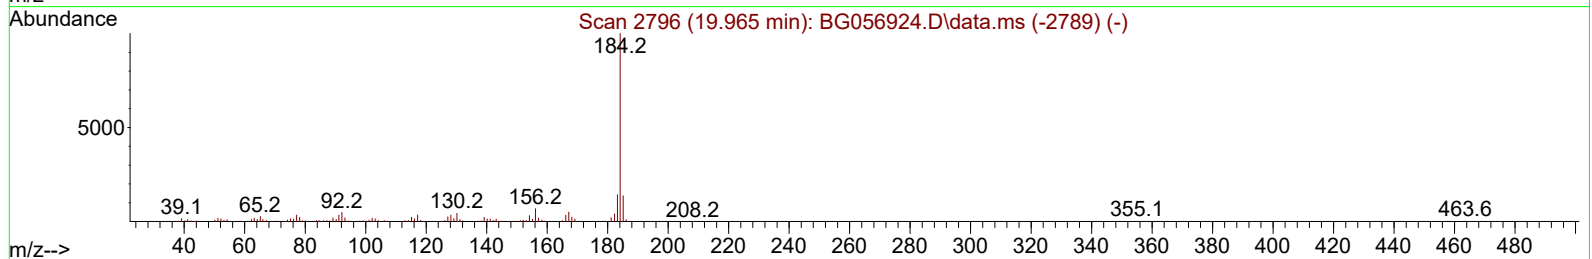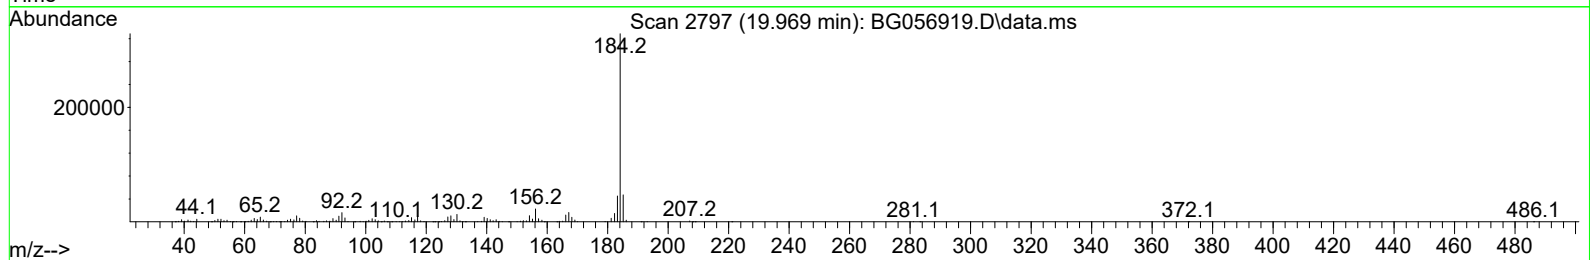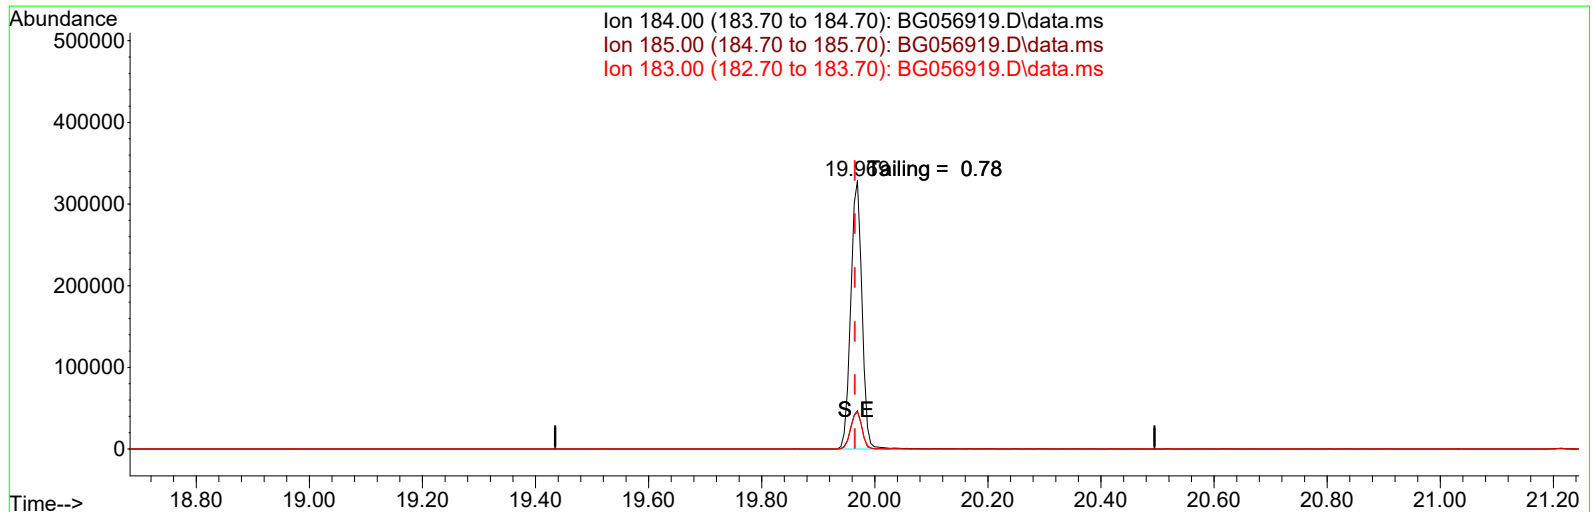

TIC: BG056919.D\data.ms

(77) Benzidine**19.969min (+ 0.004) 262447.26 ng****response 451933**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.33
183.00	14.20	13.77
0.00	0.00	0.00