


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033023\
Data File : BG056919.D
Acq On : 30 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 03:23:11 2023

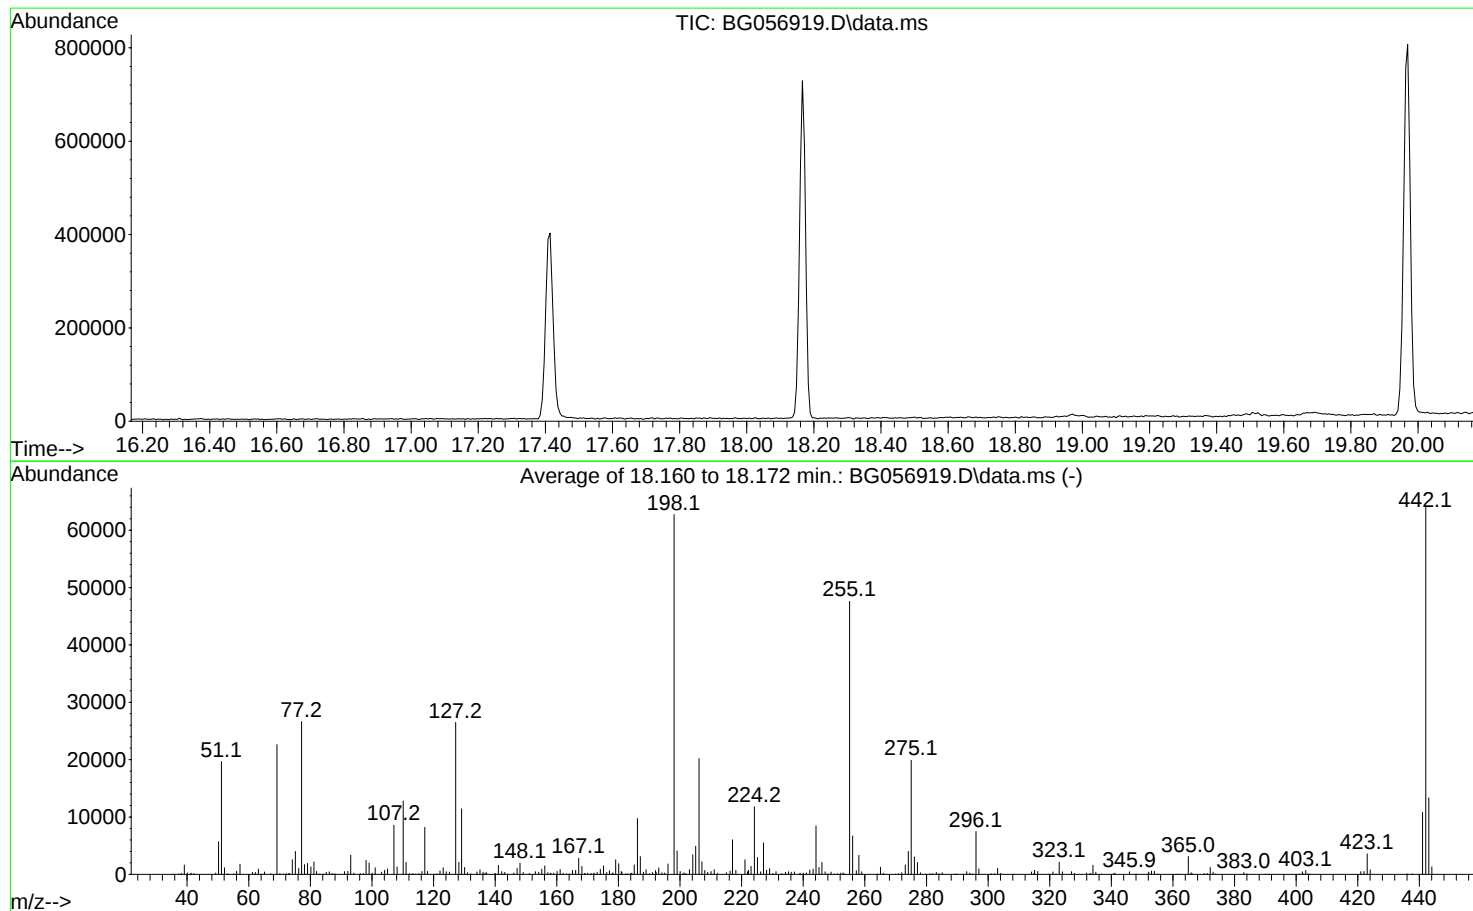




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	19676	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.0	22613	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	42.2	26501	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62736	PASS
199	198	5	9	6.5	4070	PASS
275	198	10	60	31.7	19881	PASS
365	198	1	100	5.0	3124	PASS
441	198	0.01	100	17.2	10804	PASS
442	442	50	100	100.0	64139	PASS
443	442	15	24	20.8	13331	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033023\
Data File : BG056919.D
Acq On : 30 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 04:59:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

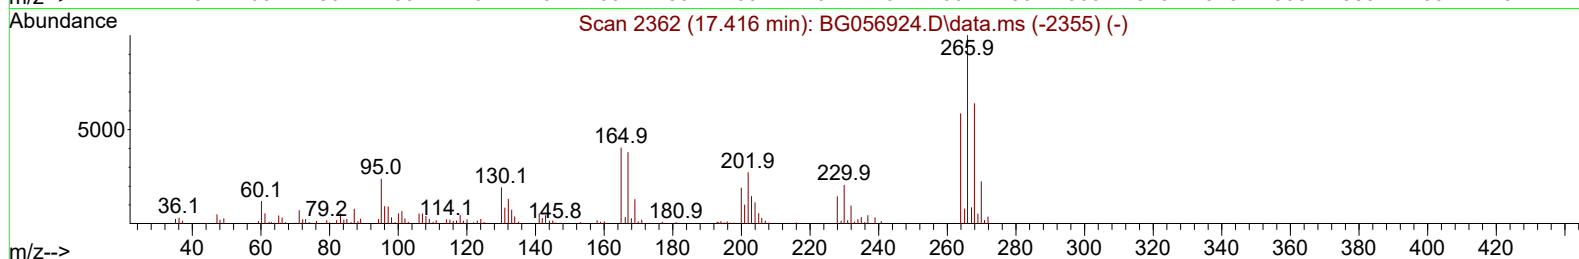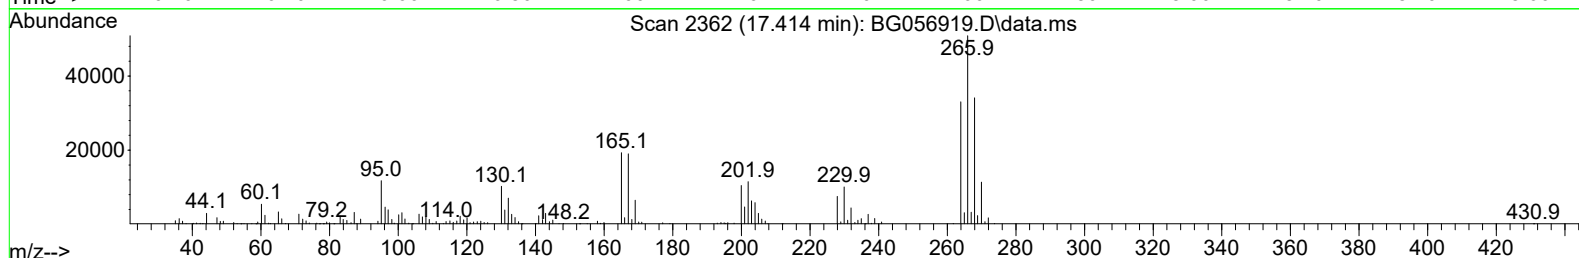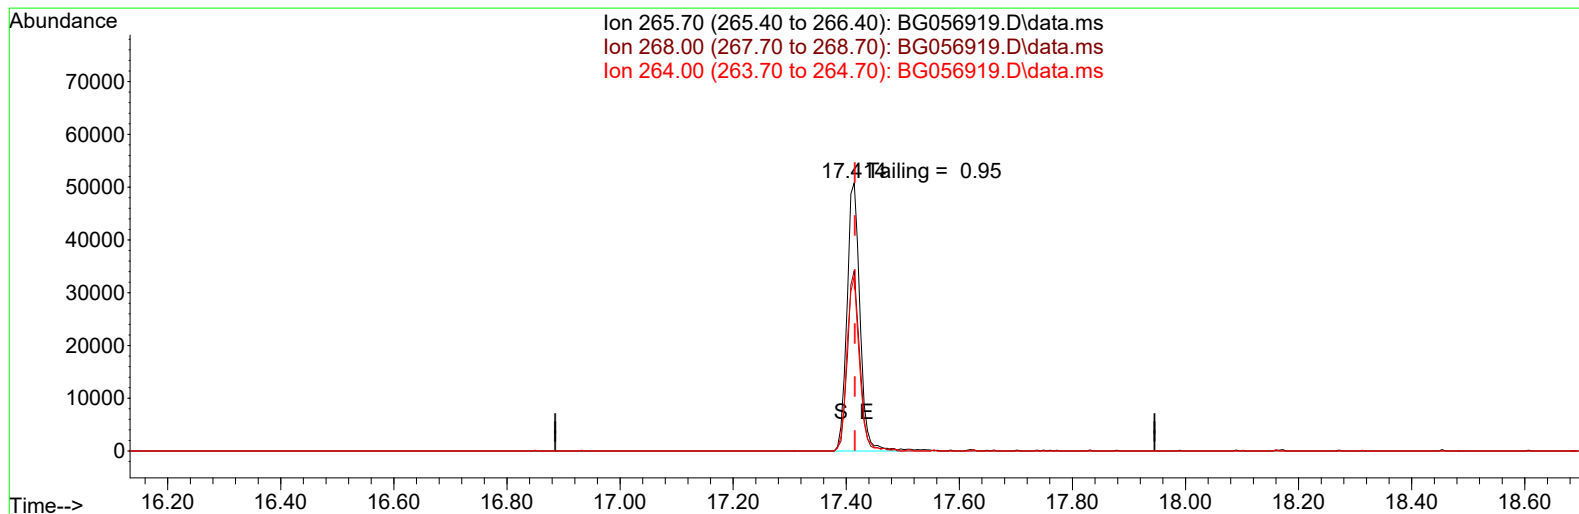

TIC: BG056919.D\data.ms

(70) Pentachlorophenol (C)

17.414min (-0.002) 19773.86 ng




response 80694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	67.12
264.00	58.50	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033023\
Data File : BG056919.D
Acq On : 30 Mar 2023 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 04:59:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

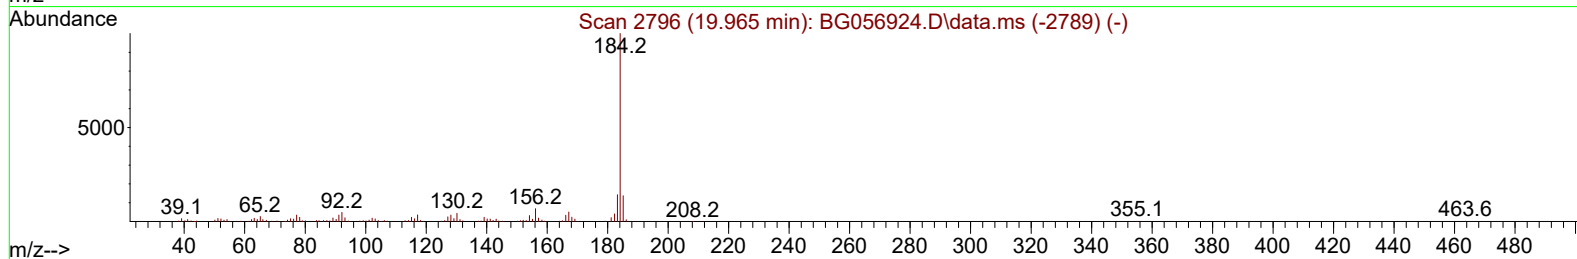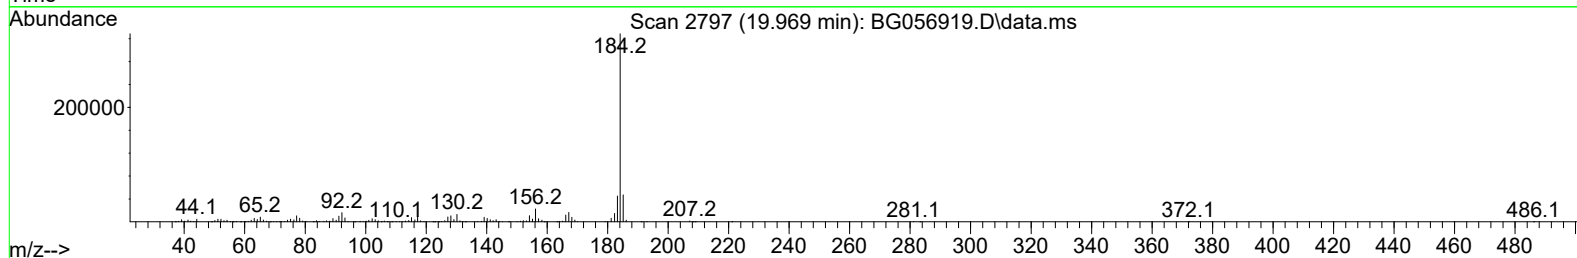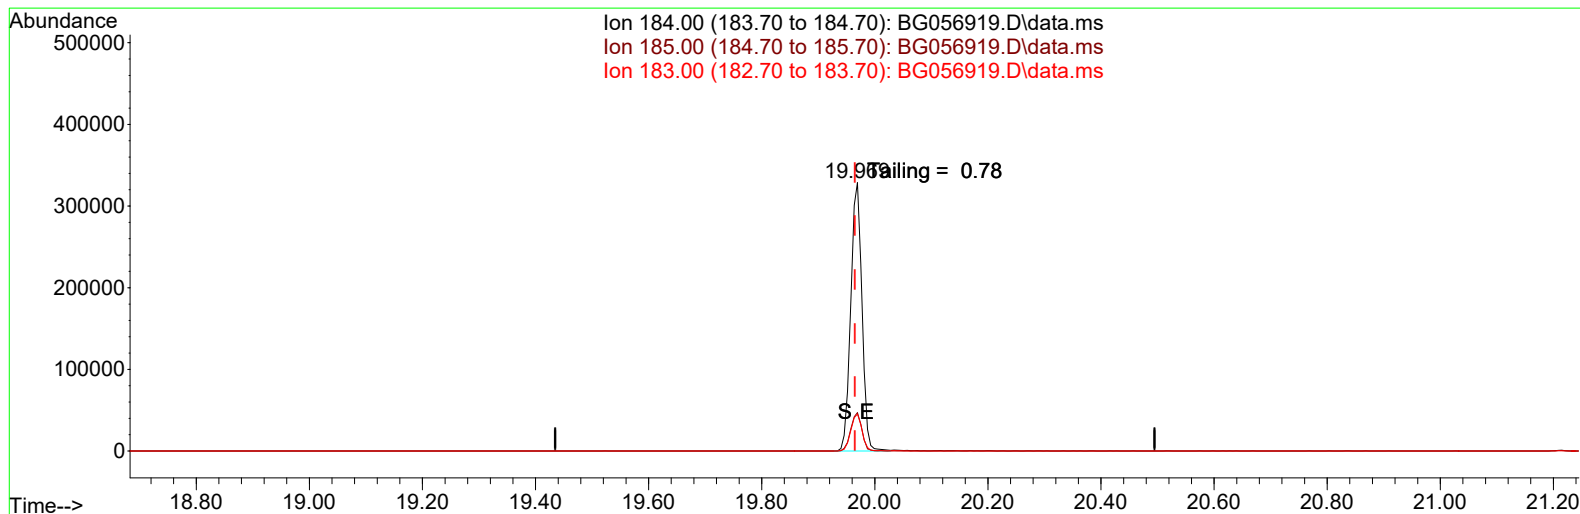

TIC: BG056919.D\data.ms

(77) Benzidine

19.969min (+ 0.004) 262447.26 ng

response 451933

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.33
183.00	14.20	13.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2023	BNA_G	<u>BG056919.D</u>
Compound Name	Response	Retention Time
DDT	209172	21.215
DDD	1828	20.804
DDE	0	20.47
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1828	211000	0.87

Instrument :
BNA_G
ClientSampleId :
DFTPP