

Data Path : Z:\HPCHEM1\BNA G\DATA\BG033117\
 Data File : BG026533.D
 Acq On : 1 Apr 2017 1:47
 Operator : SJ/MA
 Sample : I2464-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Apr 01 04:34:32 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 01 01:49:21 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	191731	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	803160	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.65	164	472976	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.38	188	1136337	20.00	ng/ul	0.00
77) Chrysene-d12	21.63	240	1323805	20.00	ng/ul	0.00
85) Perylene-d12	24.81	264	1312749	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.47	96	21678	5.41	ng/uL	0.00
5) Phenol-d5	7.20	99	92532	6.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	238696	30.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	311911	24.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	184304	16.20	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	182352	31.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	219548	32.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	344142	27.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	27246	2.22	ng/ul	0.01
43) Dimethylphthalate-d6	14.05	166	1189456	32.48	ng/ul	0.00
46) Acenaphthylene-d8	14.34	160	1419129	31.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	30992	4.35	ng/ul	0.01
57) Fluorene-d10	15.64	176	1107378	33.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.75	200	217846	29.81	ng/ul	0.00
70) Anthracene-d10	17.48	188	1742323	33.76	ng/ul	0.00
78) Pyrene-d10	19.75	212	2019044	34.19	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.59	264	2023119	35.87	ng/ul	0.00


Target Compounds					Ovalue
2) 1,4-Dioxane	3.51	88	5107	1.19 ng/uL#	36


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG033117\
Data File : BG026533.D
Acq On : 1 Apr 2017 1:47
Operator : SJ/MA
Sample : I2464-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Apr 01 04:34:32 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG032717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 01 01:49:21 2017
Response via : Initial Calibration

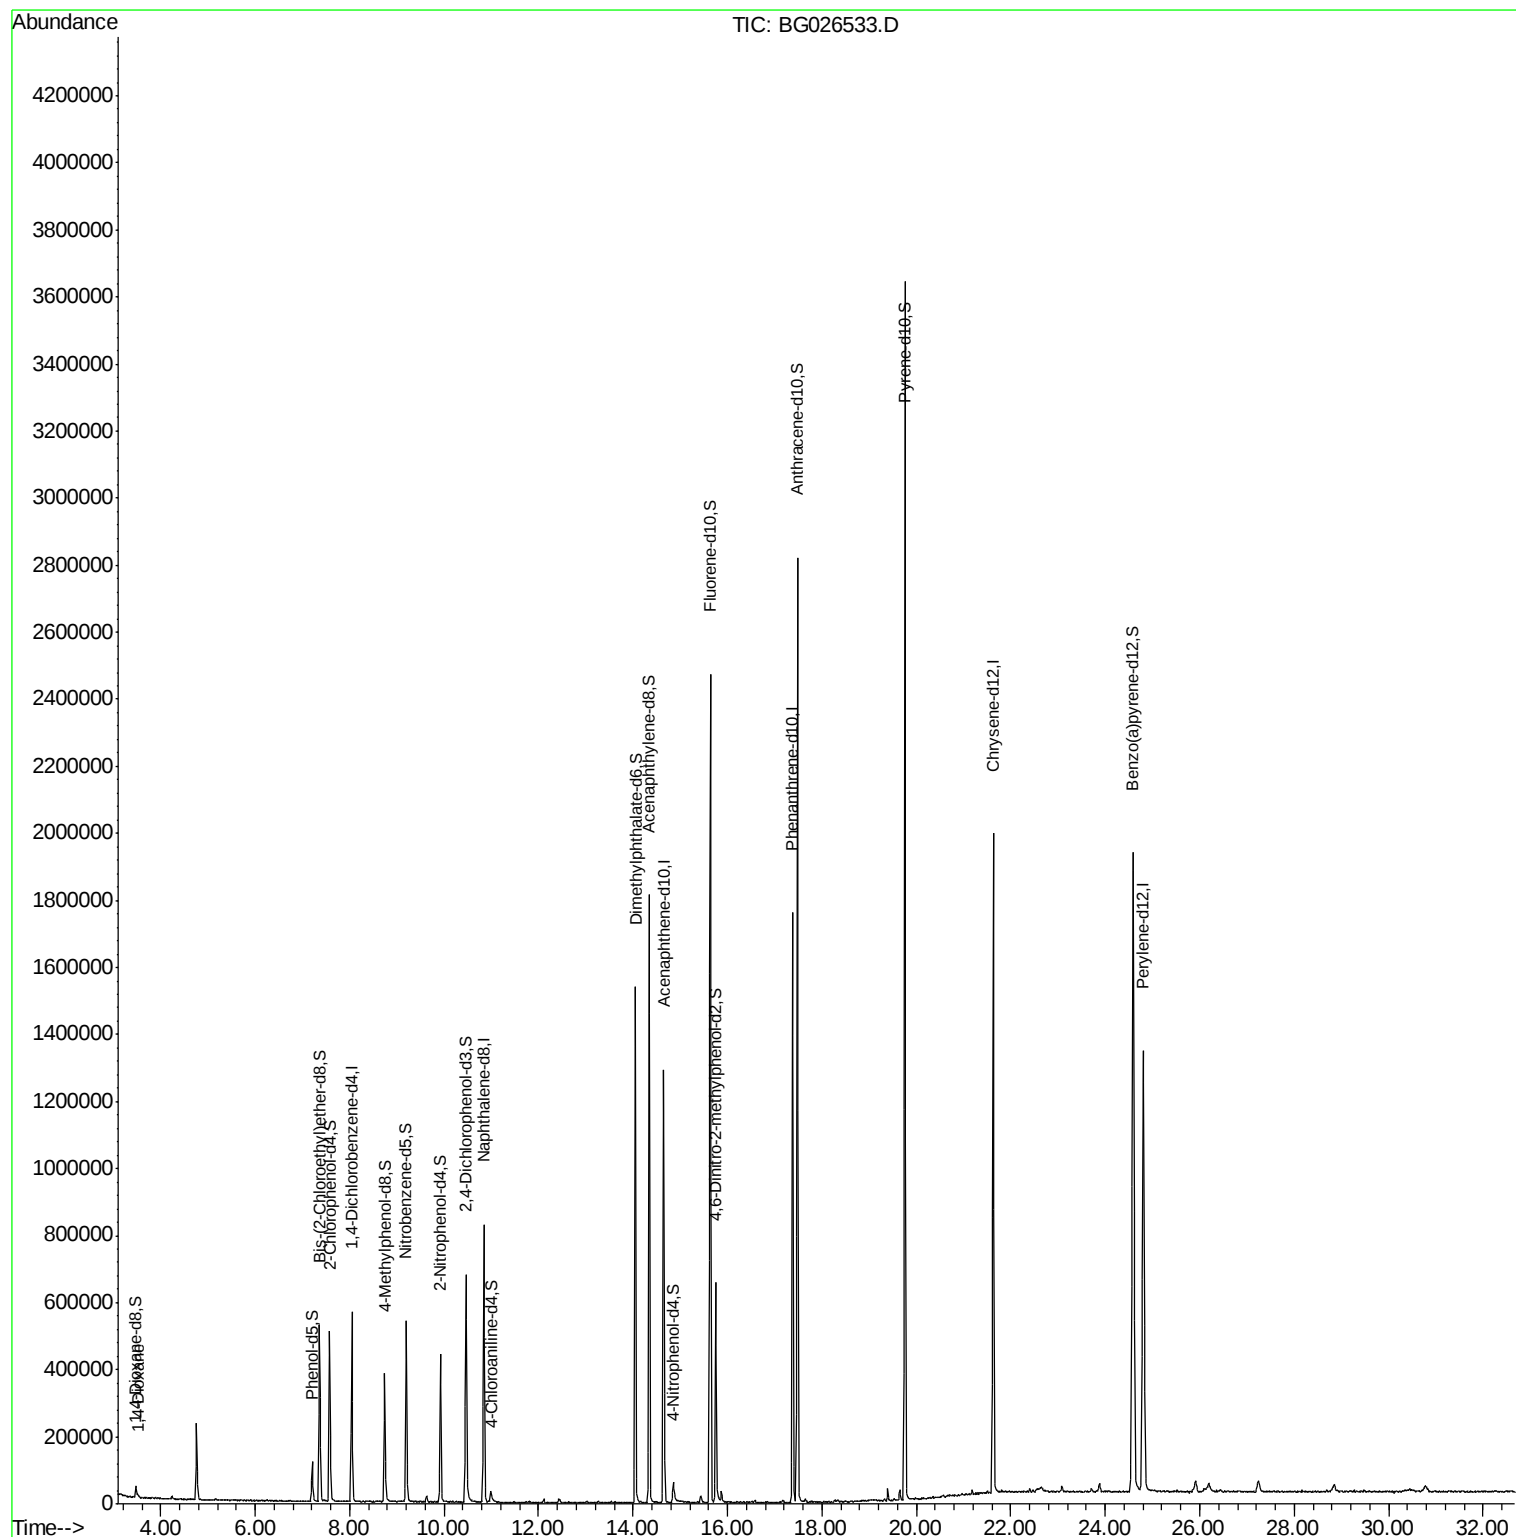

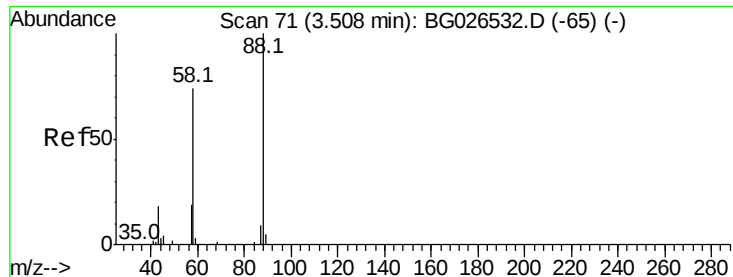

#2

1,4-Dioxane

Concen: 1.19 ng/uL

RT: 3.51 min Scan# 71

Delta R.T. 0.00 min


Lab File: BG026533.D

Acq: 1 Apr 2017 1:47

Instrument :

BNA_G

ClientSampleId :

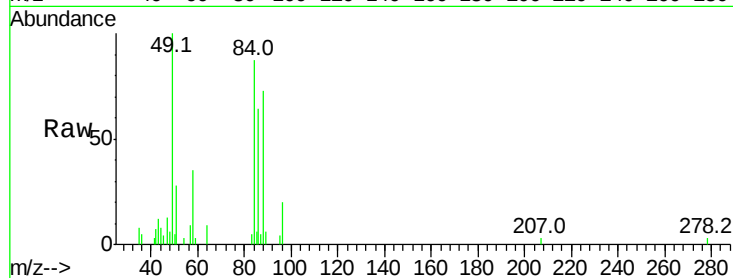

Tot Ion:	88	Resp:	5107
Ion	Ratio	Lower	Upper
88	100		
43	12.0	21.0	31.6#
58	0.0	47.8	71.8#

