
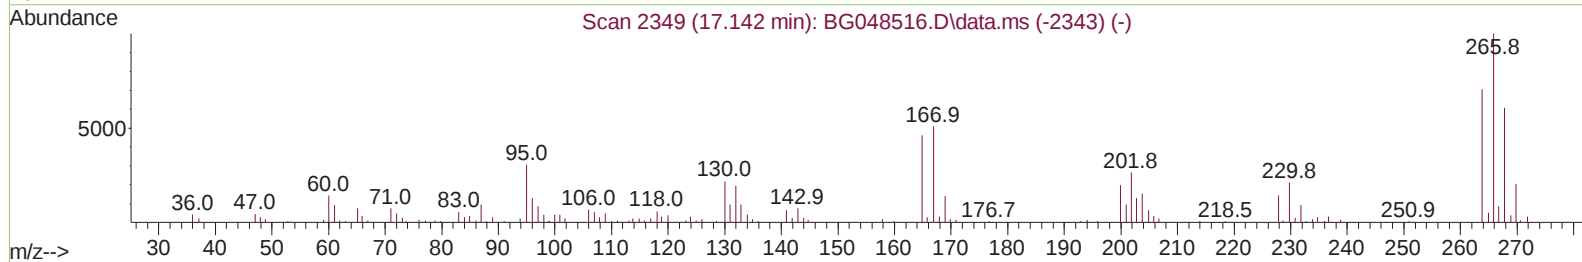
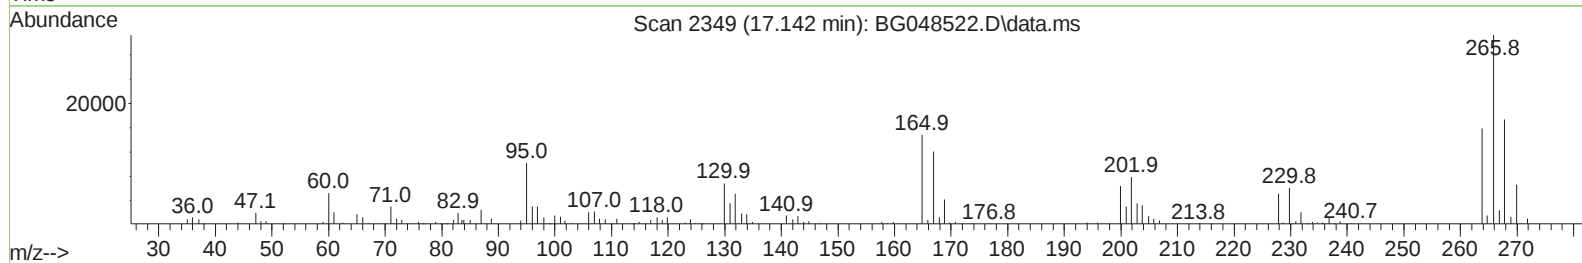


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048522.D
Acq On : 31 Mar 2021 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 11:47:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 11:41:32 2021
Response via : Initial Calibration

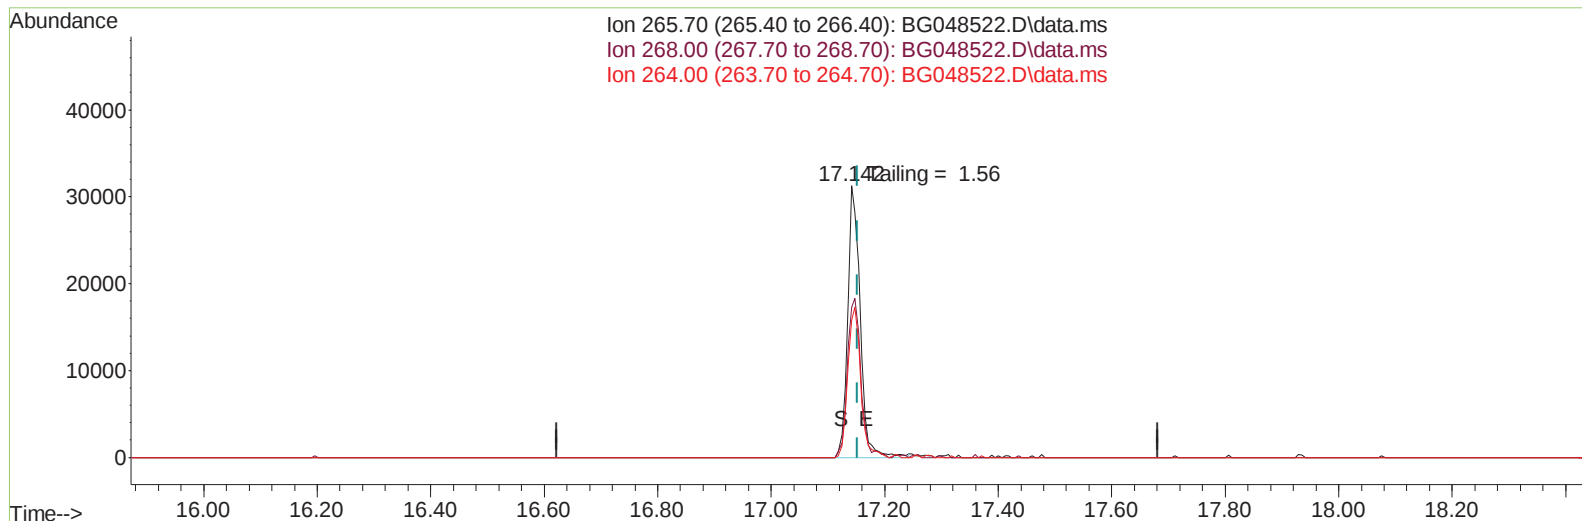

TIC: BG048522.D\data.ms

(70) Pentachlorophenol (C)




17.142min (-0.010) 74652.25 ng

response 47262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	55.35
264.00	70.50	55.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048522.D
Acq On : 31 Mar 2021 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 11:47:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 11:41:32 2021
Response via : Initial Calibration

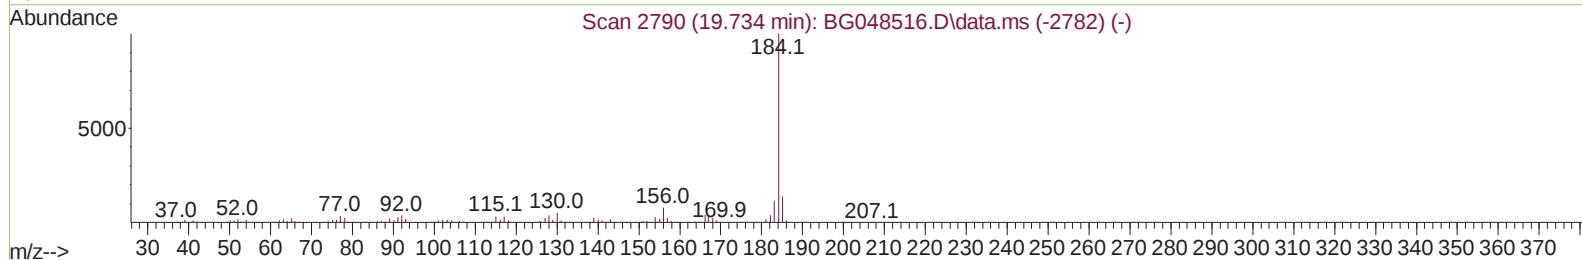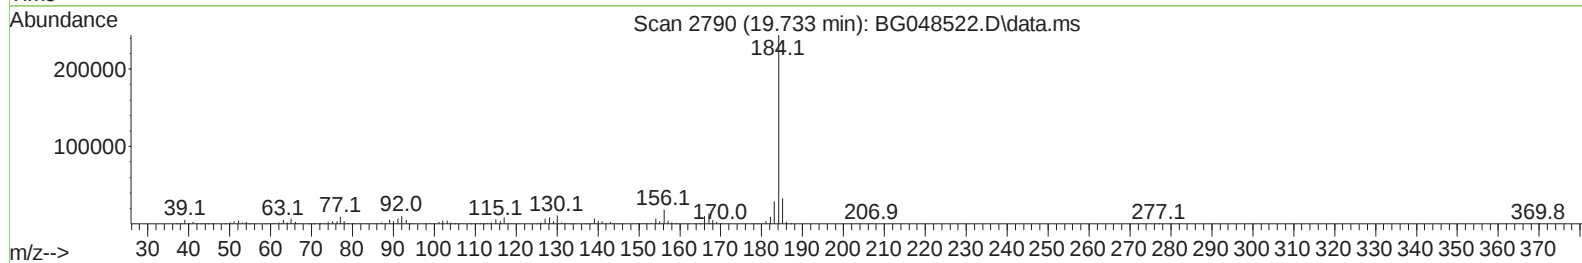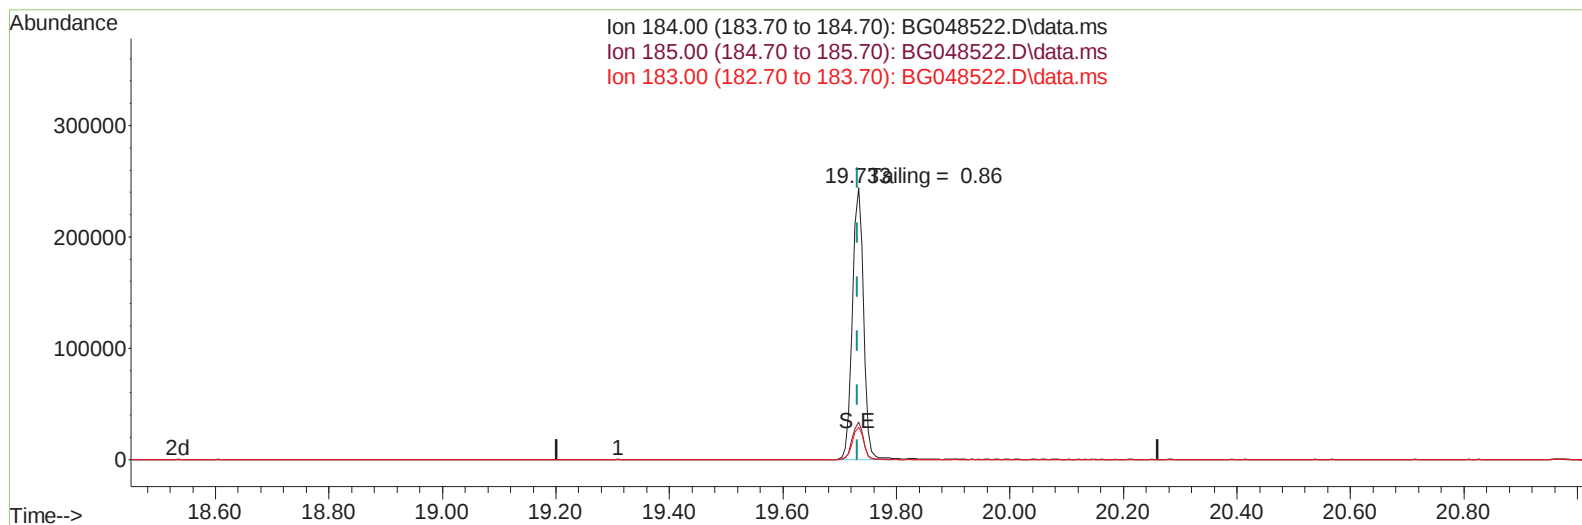

TIC: BG048522.D\data.ms

(77) Benzidine**19.733min (+ 0.002) 3827.09 ng m****response 331638**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.78
183.00	11.50	11.87
0.00	0.00	0.00