

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG033121\  
 Data File : BG048524.D  
 Acq On : 31 Mar 2021 10:49  
 Operator : CG/JU  
 Sample : PB135064BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB135064BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048524.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.640       | 383           | 392         | 401          | rBV      | 379739         | 581728        | 30.71%          | 8.396%        |
| 2         | 7.244       | 657           | 665         | 674          | rBV      | 372494         | 632005        | 33.36%          | 9.122%        |
| 3         | 8.096       | 803           | 810         | 816          | rBV      | 76787          | 121344        | 6.41%           | 1.751%        |
| 4         | 9.266       | 1001          | 1009        | 1018         | rVB      | 237985         | 410209        | 21.65%          | 5.921%        |
| 5         | 10.923      | 1284          | 1291        | 1299         | rBB      | 101156         | 172560        | 9.11%           | 2.491%        |
| 6         | 13.367      | 1699          | 1707        | 1714         | rBV      | 632346         | 955034        | 50.41%          | 13.784%       |
| 7         | 14.747      | 1934          | 1942        | 1949         | rBV2     | 153228         | 235943        | 12.45%          | 3.405%        |
| 8         | 16.234      | 2189          | 2195        | 2207         | rBV      | 526546         | 790482        | 41.73%          | 11.409%       |
| 9         | 17.503      | 2402          | 2411        | 2418         | rBV      | 226351         | 334980        | 17.68%          | 4.835%        |
| 10        | 20.112      | 2849          | 2855        | 2861         | rBV      | 1536786        | 1894478       | 100.00%         | 27.343%       |
| 11        | 21.798      | 3135          | 3142        | 3151         | rVB      | 250494         | 399684        | 21.10%          | 5.769%        |
| 12        | 25.141      | 3698          | 3711        | 3725         | rBV2     | 137395         | 400008        | 21.11%          | 5.773%        |




Sum of corrected areas: 6928455

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG033121\  
Data File : BG048524.D  
Acq On : 31 Mar 2021 10:49  
Operator : CG/JU  
Sample : PB135064BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135064BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

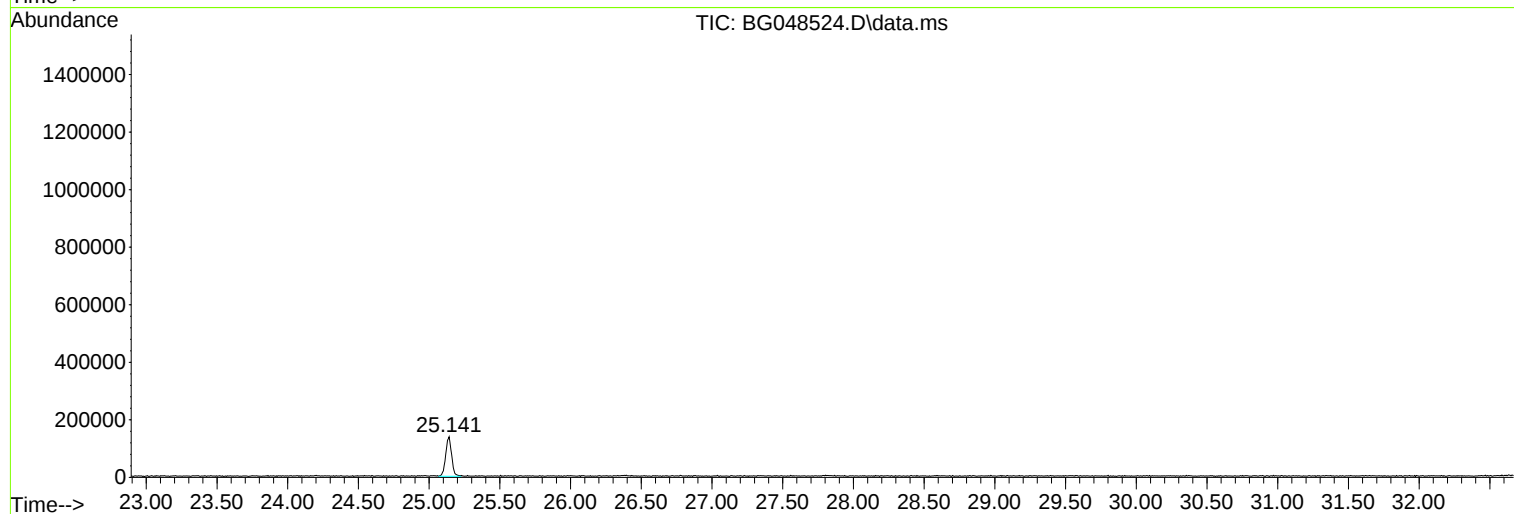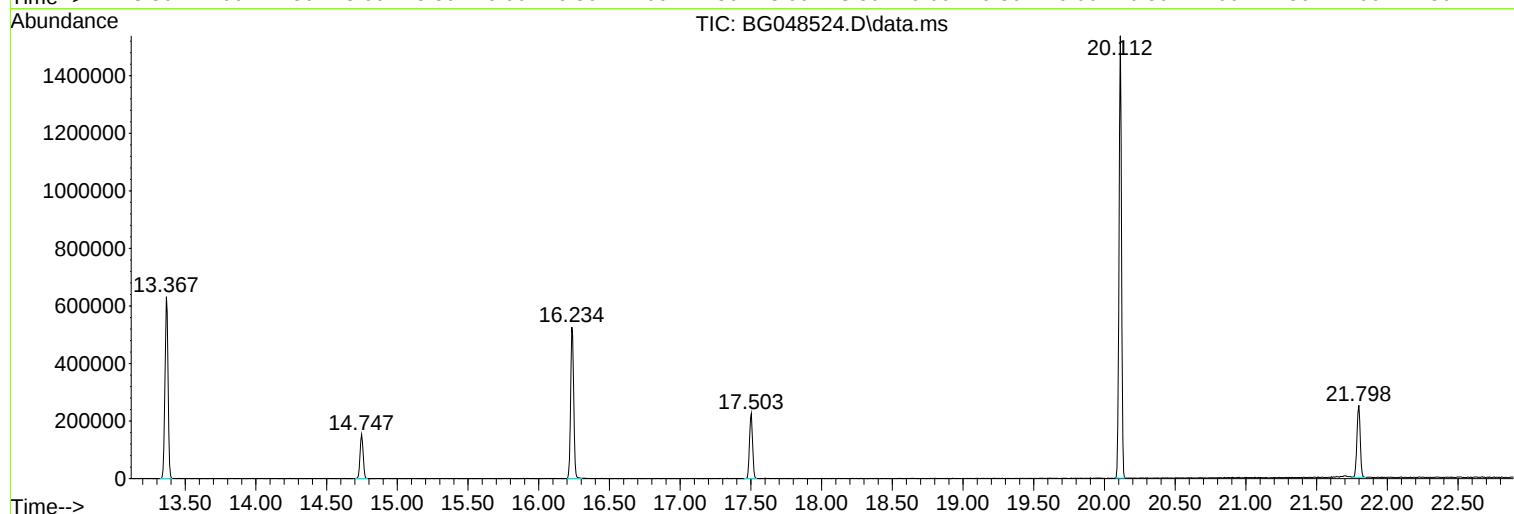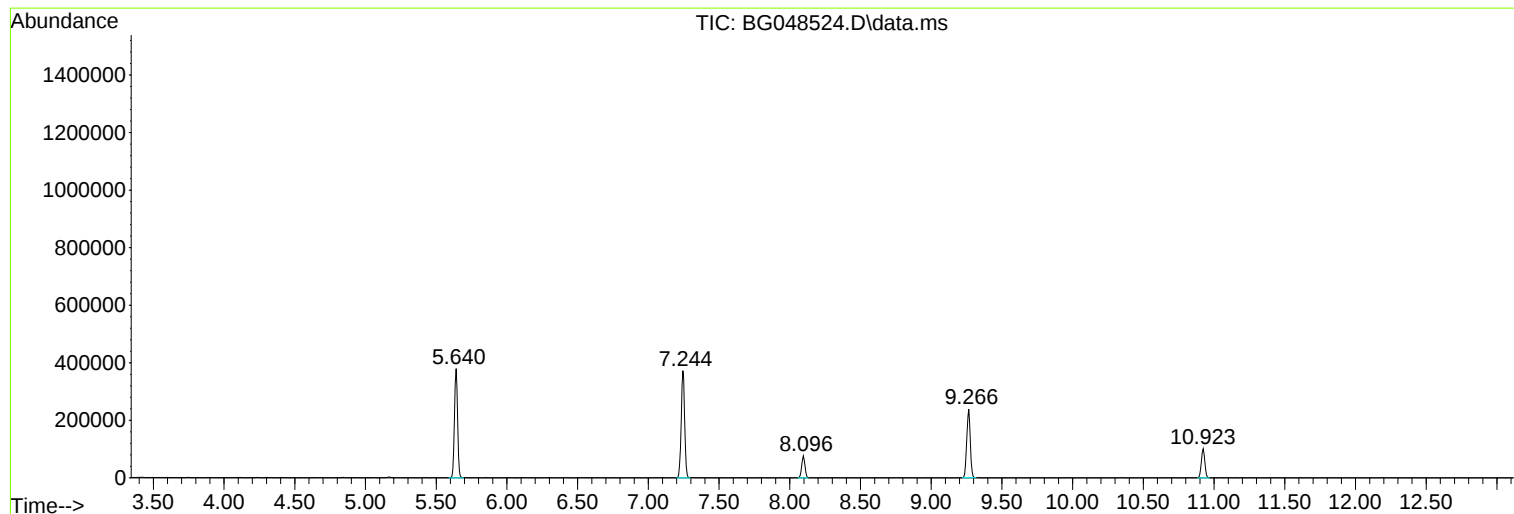

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG033121\  
Data File : BG048524.D  
Acq On : 31 Mar 2021 10:49  
Operator : CG/JU  
Sample : PB135064BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135064BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG033121\  
Data File : BG048524.D  
Acq On : 31 Mar 2021 10:49  
Operator : CG/JU  
Sample : PB135064BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB135064BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG033021.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|