

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
 Data File : BG048525.D
 Acq On : 31 Mar 2021 11:31
 Operator : CG/JU
 Sample : PB135047BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB135047BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.643	386	392	398	rBV	344129	534248	28.77%	8.165%
2	7.247	658	665	673	rBV	357215	574208	30.92%	8.776%
3	8.099	801	810	818	rBB2	67593	112607	6.06%	1.721%
4	9.268	1000	1009	1019	rBV	225366	381119	20.52%	5.825%
5	10.925	1283	1291	1298	rBB	87924	155799	8.39%	2.381%
6	13.369	1700	1707	1717	rVB	592051	883782	47.59%	13.507%
7	14.750	1935	1942	1950	rVB	147719	226110	12.18%	3.456%
8	16.236	2188	2195	2204	rBV	513322	748338	40.30%	11.437%
9	17.499	2404	2410	2417	rBV	205781	309694	16.68%	4.733%
10	20.114	2847	2855	2860	rBV	1474262	1857034	100.00%	28.382%
11	21.800	3134	3142	3149	rBV2	232560	383970	20.68%	5.868%
12	25.143	3701	3711	3726	rVB2	130079	376182	20.26%	5.749%




Sum of corrected areas: 6543091

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048525.D
Acq On : 31 Mar 2021 11:31
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135047BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

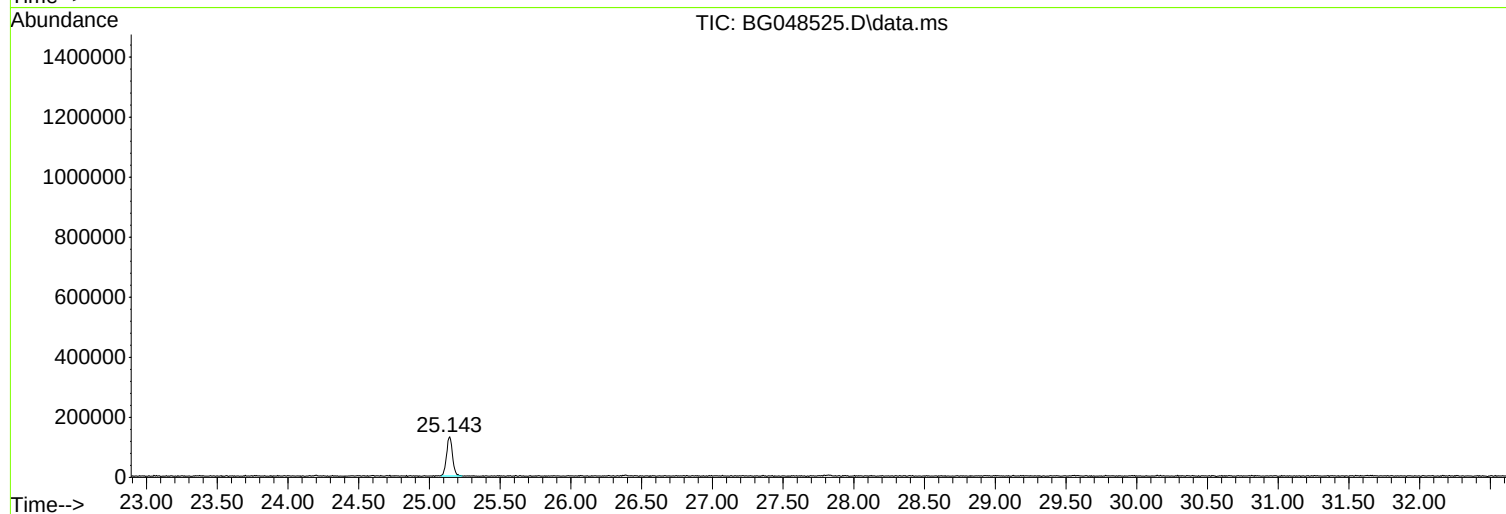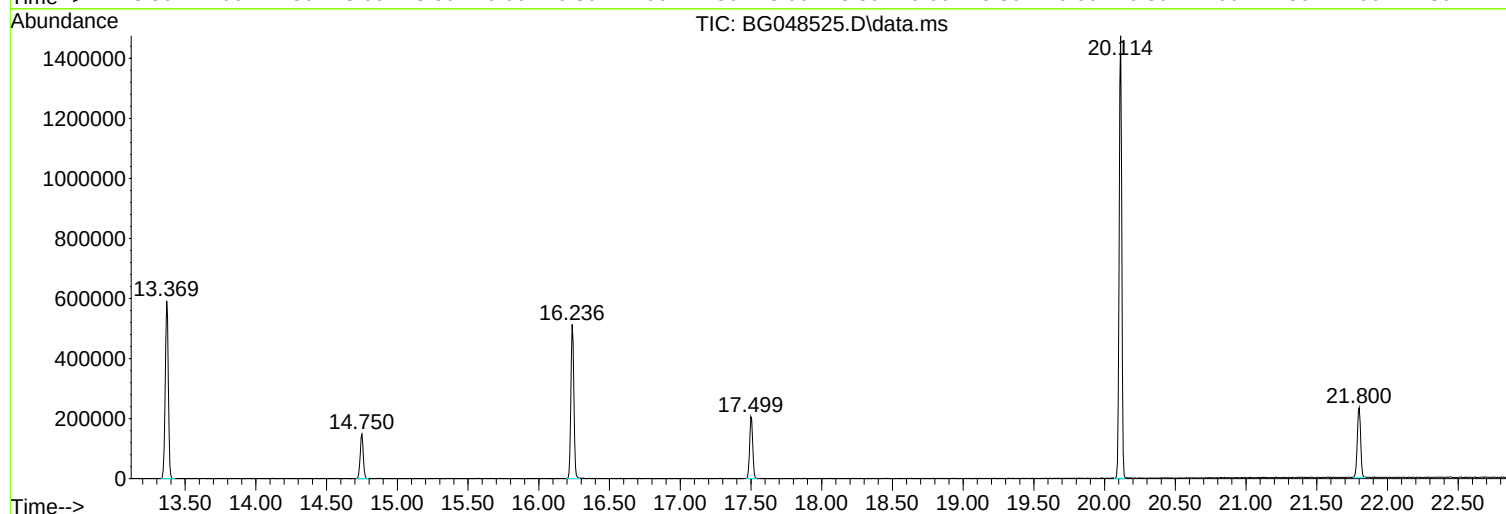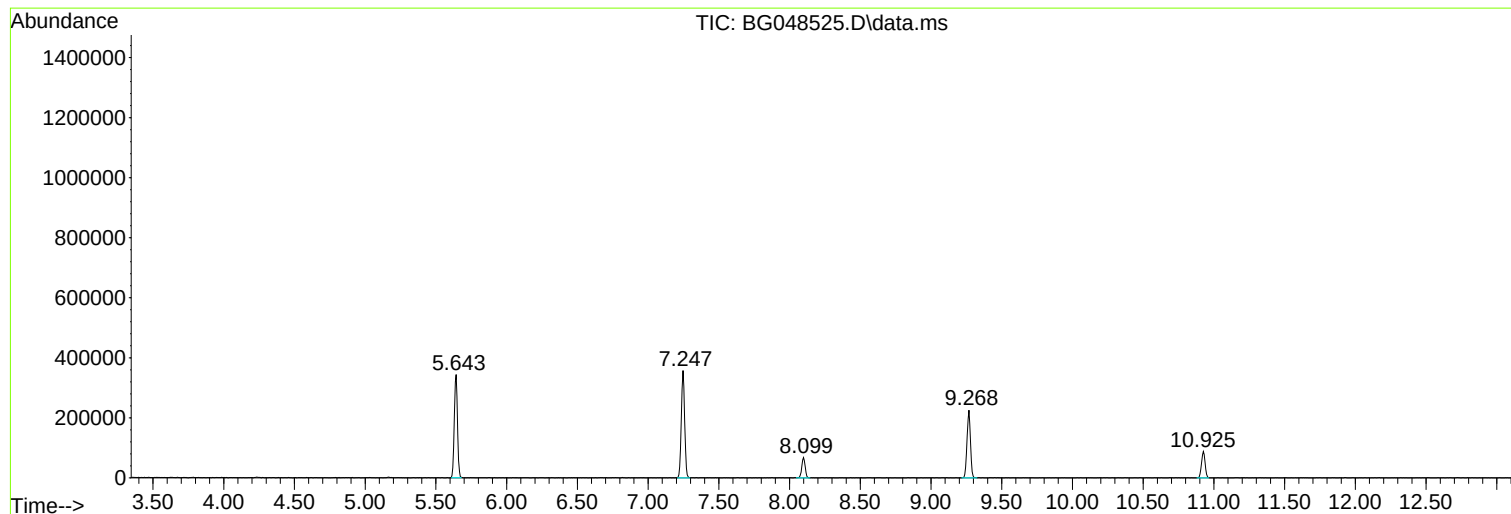

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048525.D
Acq On : 31 Mar 2021 11:31
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135047BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048525.D
Acq On : 31 Mar 2021 11:31
Operator : CG/JU
Sample : PB135047BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB135047BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------