
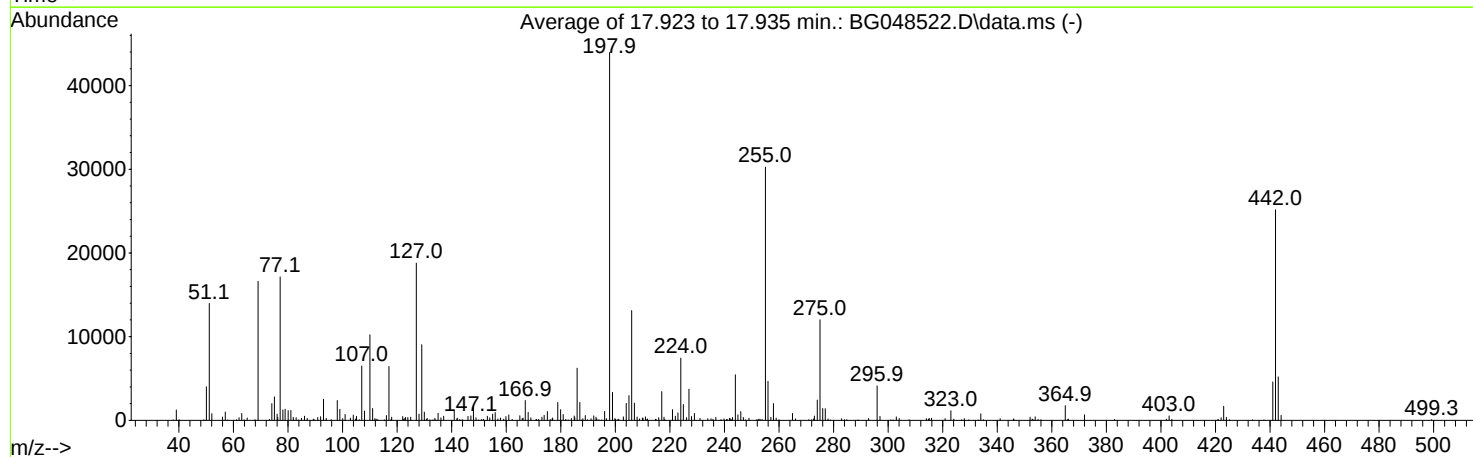


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
 Data File : BG048522.D
 Acq On : 31 Mar 2021 9:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 31 11:41:32 2021

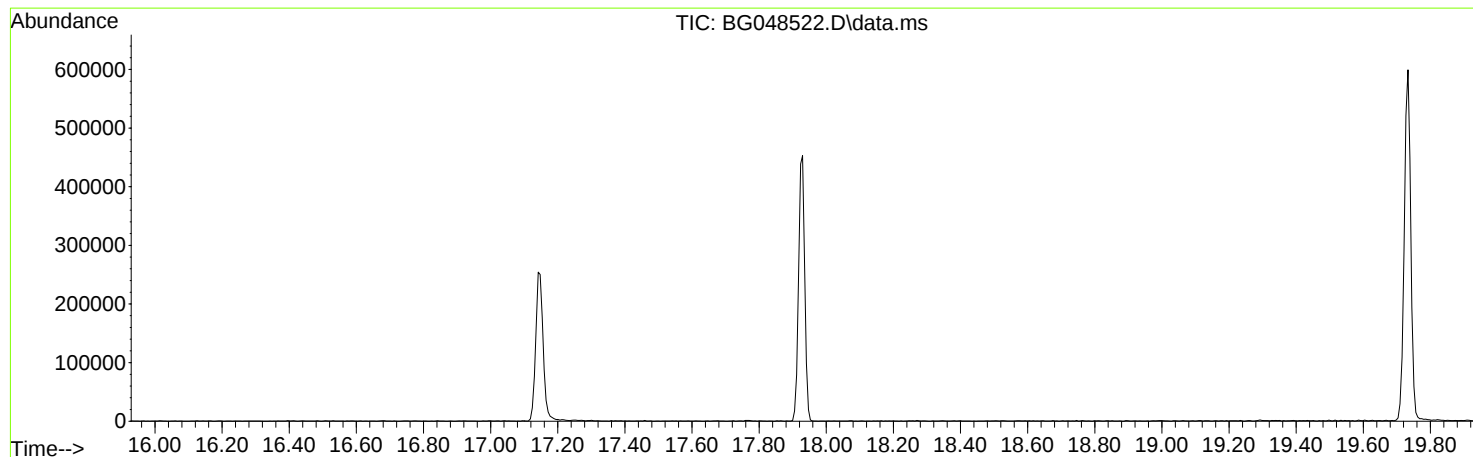

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	13970	PASS
68	69	0.00	2	0.5	75	PASS
69	198	0.00	100	37.8	16605	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.8	18795	PASS
197	198	0.00	2	0.5	217	PASS
198	198	100	100	100.0	43949	PASS
199	198	5	9	7.6	3343	PASS
275	198	10	60	27.4	12030	PASS
365	198	1	100	4.0	1766	PASS
441	198	0.01	100	10.4	4590	PASS
442	198	50	100	57.2	25160	PASS
443	442	15	24	20.7	5196	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/31/2021	BNA_G	<u>BG048522.D</u>
Compound Name	Response	Retention Time
DDT	162556	20.967
DDD	2673	20.52
DDE	316	20.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2989	165545	1.81

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048522.D
Acq On : 31 Mar 2021 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 11:47:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 11:41:32 2021
Response via : Initial Calibration

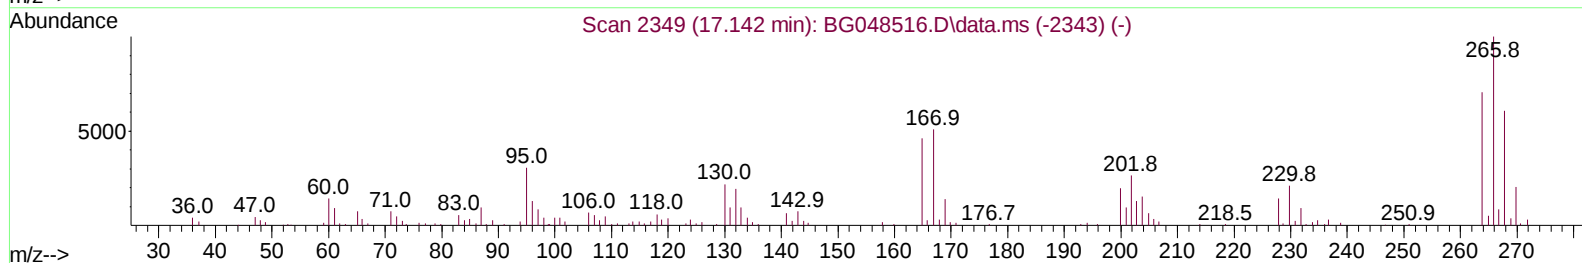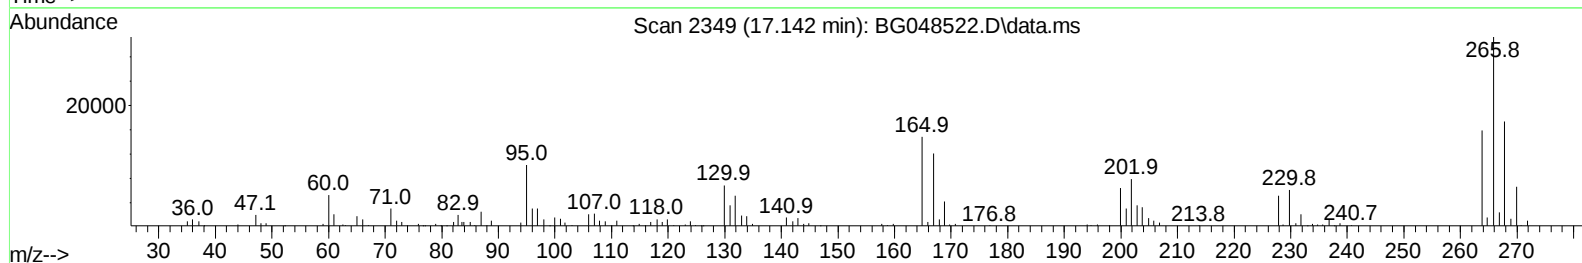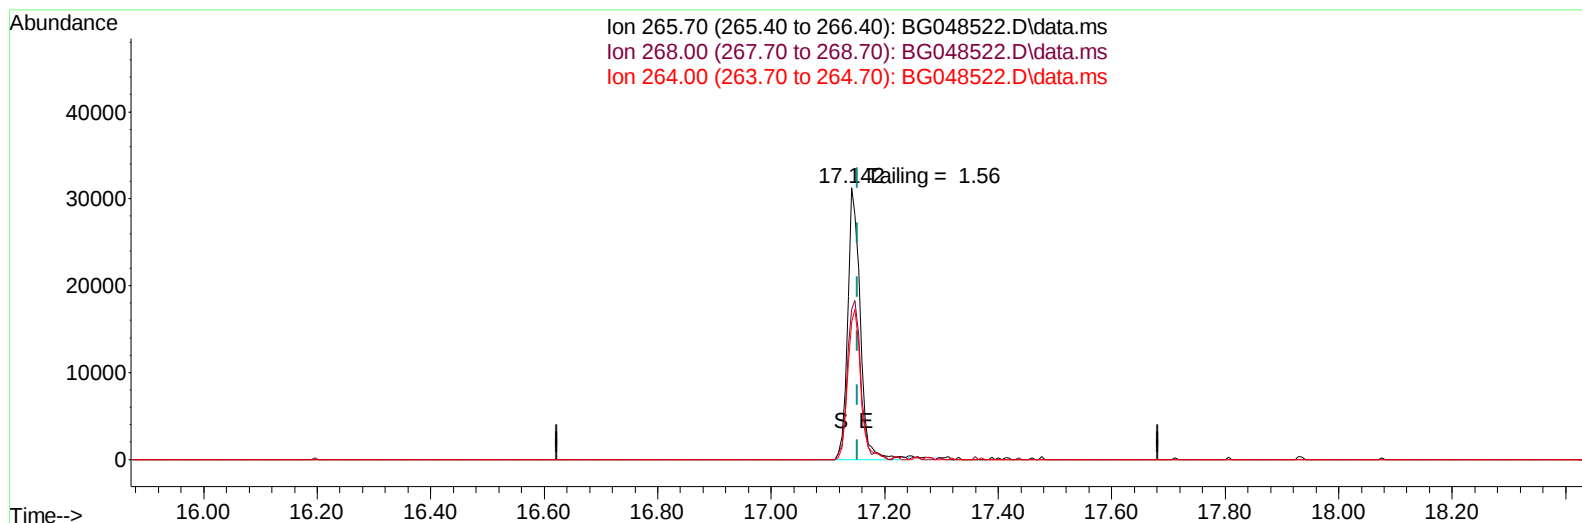

TIC: BG048522.D\data.ms

(70) Pentachlorophenol (C)

17.142min (-0.010) 74652.25 ng




response 47262

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.80	55.35
264.00	70.50	55.57#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033121\
Data File : BG048522.D
Acq On : 31 Mar 2021 9:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 31 11:47:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG033021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 31 11:41:32 2021
Response via : Initial Calibration

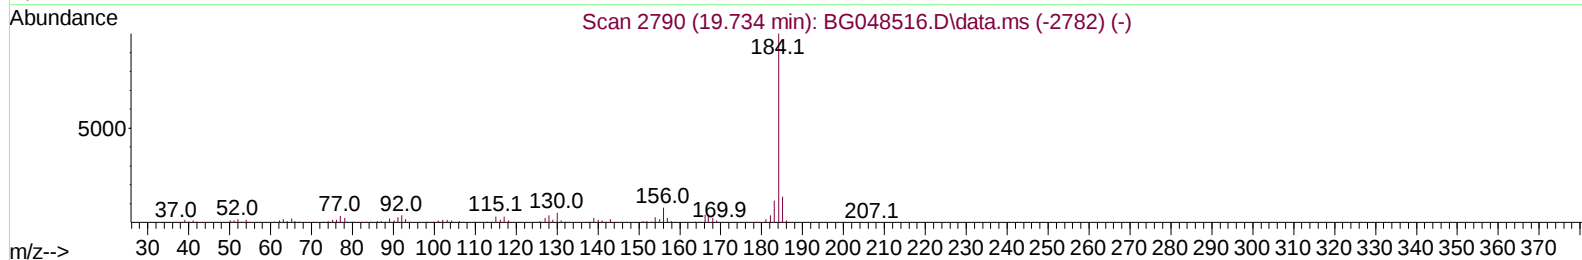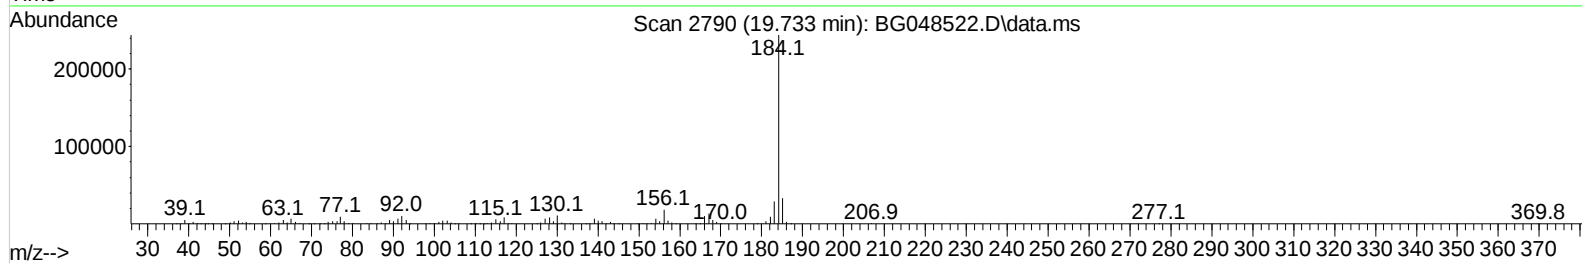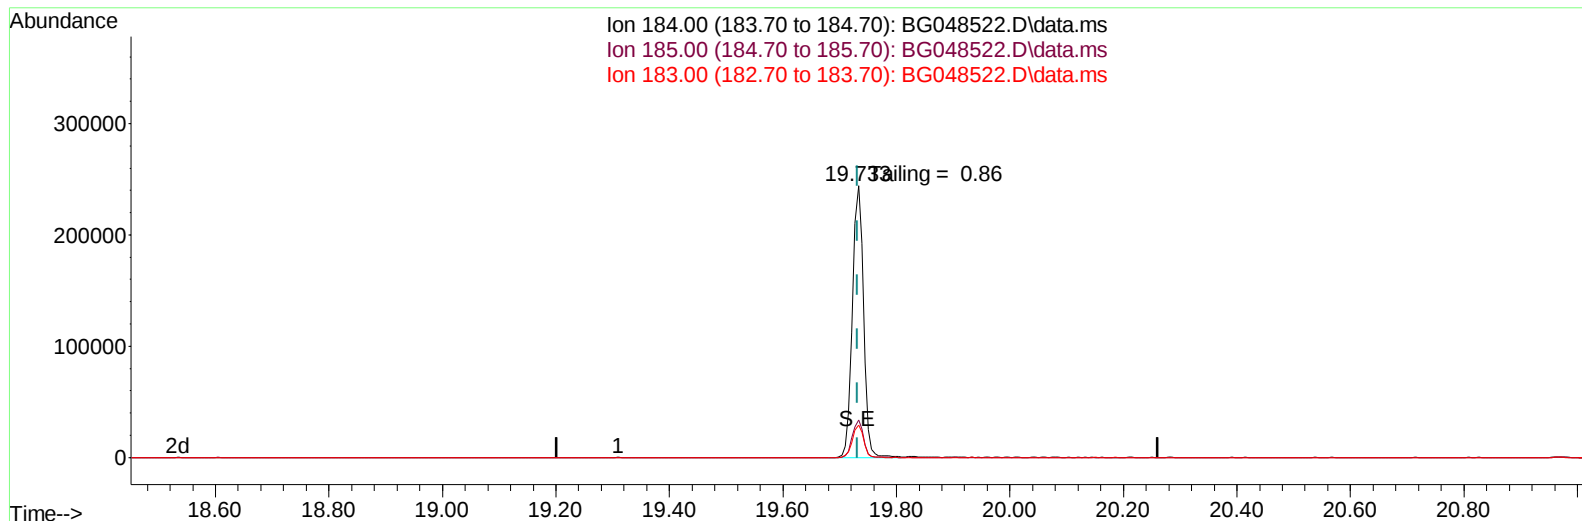

TIC: BG048522.D\data.ms

(77) Benzidine

19.733min (+ 0.002) 3827.09 ng m

response 331638

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.78
183.00	11.50	11.87
0.00	0.00	0.00