
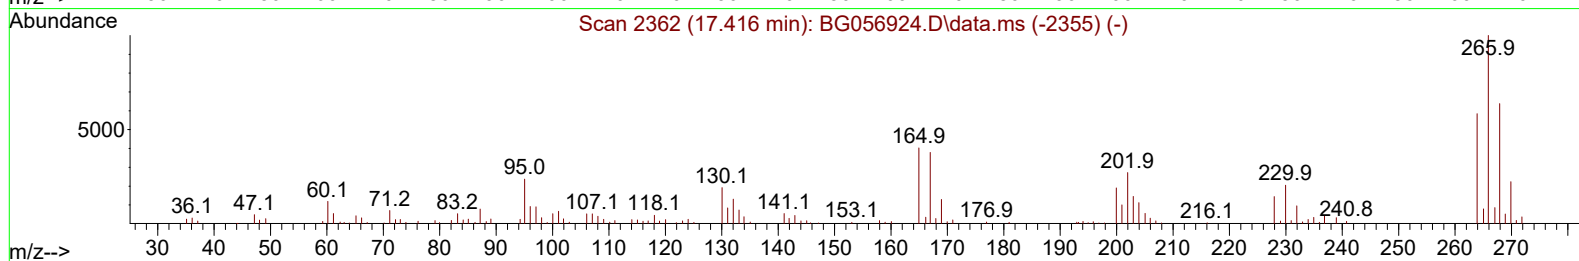
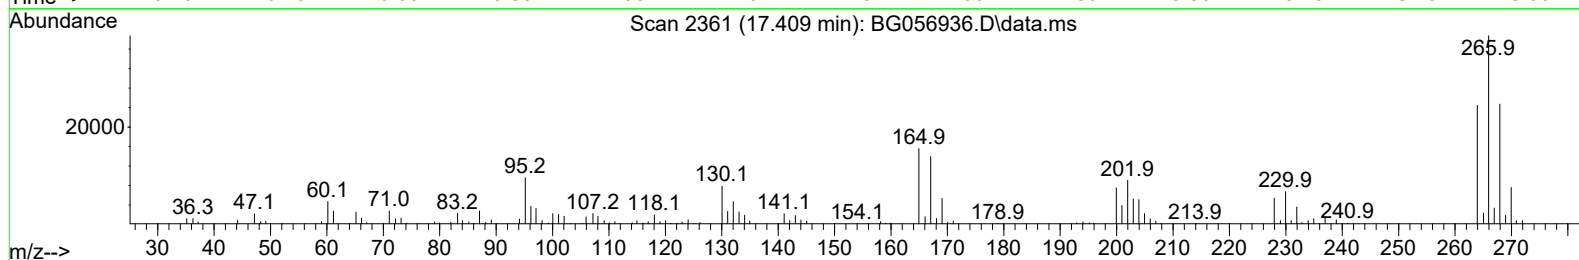


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033123\
Data File : BG056936.D
Acq On : 31 Mar 2023 7:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:35:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

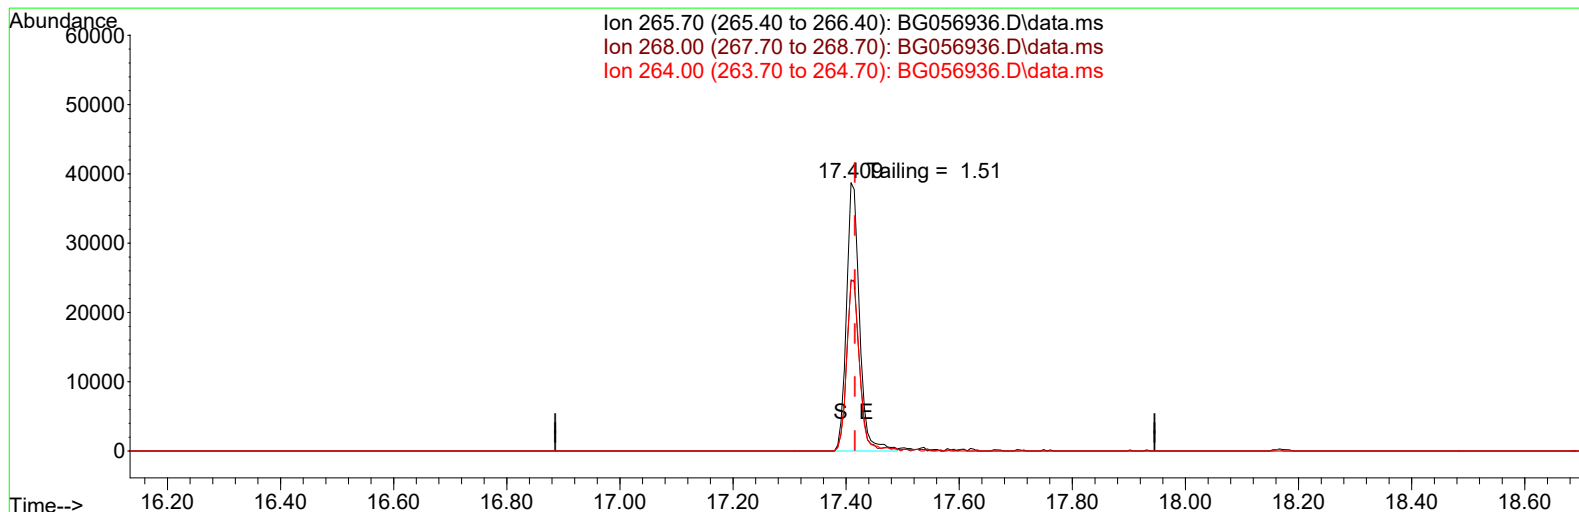

TIC: BG056936.D\data.ms

(70) Pentachlorophenol (C)




17.409min (-0.007) 99657.14 ng

response 62096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	58.50	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033123\
Data File : BG056936.D
Acq On : 31 Mar 2023 7:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 01 04:35:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

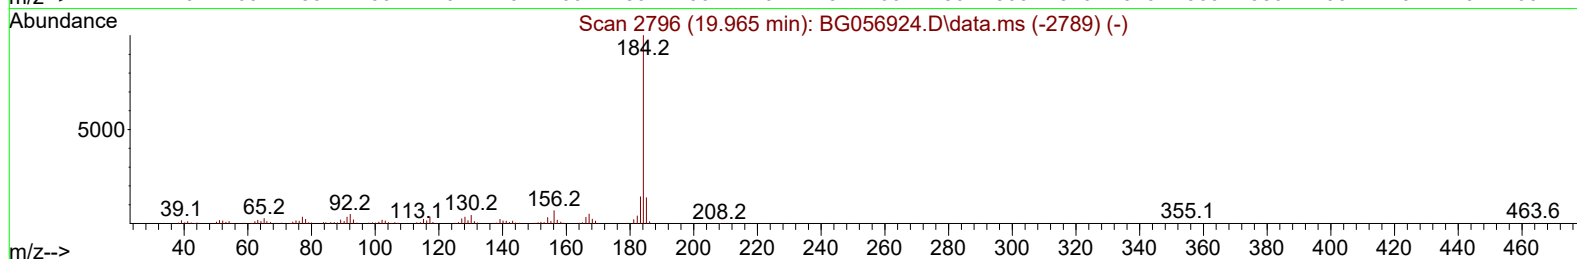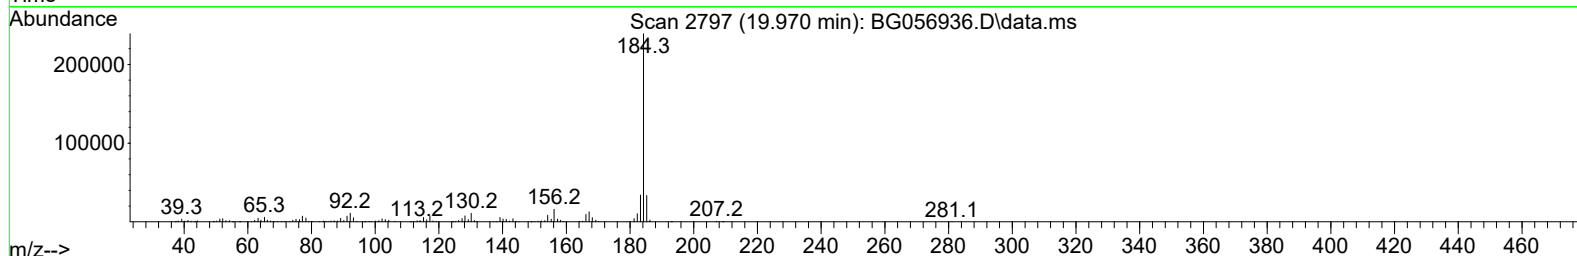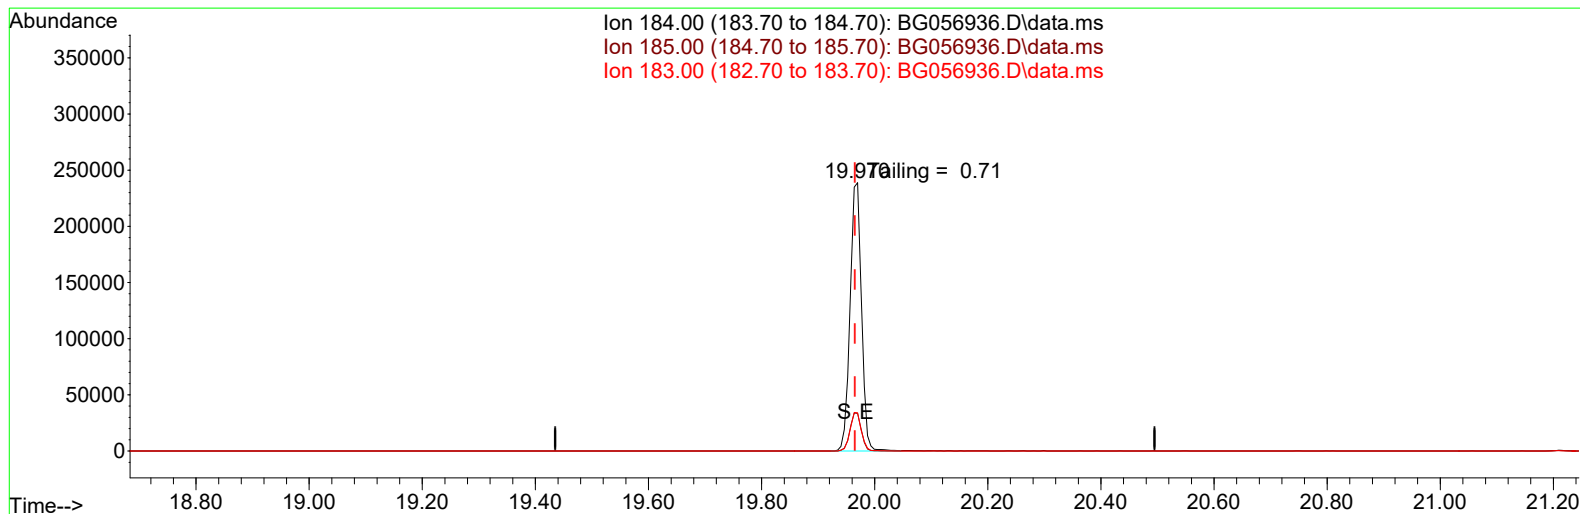

TIC: BG056936.D\data.ms

(77) Benzidine**19.970min (+ 0.005) 211089.28 ng****response 334646**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.04
183.00	14.20	14.27
0.00	0.00	0.00