


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033123\
Data File : BG056936.D
Acq On : 31 Mar 2023 7:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 31 03:23:11 2023

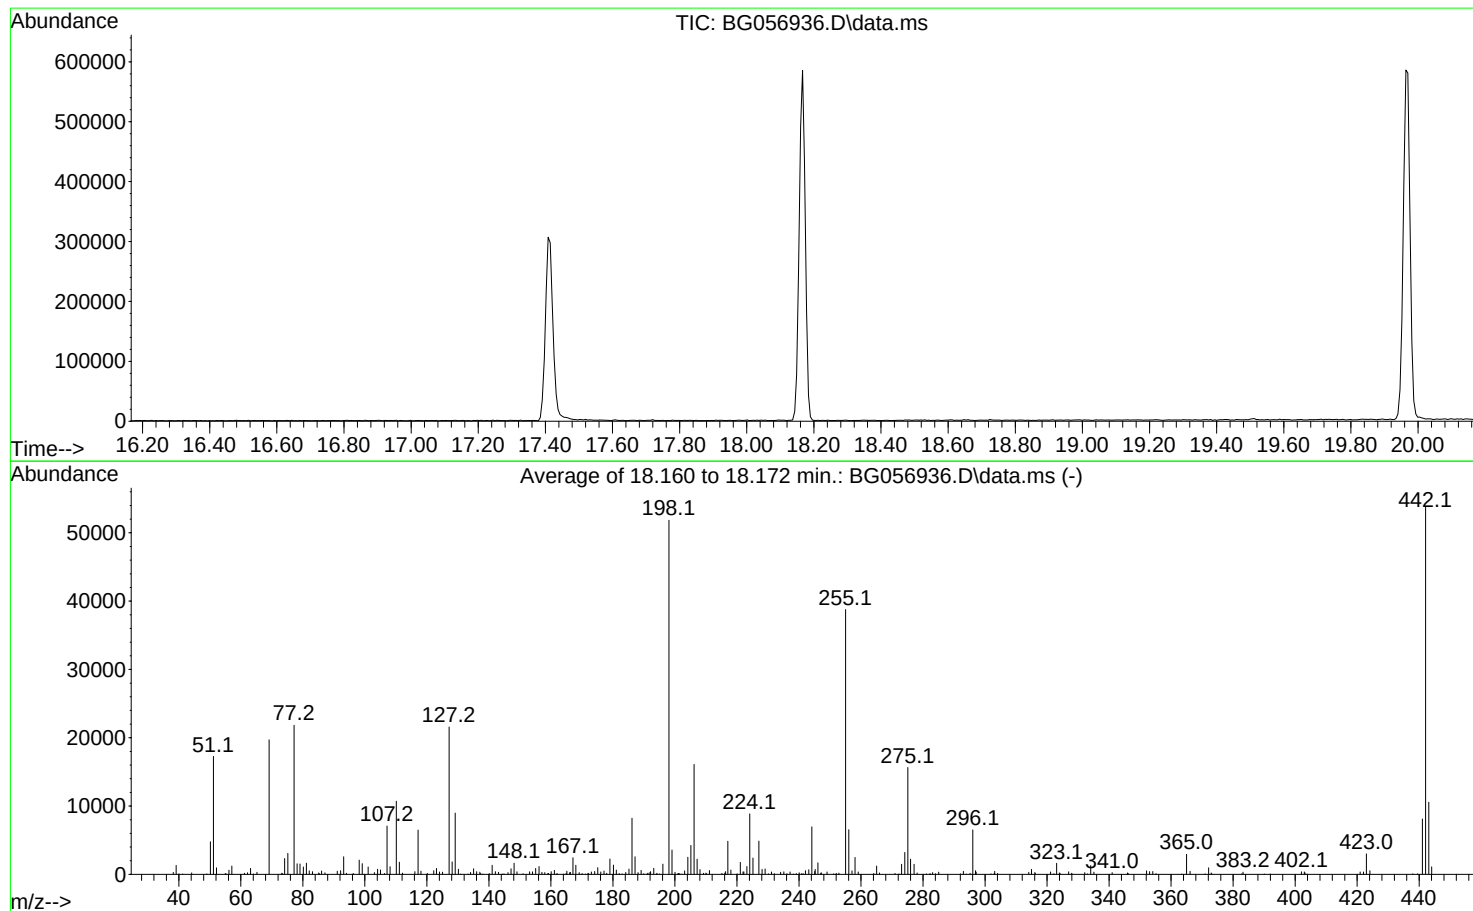




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	17260	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.0	19712	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.6	21584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51835	PASS
199	198	5	9	6.9	3562	PASS
275	198	10	60	30.2	15655	PASS
365	198	1	100	5.7	2937	PASS
441	198	0.01	100	15.6	8107	PASS
442	442	50	100	100.0	53853	PASS
443	442	15	24	19.6	10568	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033123\
Data File : BG056936.D
Acq On : 31 Mar 2023 7:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 01 04:35:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

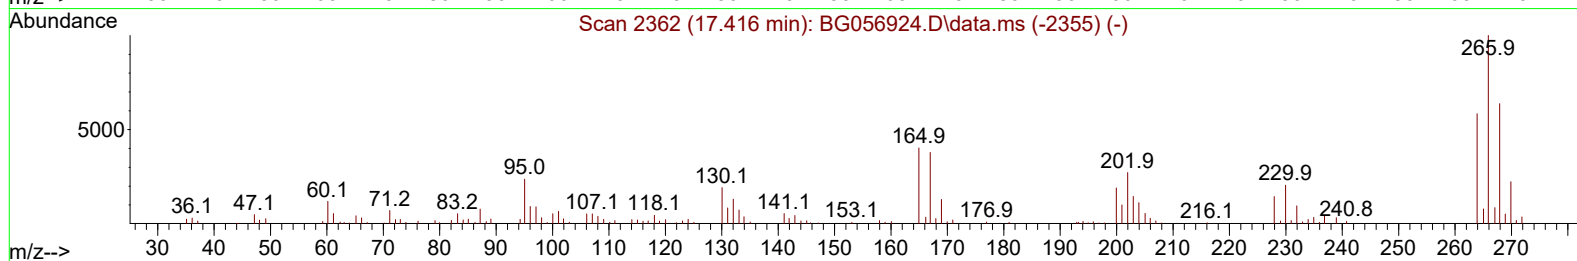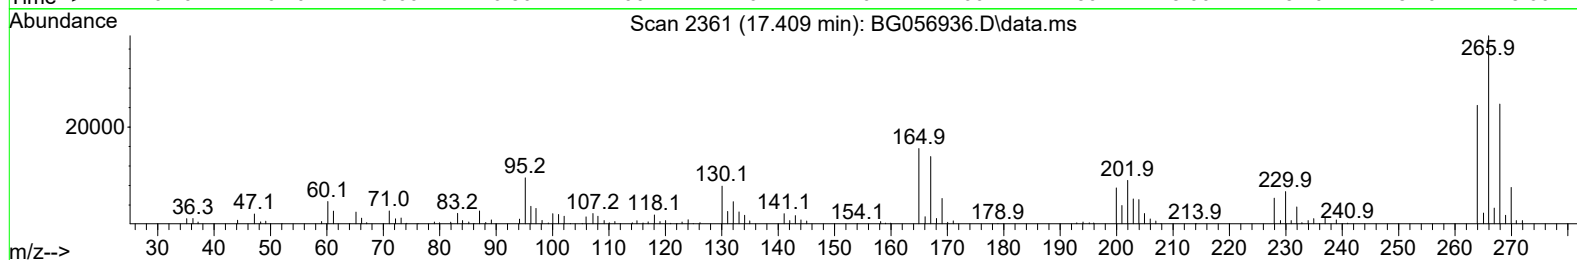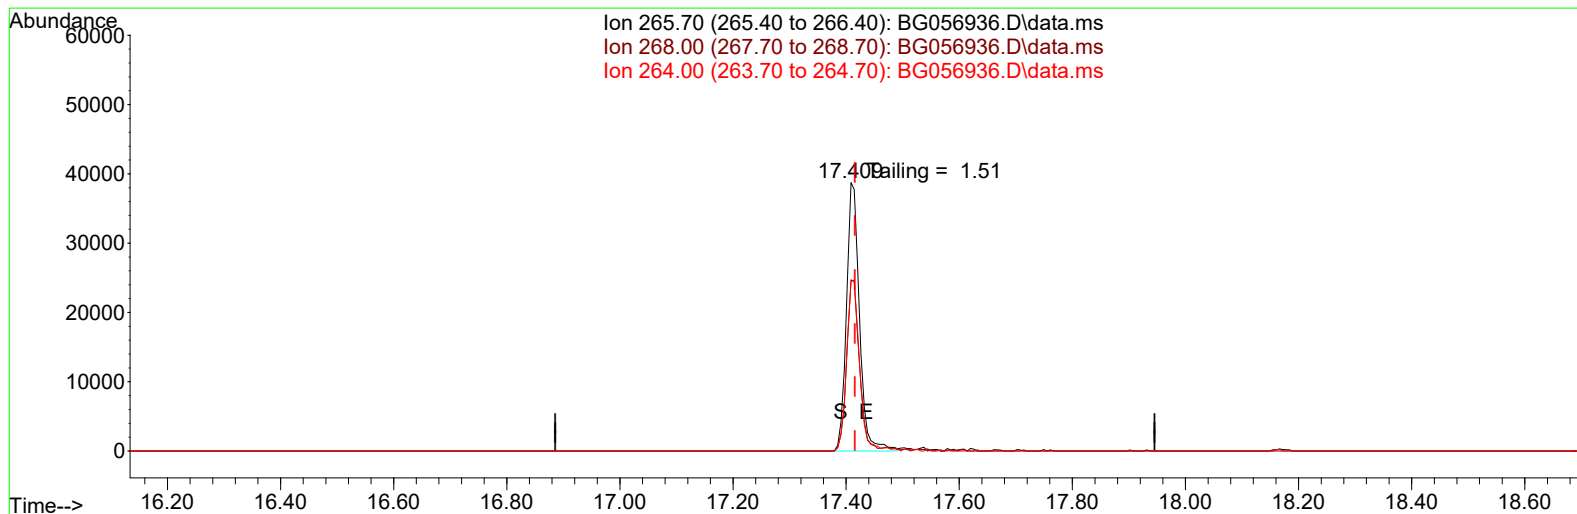

TIC: BG056936.D\data.ms

(70) Pentachlorophenol (C)

17.409min (-0.007) 99657.14 ng




response 62096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.80
264.00	58.50	63.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG033123\
Data File : BG056936.D
Acq On : 31 Mar 2023 7:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 01 04:35:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG033023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 03:23:11 2023
Response via : Initial Calibration

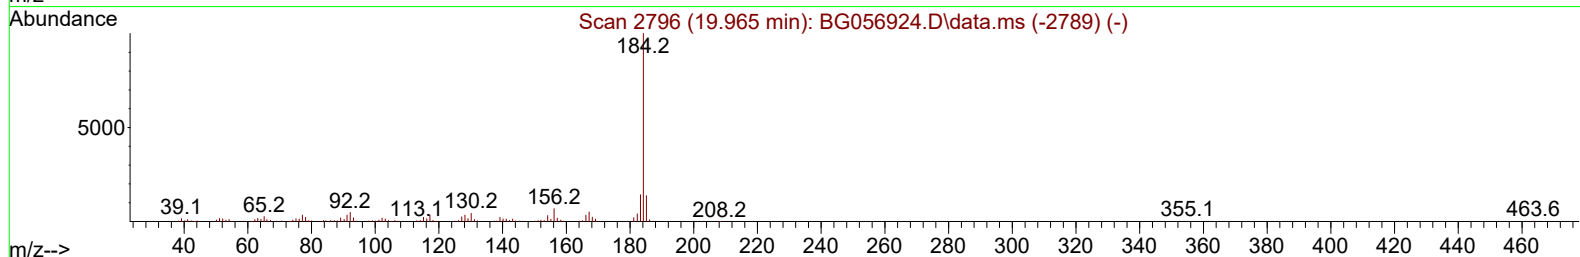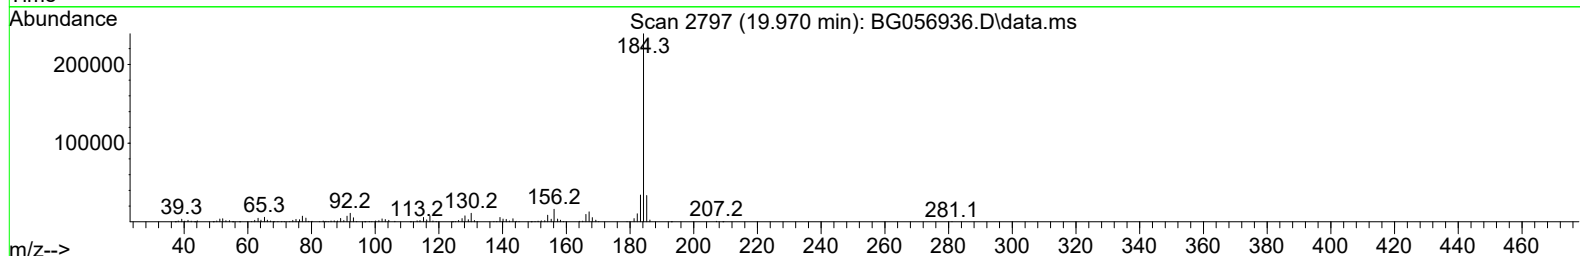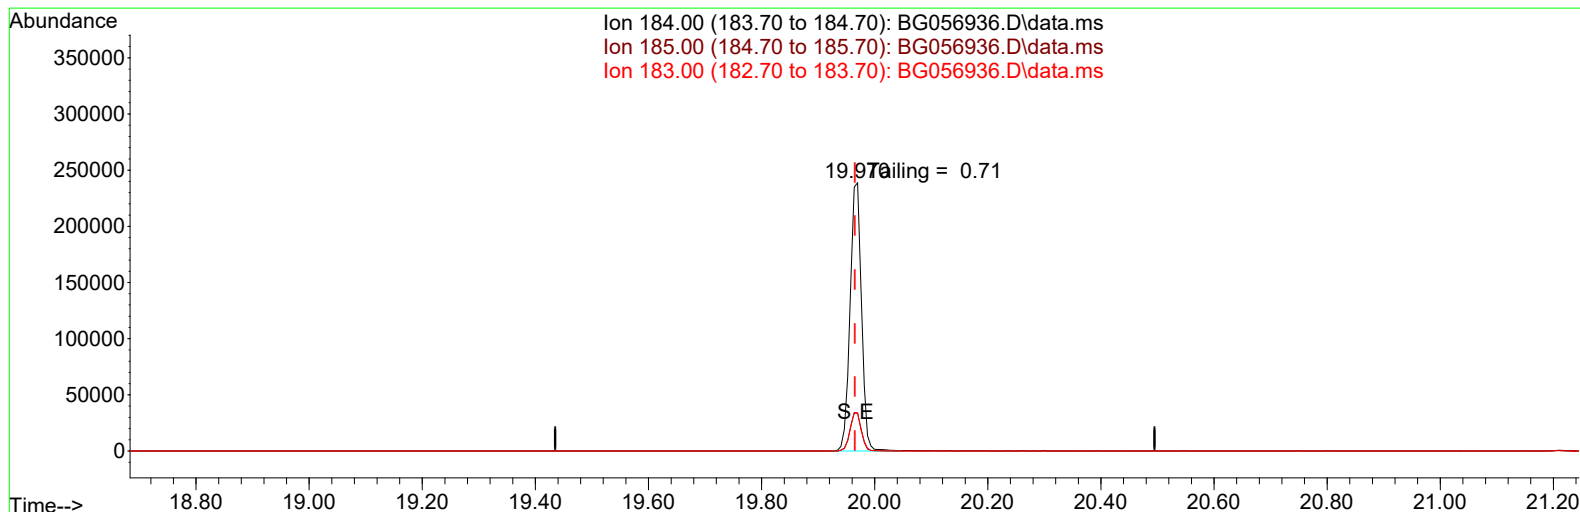

TIC: BG056936.D\data.ms

(77) Benzidine**19.970min (+ 0.005) 211089.28 ng****response 334646**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.04
183.00	14.20	14.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2023	BNA_G	<u>BG056936.D</u>
Compound Name	Response	Retention Time
DDT	170248	21.209
DDD	4962	20.745
DDE	383	20.24
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5345	175593	3.04

Instrument :
BNA_G
ClientSampleId :
DFTPP