

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040119\
 Data File : BG040291.D
 Acq On : 2 Apr 2019 9:06
 Operator : JU/SJ
 Sample : K1689-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-032919-A

Quant Time: Apr 02 11:13:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 28 05:47:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	59177	20.00	ng	-0.02
21) Naphthalene-d8	10.87	136	252596	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	173396	20.00	ng	-0.02
64) Phenanthrene-d10	17.43	188	440499	20.00	ng	-0.02
76) Chrysene-d12	21.71	240	437584	20.00	ng	-0.02
87) Perylene-d12	25.01	264	437551	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	463278	130.14	ng	-0.01
7) Phenol-d6	7.21	99	594032	120.75	ng	-0.02
23) Nitrobenzene-d5	9.23	82	456677	96.10	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	306999	163.82	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	1085832	92.79	ng	-0.02
79) Terphenyl-d14	20.03	244	1806833	92.89	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG040119\
Data File : BG040291.D
Acq On : 2 Apr 2019 9:06
Operator : JU/SJ
Sample : K1689-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
NB-08-032919-A

Quant Time: Apr 02 11:13:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 28 05:47:00 2019
Response via : Initial Calibration

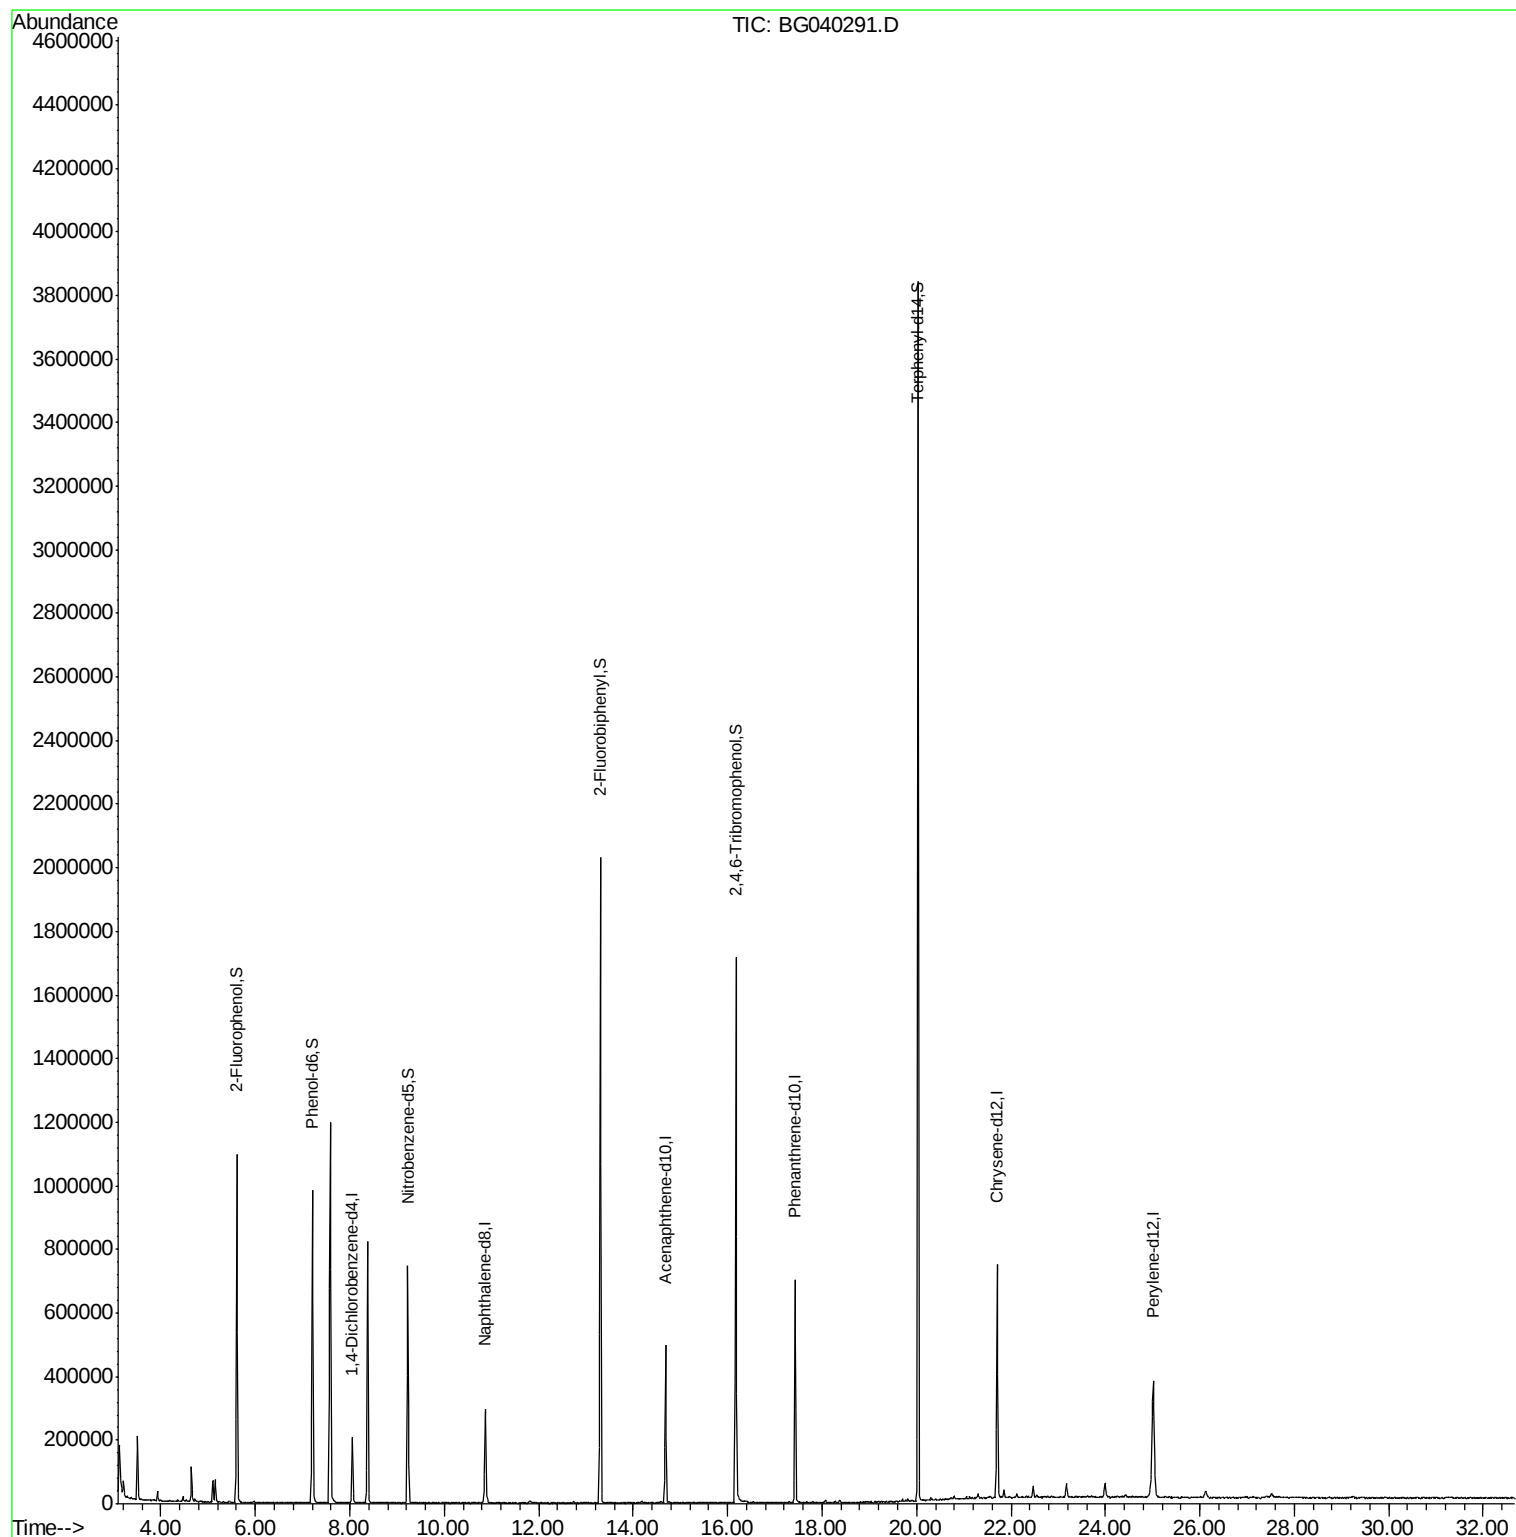




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.05 min Scan# 845
Delta R.T. -0.02 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06

Instrument :
BNA_G
ClientSampleId :
NB-08-032919-A

Tgt Ion:152 Resp: 59177
Ion Ratio Lower Upper
152 100
150 146.5 123.7 185.5
115 54.7 46.9 70.3

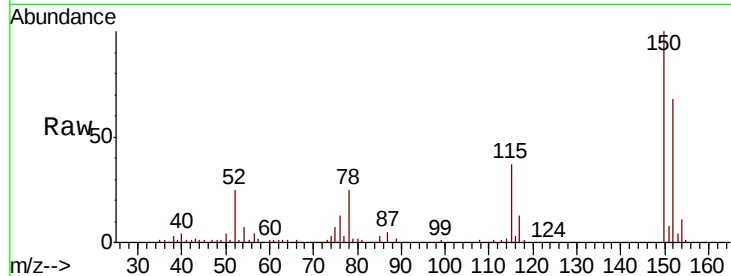


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

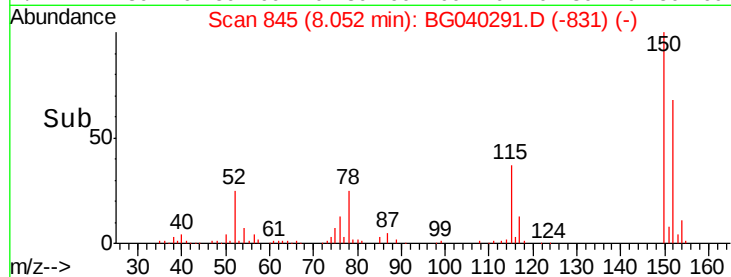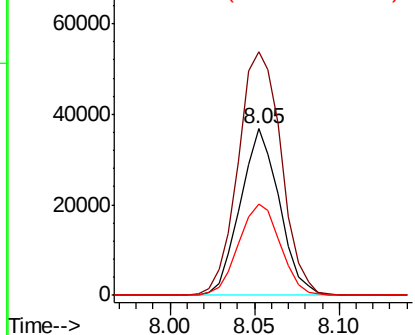



#5


2-Fluorophenol
Concen: 130.145 ng
RT: 5.61 min Scan# 429
Delta R.T. -0.01 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06

Tgt Ion:112 Resp: 463278
Ion Ratio Lower Upper
112 100
64 68.5 54.2 81.2
63 34.0 26.4 39.6

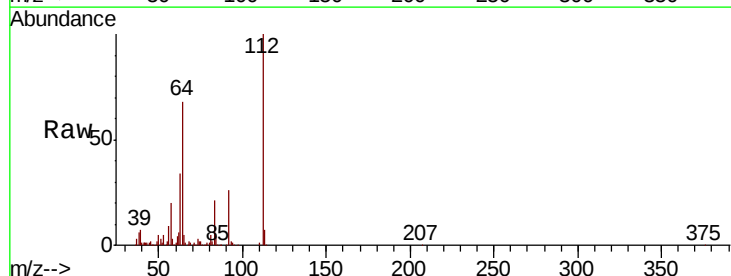

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

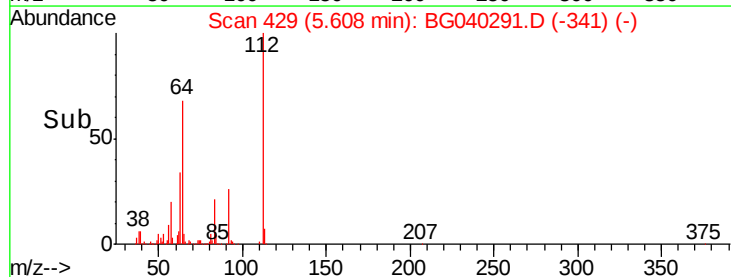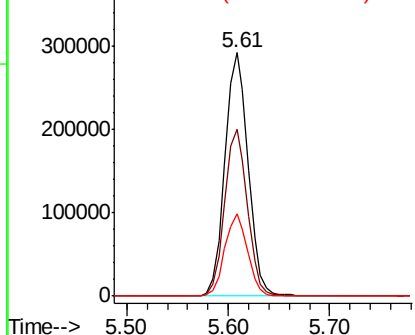

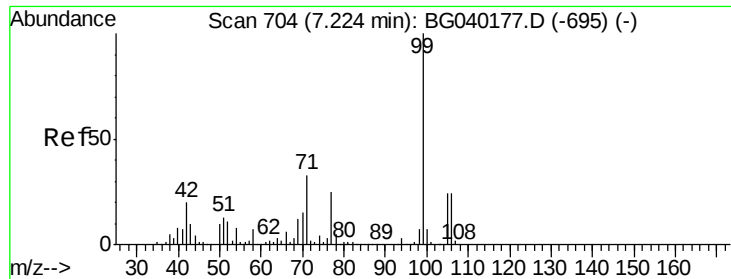

#7

Phenol-d6

Concen: 120.749 ng

RT: 7.21 min Scan# 701

Delta R.T. -0.02 min

Lab File: BG040291.D

Acq: 2 Apr 2019 9:06

Instrument :

BNA_G

ClientSampleId :

NB-08-032919-A


Tgt Ion: 99 Resp: 594032

Ion Ratio Lower Upper




99 100

42 19.0 16.2 24.2

71 33.1 26.8 40.2

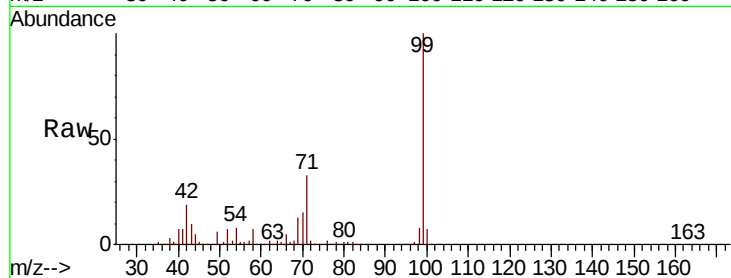

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

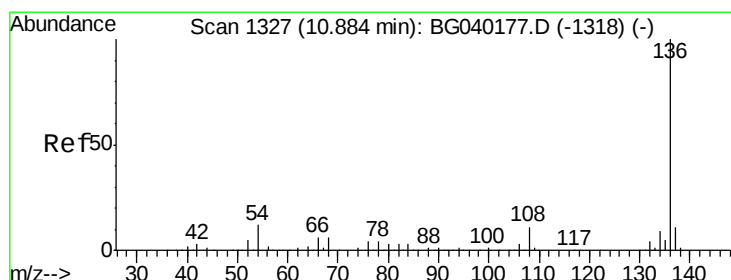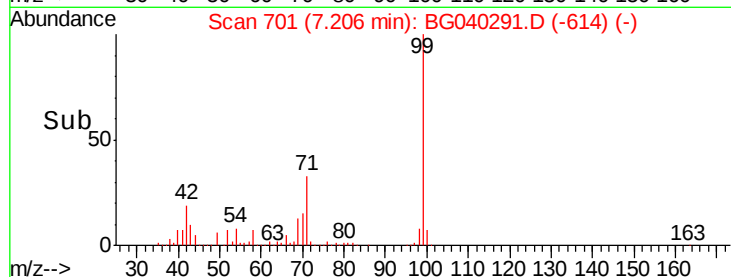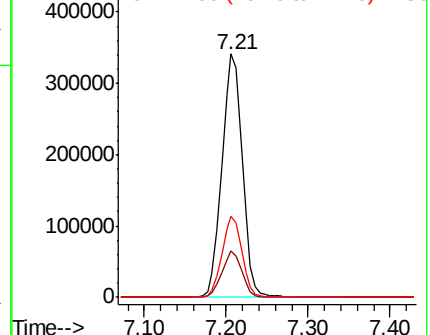

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.87 min Scan# 1324

Delta R.T. -0.02 min

Lab File: BG040291.D

Acq: 2 Apr 2019 9:06

Tgt Ion: 136 Resp: 252596


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 10.6 9.6 14.4

68 6.1 5.1 7.7

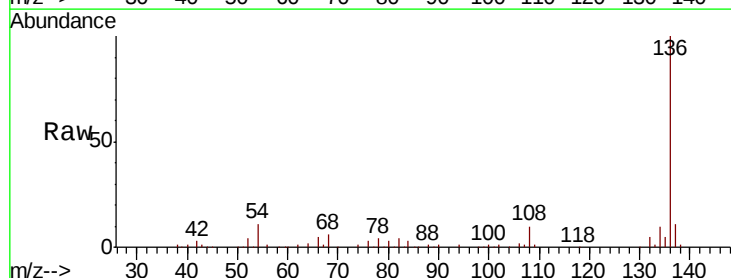

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



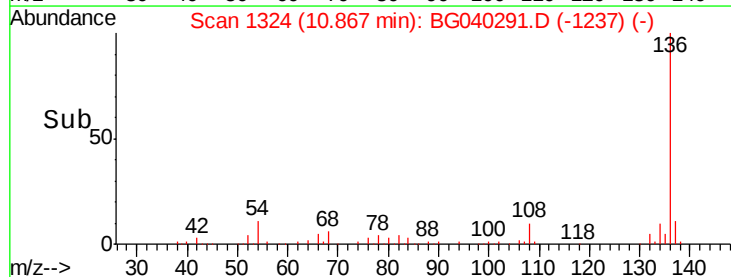
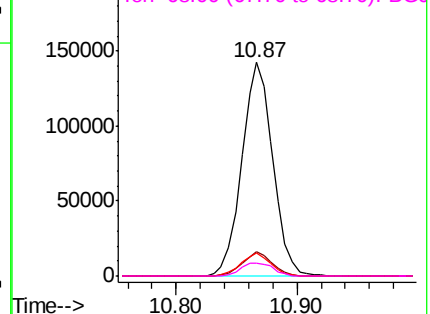


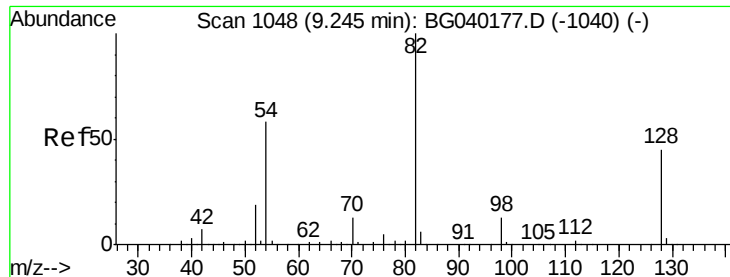

#23
Nitrobenzene-d5
Concen: 96.098 ng
RT: 9.23 min Scan# 1045
Delta R.T. -0.02 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06




Instrument :
BNA_G
ClientSampleId :
NB-08-032919-A

Tgt Ion: 82 Resp: 456677
Ion Ratio Lower Upper
82 100
128 42.6 35.8 53.8
54 54.3 46.2 69.2

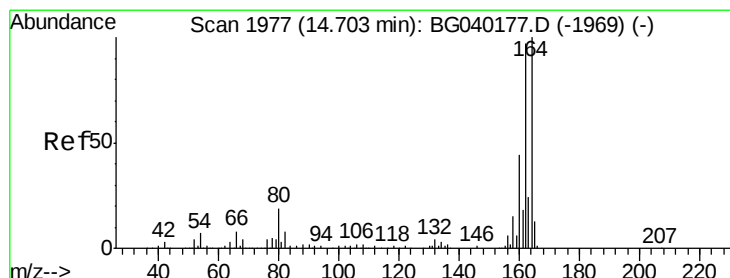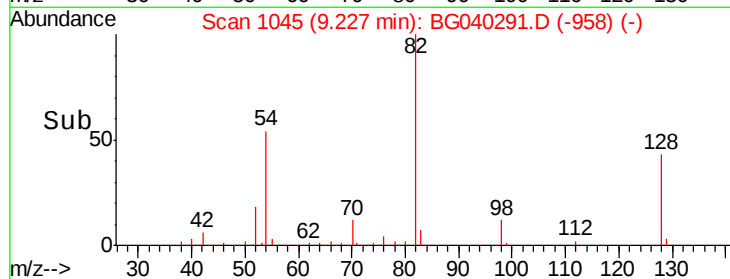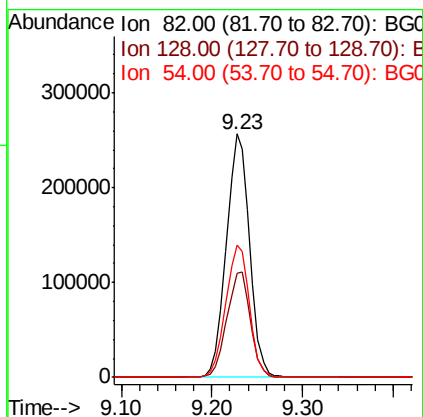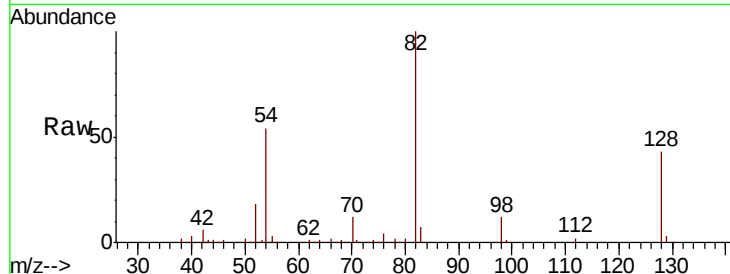

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1973
Delta R.T. -0.02 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06

Tgt Ion: 164 Resp: 173396
Ion Ratio Lower Upper
164 100
162 100.8 77.4 116.2
160 43.8 35.3 52.9

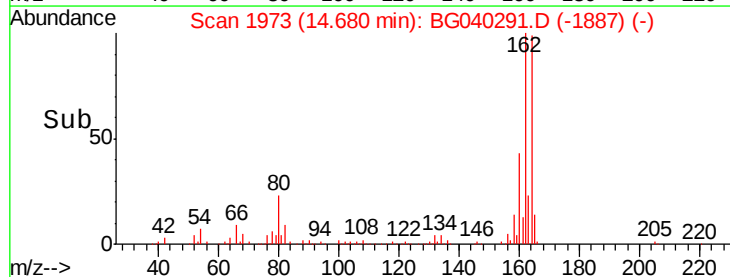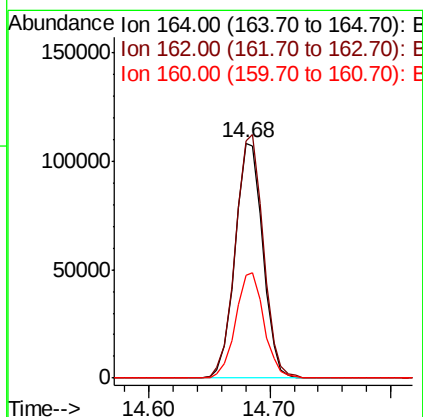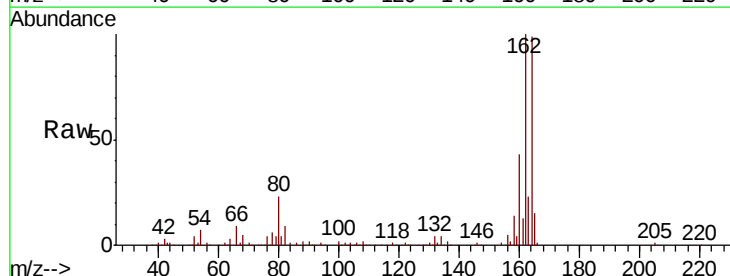






#42
 2,4,6-Tribromophenol
 Concen: 163.824 ng
 RT: 16.17 min Scan# 2227
 Delta R.T. -0.02 min
 Lab File: BG040291.D
 Acq: 2 Apr 2019 9:06

Instrument :
 BNA_G
 ClientSampleId :
 NB-08-032919-A

Tgt Ion:330 Resp: 306999
 Ion Ratio Lower Upper
 330 100
 332 97.5 76.6 115.0
 141 38.1 32.6 48.8

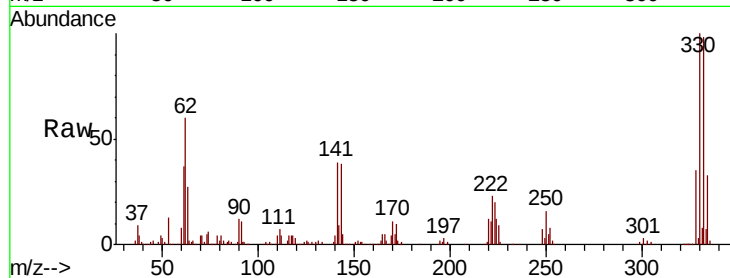


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

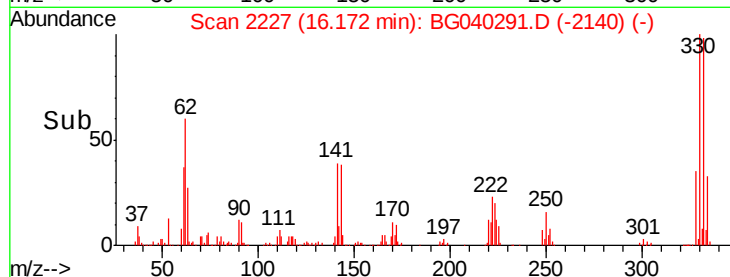
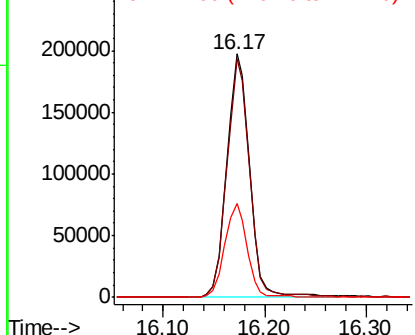



#45
 2-Fluorobiphenyl
 Concen: 92.790 ng
 RT: 13.30 min Scan# 1739
 Delta R.T. -0.02 min
 Lab File: BG040291.D
 Acq: 2 Apr 2019 9:06

Tgt Ion:172 Resp: 1085832
 Ion Ratio Lower Upper
 172 100
 171 37.3 30.5 45.7
 170 25.0 20.1 30.1

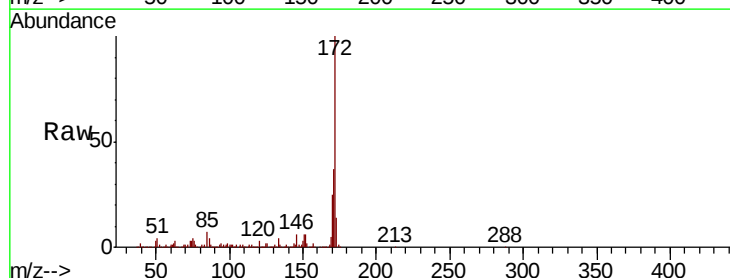

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

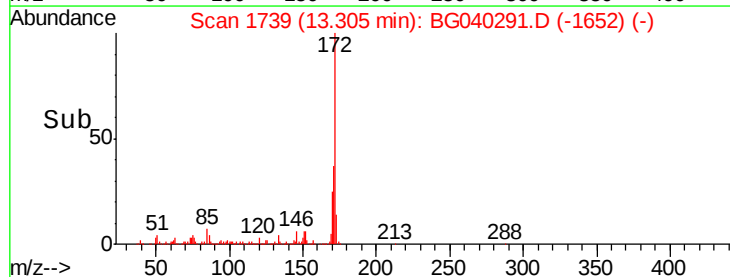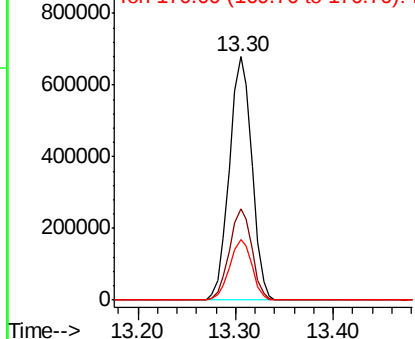


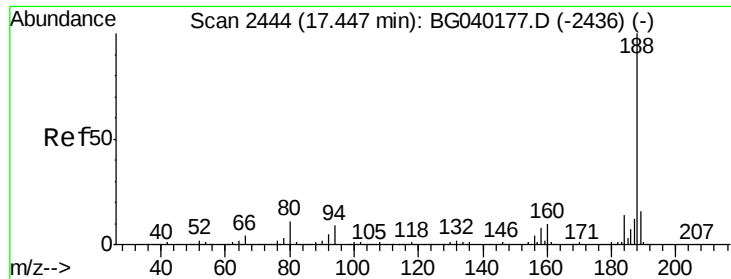




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.43 min Scan# 2441
Delta R.T. -0.02 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06

Instrument :
BNA_G
ClientSampleId :
NB-08-032919-A

Tgt Ion:188 Resp: 440499
Ion Ratio Lower Upper
188 100
94 9.1 7.0 10.4
80 9.9 8.6 13.0

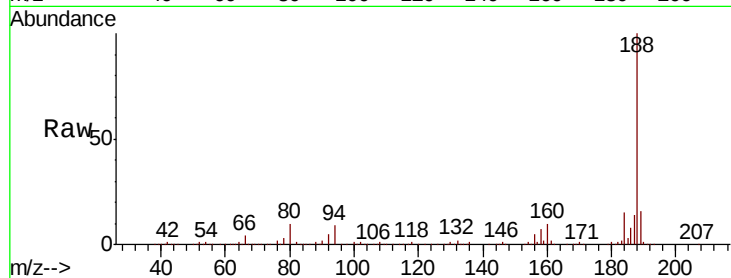


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

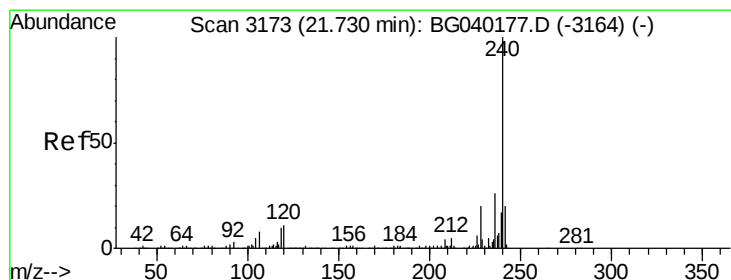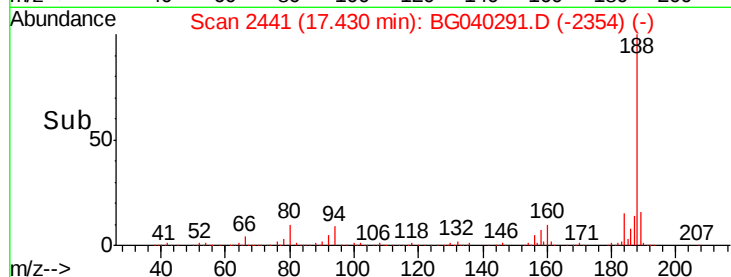
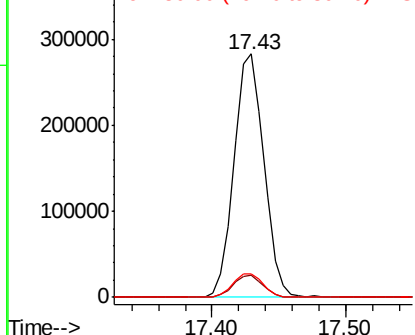


#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.71 min Scan# 3169
Delta R.T. -0.02 min
Lab File: BG040291.D
Acq: 2 Apr 2019 9:06

Tgt Ion:240 Resp: 437584
Ion Ratio Lower Upper
240 100
120 10.3 8.4 12.6
236 25.6 20.8 31.2

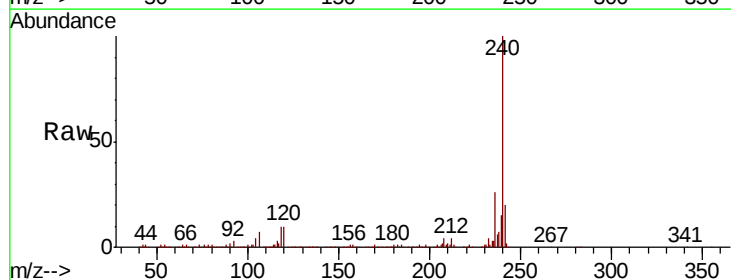

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

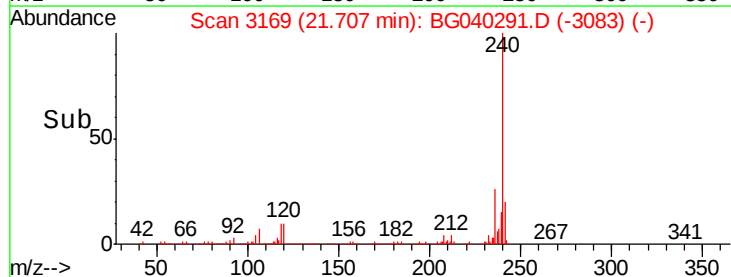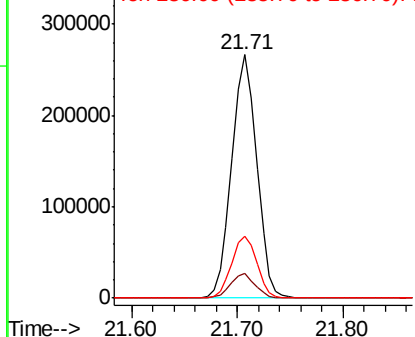



#79

Terphenyl-d14

Concen: 92.891 ng

RT: 20.03 min Scan# 2884

Delta R.T. -0.02 min

Lab File: BG040291.D

Acq: 2 Apr 2019 9:06

Instrument :

BNA_G

ClientSampleId :

NB-08-032919-A


Tgt Ion:244 Resp: 1806833

Ion Ratio Lower Upper




244 100

212 9.4 7.0 10.6

122 11.9 8.5 12.7

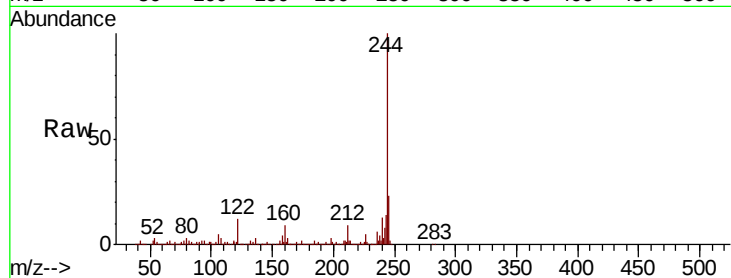

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

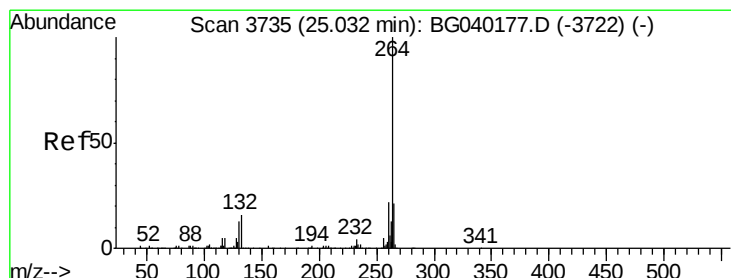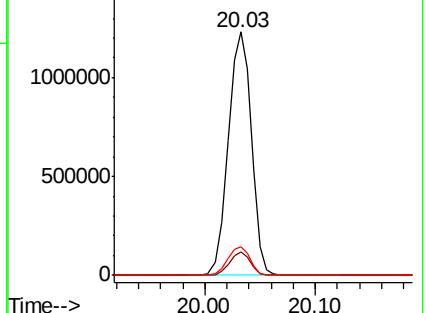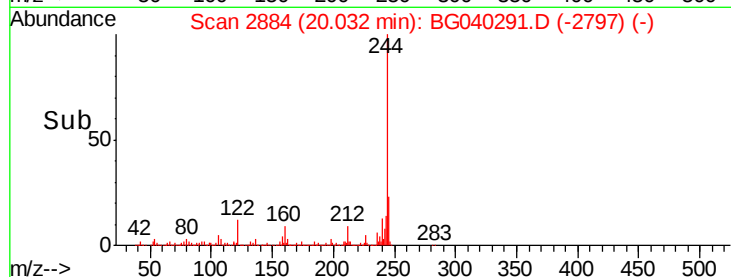

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.01 min Scan# 3732

Delta R.T. -0.02 min

Lab File: BG040291.D

Acq: 2 Apr 2019 9:06


Tgt Ion:264 Resp: 437551

Ion Ratio Lower Upper

264 100

260 22.5 17.9 26.9

265 21.4 16.8 25.2

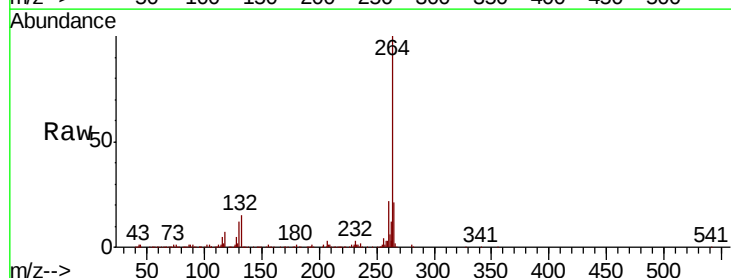

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

