


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG040119\
 Data File : BG040282.D
 Acq On : 2 Apr 2019 2:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG032719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 28 05:47:00 2019

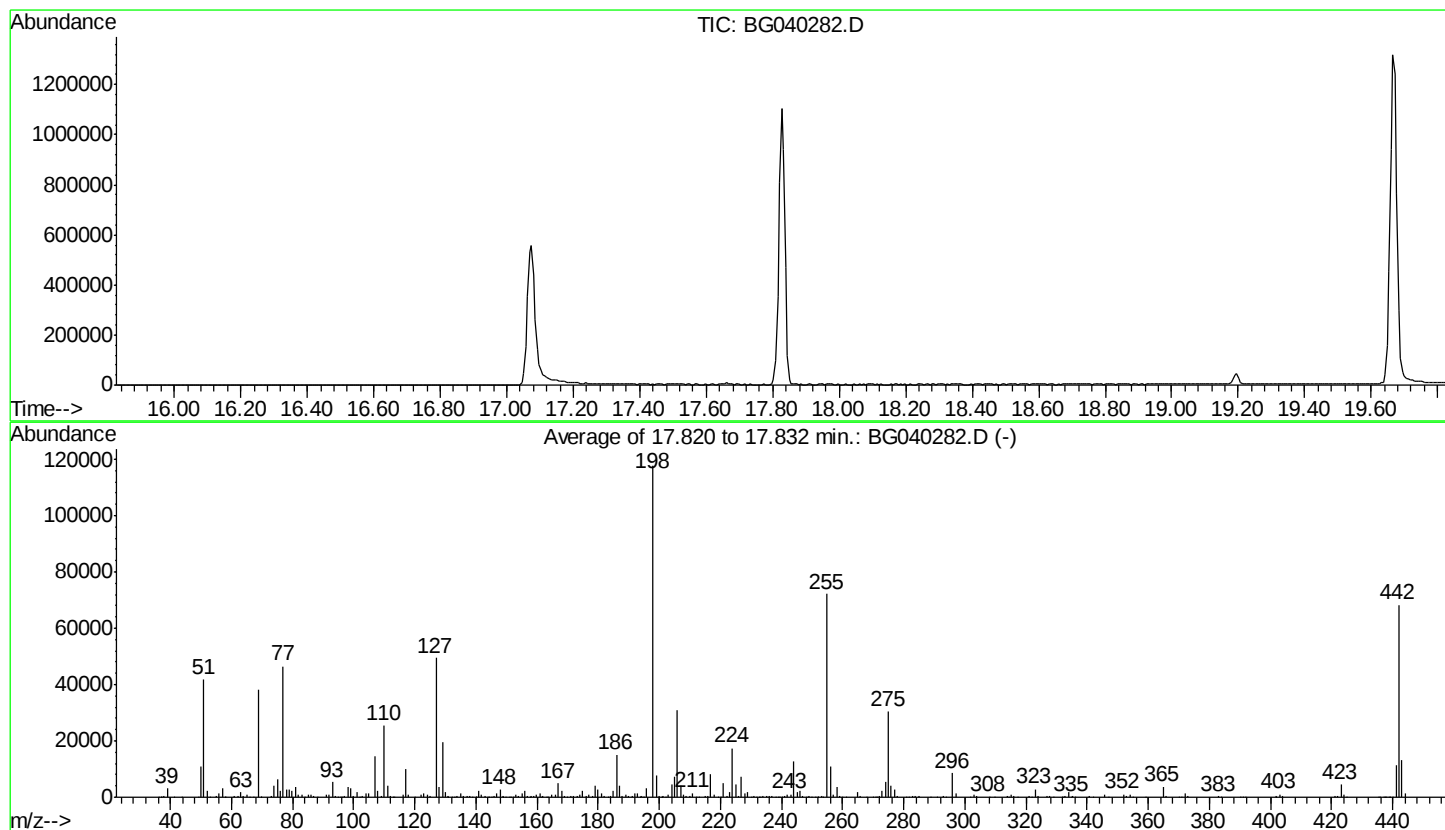

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	41642	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.5	38261	PASS
70	69	0.00	2	0.4	158	PASS
127	198	10	80	42.0	49429	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117730	PASS
199	198	5	9	6.5	7647	PASS
275	198	10	60	25.7	30245	PASS
365	198	1	100	3.2	3775	PASS
441	198	0.01	100	9.5	11232	PASS
442	198	50	100	57.9	68186	PASS
443	442	15	24	19.2	13114	PASS